

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071119\
Data File : VU033202.D
Acq On : 11 Jul 2019 20:58
Operator : JC/SP
Sample : VU0711WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0711WBL01

Quant Time: Jul 12 05:49:31 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U071119DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Jul 12 05:19:33 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene	5.72	96	30681	1.00	ug/l	0.00

System Monitoring Compounds

57) 4-Bromofluorobenzene	10.30	95	9821	0.85	ug/l	0.00
Spiked Amount	1.000		Recovery	=	85.00%	
68) 1,2-Dichlorobenzene-d4	11.85	152	11094	0.88	ug/l	0.00
Spiked Amount	1.000		Recovery	=	88.00%	


Target Compounds	Ovalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071119\
Data File : VU033202.D
Acq On : 11 Jul 2019 20:58
Operator : JC/SP
Sample : VU0711WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0711WBL01

Quant Time: Jul 12 05:49:31 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U071119DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Jul 12 05:19:33 2019
Response via : Initial Calibration

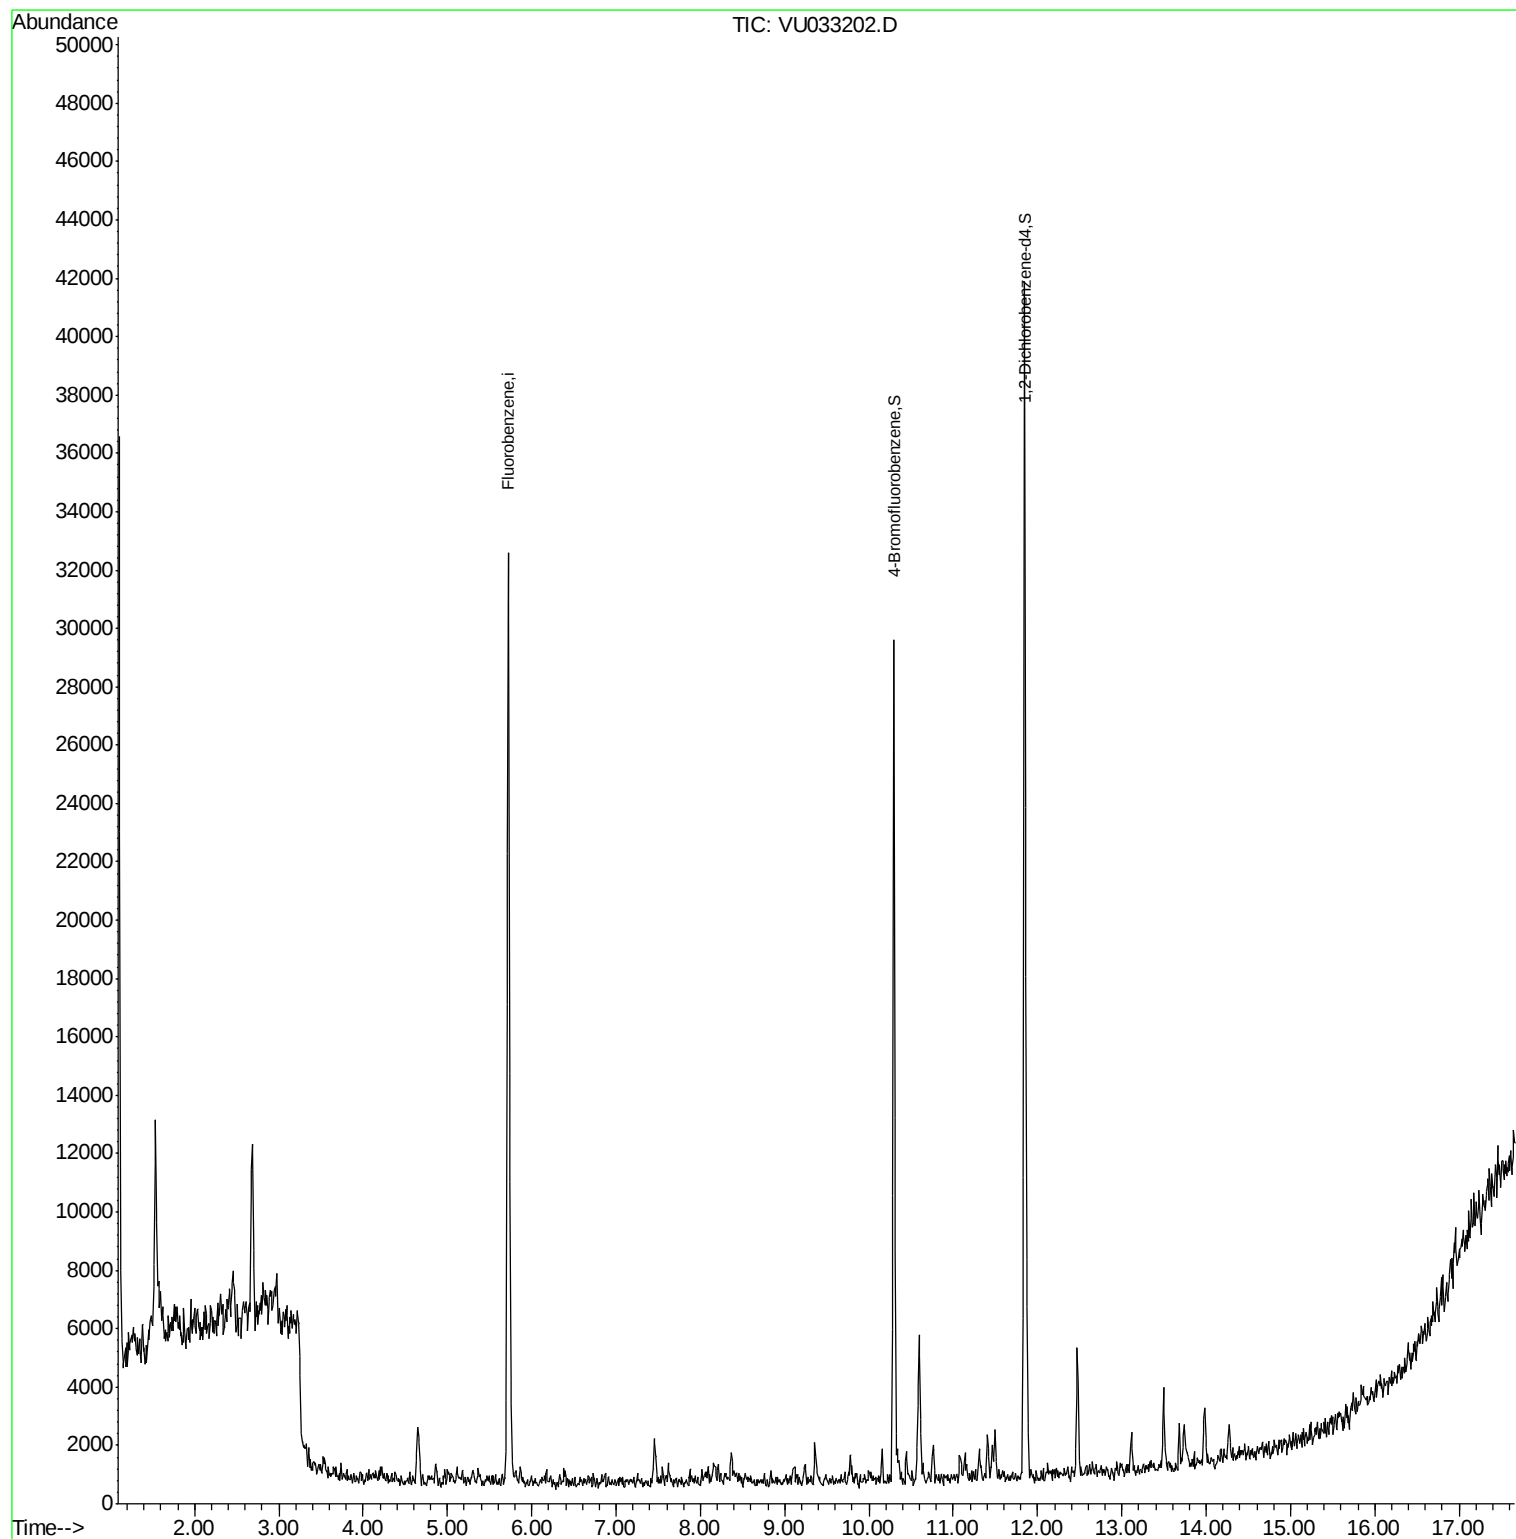

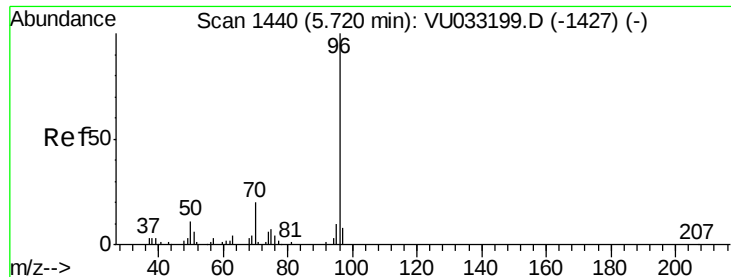

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 5.72 min Scan# 1441

Delta R.T. 0.00 min

Lab File: VU033202.D

Acq: 11 Jul 2019 20:58

Instrument :

MSVOA_U

ClientSampleId :

VU0711WBL01

Tot Ion: 96 Resp: 30681


Ion Ratio Lower Upper

96 100

70 20.0 16.2 24.4

95 9.0 7.8 11.8

97 5.9 0.0 0.0#



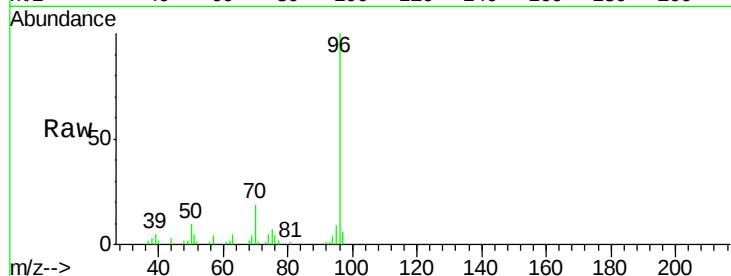


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

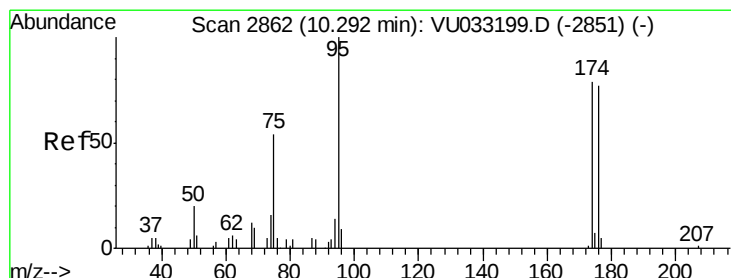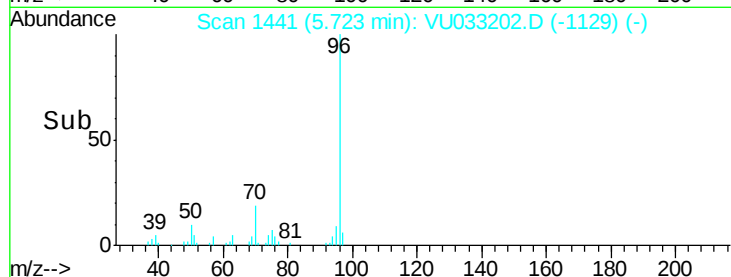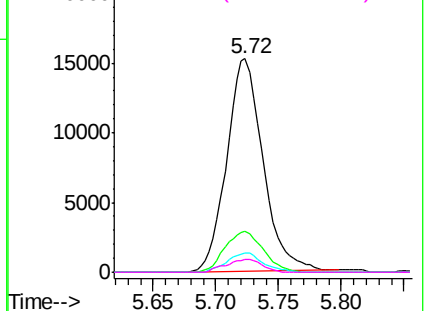

#57

4-Bromofluorobenzene

Concen: 0.847 ug/l

RT: 10.30 min Scan# 2863

Delta R.T. 0.00 min

Lab File: VU033202.D

Acq: 11 Jul 2019 20:58


Tgt Ion: 95 Resp: 9821

Ion Ratio Lower Upper

95 100

174 83.2 63.8 95.8



176 82.8 64.5 96.7

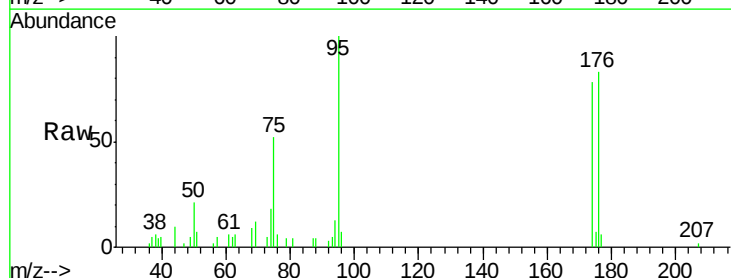


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

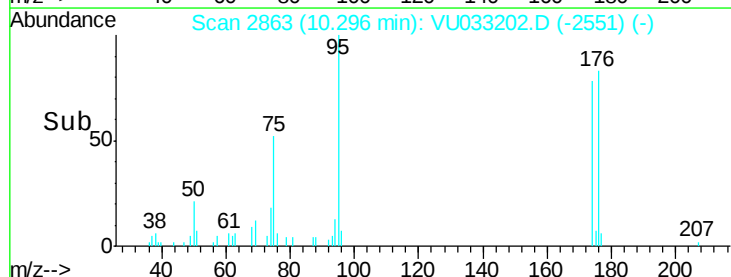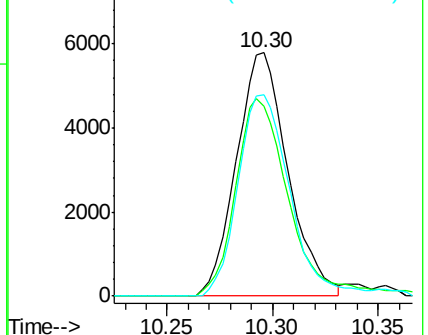


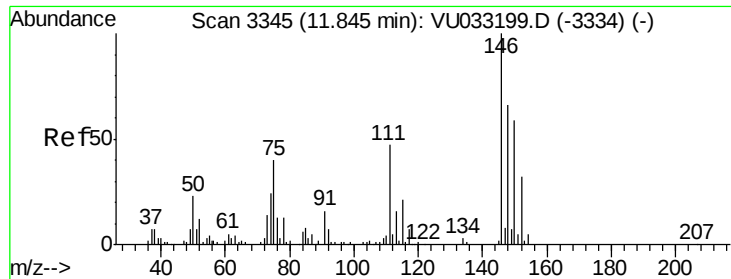

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.884 ug/l
 RT: 11.85 min Scan# 3345
 Delta R.T. 0.00 min
 Lab File: VU033202.D
 Acq: 11 Jul 2019 20:58

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0711WBL01

Tot Ion	Ratio	Lower	Upper
152	100		
115	65.8	0.0	131.0
150	154.2	0.0	634.4

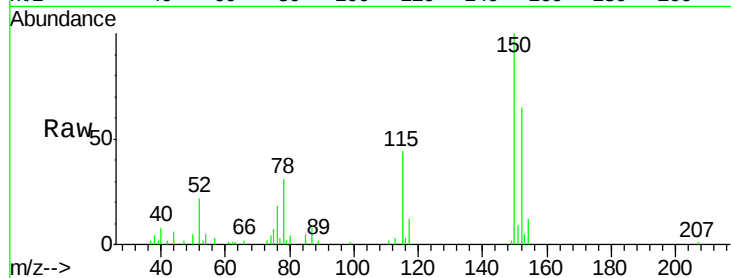

Abundance Ion 152.00 (151.70 to 152.70): V
 Ion 115.00 (114.70 to 115.70): V
 Ion 150.00 (149.70 to 150.70): V

