


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU071119\
Data File : VU033194.D
Acq On : 11 Jul 2019 15:27
Operator : JC/SP
Sample : BFB
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U071119DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Fri Jul 12 05:19:33 2019

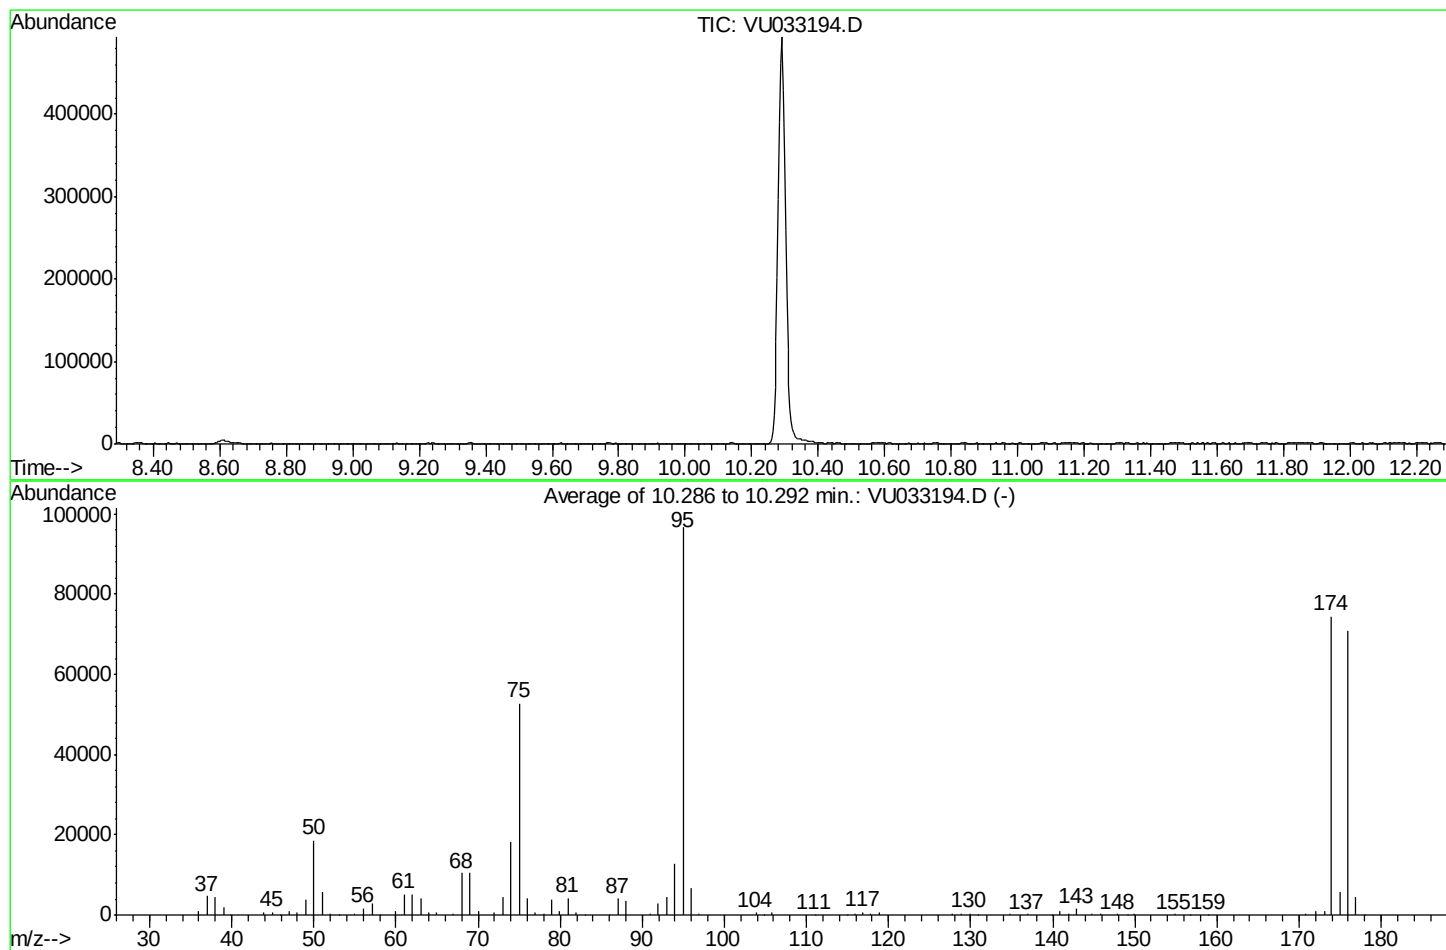

AutoFind: Scans 2860, 2861, 2862; Background Corrected with Scan 2847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	18664	PASS
75	95	30	60	54.5	52696	PASS
95	95	100	100	100.0	96701	PASS
96	95	5	9	6.9	6686	PASS
173	174	0.00	2	1.2	912	PASS
174	95	50	100	77.1	74565	PASS
175	174	5	9	7.7	5747	PASS
176	174	95	101	95.1	70930	PASS
177	176	5	9	6.4	4536	PASS