

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071122\
 Data File : VU049673.D
 Acq On : 11 Jul 2022 14:11
 Operator : SY/MD
 Sample : VU0711WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK149

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049673.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	10	rVB3	2268	1840	0.19%	0.025%
2	1.597	73	80	98	rVB	124947	142999	14.83%	1.968%
3	1.909	169	177	195	rVB	95478	124840	12.94%	1.718%
4	2.565	369	381	397	rBV	191934	308460	31.98%	4.245%
5	2.790	445	451	458	rVV3	1168	1759	0.18%	0.024%
6	2.854	469	471	478	rVB2	189	171	0.02%	0.002%
7	2.935	492	496	498	rBV	205	172	0.02%	0.002%
8	2.993	510	514	517	rBV2	229	176	0.02%	0.002%
9	3.044	520	530	543	rVB4	2424	4308	0.45%	0.059%
10	3.137	557	559	564	rVB	249	151	0.02%	0.002%
11	3.186	565	574	587	rVB4	1127	2342	0.24%	0.032%
12	3.427	646	649	653	rVB	223	163	0.02%	0.002%
13	3.453	653	657	660	rBV2	205	184	0.02%	0.003%
14	3.671	722	725	733	rVB2	252	297	0.03%	0.004%
15	3.787	758	761	767	rBV2	276	274	0.03%	0.004%
16	3.832	772	775	781	rVB2	221	209	0.02%	0.003%
17	4.247	898	904	907	rBV2	282	278	0.03%	0.004%
18	4.623	1008	1021	1046	rBV	108840	265907	27.57%	3.659%
19	4.961	1123	1126	1130	rBV2	208	176	0.02%	0.002%
20	5.063	1142	1158	1177	rBV	169629	374217	38.80%	5.150%
21	5.208	1201	1203	1208	rVB2	339	282	0.03%	0.004%
22	5.256	1215	1218	1220	rBV2	234	129	0.01%	0.002%
23	5.295	1220	1230	1237	rVB3	785	1242	0.13%	0.017%
24	5.330	1237	1241	1242	rBV	172	135	0.01%	0.002%
25	5.366	1250	1252	1255	rBV2	431	307	0.03%	0.004%
26	5.382	1255	1257	1260	rVB	268	158	0.02%	0.002%
27	5.449	1275	1278	1281	rBV	217	164	0.02%	0.002%
28	5.726	1339	1364	1387	rBV2	357061	964393	100.00%	13.272%
29	5.909	1417	1421	1424	rVB3	338	284	0.03%	0.004%
30	5.960	1432	1437	1441	rVB2	274	287	0.03%	0.004%
31	5.980	1441	1443	1447	rBV2	354	212	0.02%	0.003%
32	6.118	1481	1486	1489	rVB2	270	235	0.02%	0.003%
33	6.137	1489	1492	1500	rBV2	259	242	0.03%	0.003%
34	6.189	1505	1508	1511	rVB	226	129	0.01%	0.002%
35	6.250	1511	1527	1550	rBV	292312	555169	57.57%	7.640%
36	6.465	1591	1594	1598	rVB2	238	177	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071122\
 Data File : VU049673.D
 Acq On : 11 Jul 2022 14:11
 Operator : SY/MD
 Sample : VU0711WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK149

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.494	1600	1603	1606	rBV	226	173	0.02%	0.002%
38	6.523	1608	1612	1614	rBV2	1053	743	0.08%	0.010%
39	6.690	1649	1664	1687	rBV	232219	445521	46.20%	6.131%
40	6.790	1693	1695	1697	rBV2	257	135	0.01%	0.002%
41	7.005	1758	1762	1765	rBV2	264	231	0.02%	0.003%
42	7.131	1796	1801	1804	rBV2	170	185	0.02%	0.003%
43	7.182	1813	1817	1823	rBV3	440	558	0.06%	0.008%
44	7.227	1829	1831	1838	rVB2	352	420	0.04%	0.006%
45	7.285	1843	1849	1852	rVV2	268	304	0.03%	0.004%
46	7.301	1852	1854	1858	rVB	289	204	0.02%	0.003%
47	7.430	1889	1894	1899	rBV2	248	262	0.03%	0.004%
48	7.501	1912	1916	1918	rBV2	253	201	0.02%	0.003%
49	7.568	1924	1937	1958	rBV	120315	213971	22.19%	2.945%
50	7.677	1968	1971	1975	rVV2	368	295	0.03%	0.004%
51	7.780	2000	2003	2005	rVV2	500	348	0.04%	0.005%
52	7.800	2005	2009	2018	rVB4	947	1200	0.12%	0.017%
53	7.899	2026	2040	2058	rBV	427723	722703	74.94%	9.946%
54	8.089	2095	2099	2102	rVB2	286	250	0.03%	0.003%
55	8.118	2105	2108	2110	rVB2	250	163	0.02%	0.002%
56	8.134	2110	2113	2115	rBV	273	192	0.02%	0.003%
57	8.179	2116	2127	2145	rBV	80286	137148	14.22%	1.887%
58	8.398	2192	2195	2200	rVB	417	334	0.03%	0.005%
59	8.501	2225	2227	2234	rVB2	267	235	0.02%	0.003%
60	8.636	2256	2269	2301	rBV2	297410	569963	59.10%	7.844%
61	8.806	2320	2322	2326	rVB2	448	261	0.03%	0.004%
62	8.841	2326	2333	2338	rVB2	497	685	0.07%	0.009%
63	8.909	2349	2354	2357	rBV2	342	301	0.03%	0.004%
64	9.079	2404	2407	2409	rBV	200	145	0.02%	0.002%
65	9.185	2437	2440	2445	rVB2	218	204	0.02%	0.003%
66	9.417	2499	2512	2532	rBV	405859	672476	69.73%	9.255%
67	9.558	2553	2556	2558	rBV2	356	246	0.03%	0.003%
68	9.578	2558	2562	2566	rVB2	895	836	0.09%	0.012%
69	9.661	2583	2588	2592	rVB2	377	404	0.04%	0.006%
70	9.700	2592	2600	2605	rBV	818	1127	0.12%	0.016%
71	9.925	2667	2670	2671	rBV	277	163	0.02%	0.002%
72	10.009	2693	2696	2699	rBV	197	175	0.02%	0.002%
73	10.099	2720	2724	2726	rBV2	676	540	0.06%	0.007%
74	10.118	2727	2730	2737	rVB3	836	854	0.09%	0.012%
75	10.259	2768	2774	2777	rBV2	333	397	0.04%	0.005%
76	10.320	2790	2793	2797	rVB2	332	208	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071122\
 Data File : VU049673.D
 Acq On : 11 Jul 2022 14:11
 Operator : SY/MD
 Sample : VU0711WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK149

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	10.401	2815	2818	2820	rBV	227	162	0.02%	0.002%
78	10.481	2838	2843	2845	rBV	668	642	0.07%	0.009%
79	10.709	2912	2914	2916	rBV	245	153	0.02%	0.002%
80	10.758	2916	2929	2945	rVV	303682	483934	50.18%	6.660%
81	11.095	3028	3034	3036	rBV2	563	504	0.05%	0.007%
82	11.163	3052	3055	3057	rBV	313	220	0.02%	0.003%
83	11.446	3140	3143	3145	rBV2	218	154	0.02%	0.002%
84	11.475	3148	3152	3154	rVV2	412	335	0.03%	0.005%
85	11.552	3173	3176	3177	rBV	228	137	0.01%	0.002%
86	11.748	3232	3237	3244	rVB3	1387	1978	0.21%	0.027%
87	11.812	3245	3257	3275	rBV	386187	608729	63.12%	8.377%
88	11.960	3300	3303	3309	rVB2	301	259	0.03%	0.004%
89	12.195	3362	3376	3394	rBV	369391	610920	63.35%	8.407%
90	12.343	3418	3422	3425	rBV	293	298	0.03%	0.004%
91	12.578	3492	3495	3499	rVB2	403	264	0.03%	0.004%
92	13.079	3649	3651	3654	rBV3	248	132	0.01%	0.002%
93	13.156	3671	3675	3678	rBV2	449	357	0.04%	0.005%
94	13.224	3688	3696	3706	rBV4	1926	2857	0.30%	0.039%
95	13.291	3714	3717	3719	rBV	313	252	0.03%	0.003%
96	13.352	3733	3736	3739	rBV	330	284	0.03%	0.004%
97	13.844	3882	3889	3900	rVB4	3594	5196	0.54%	0.072%
98	14.092	3955	3966	3976	rBV3	8370	14654	1.52%	0.202%
99	14.205	3999	4001	4003	rBV2	335	193	0.02%	0.003%
100	14.336	4034	4042	4054	rVB3	4624	6579	0.68%	0.091%




Sum of corrected areas: 7266422

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071122\
Data File : VU049673.D
Acq On : 11 Jul 2022 14:11
Operator : SY/MD
Sample : VU0711WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK149

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

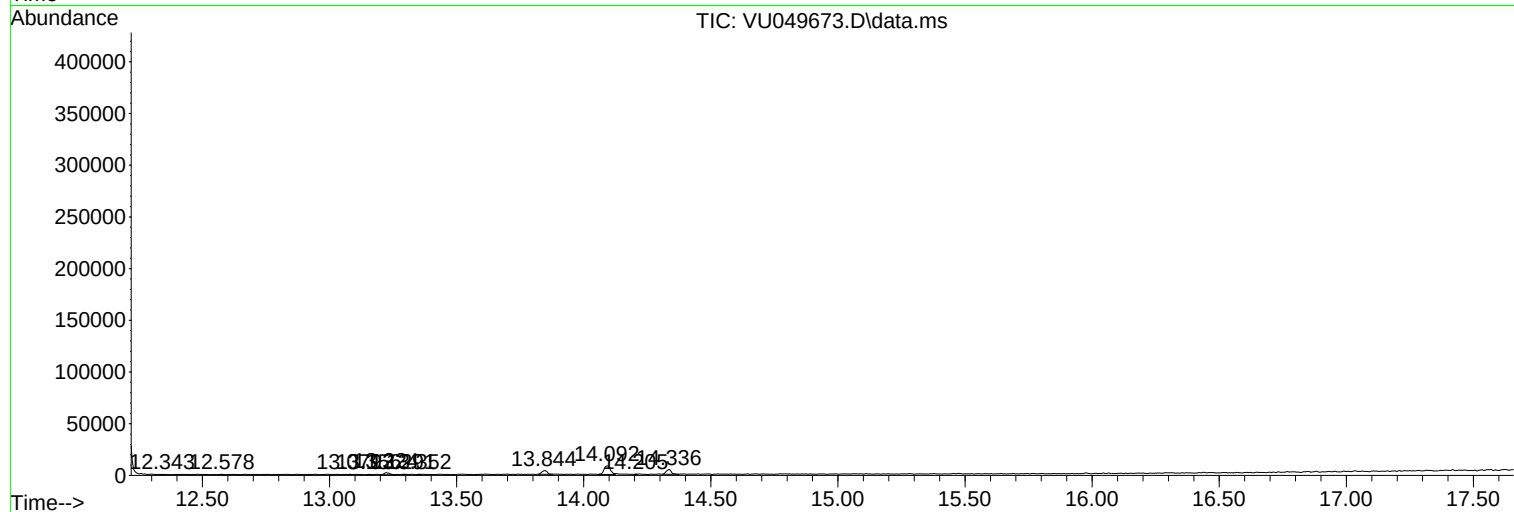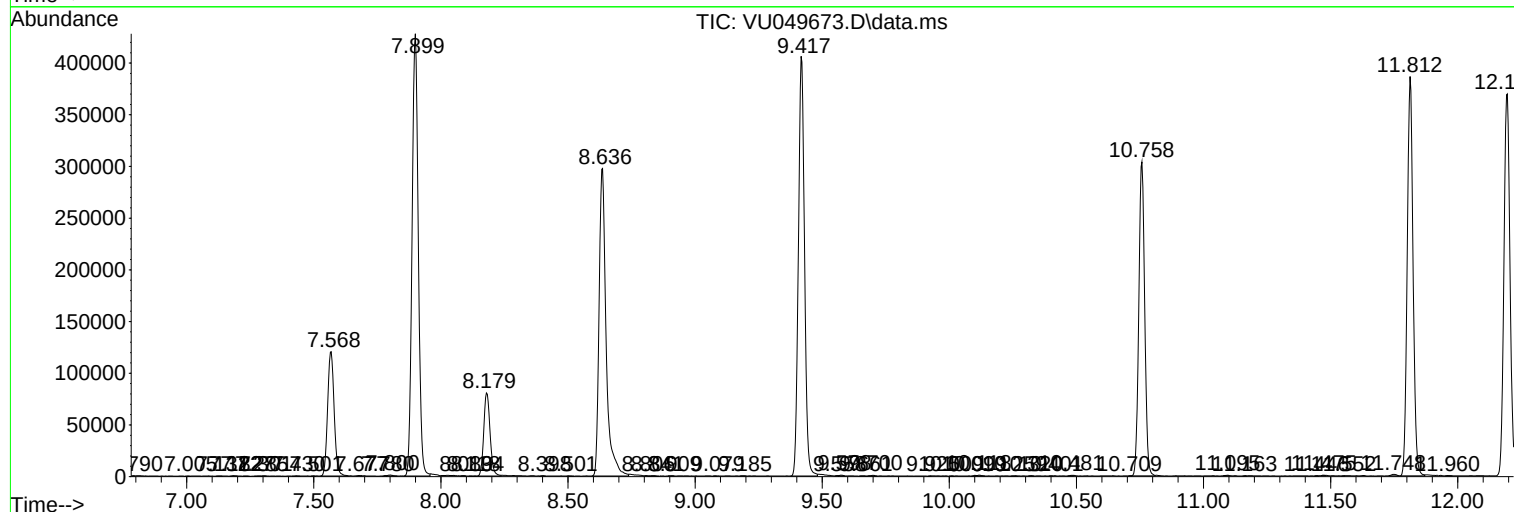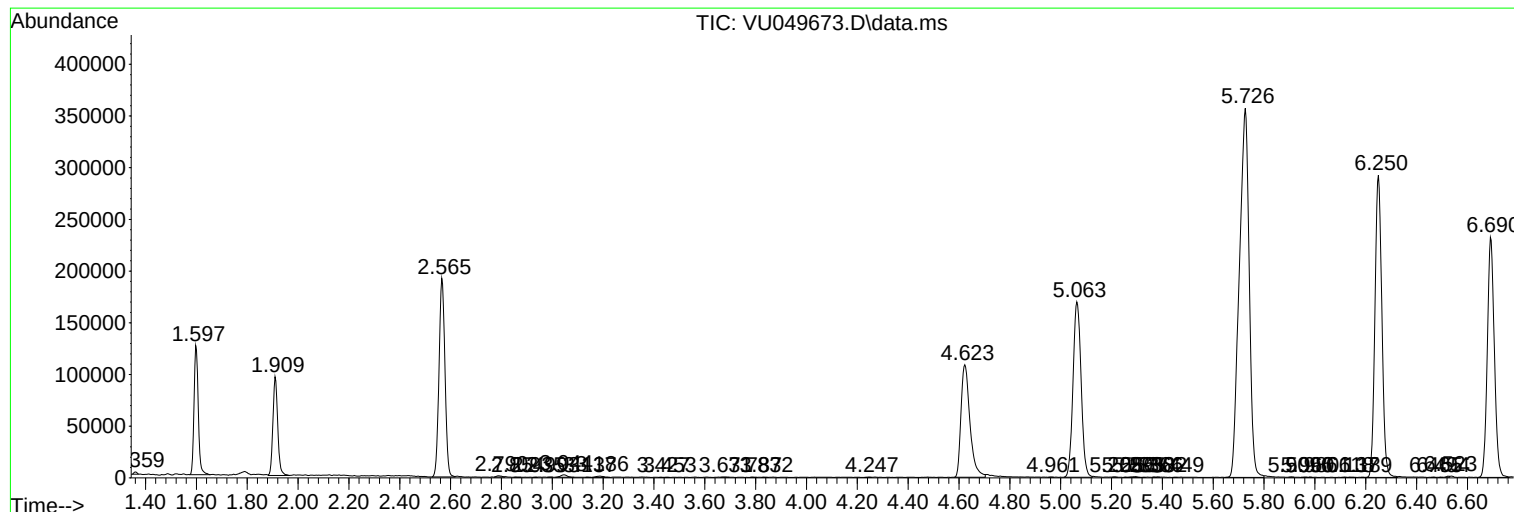

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071122\
Data File : VU049673.D
Acq On : 11 Jul 2022 14:11
Operator : SY/MD
Sample : VU0711WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK149

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071122\
Data File : VU049673.D
Acq On : 11 Jul 2022 14:11
Operator : SY/MD
Sample : VU0711WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK149

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------