

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071122\
 Data File : VU049683.D
 Acq On : 11 Jul 2022 18:07
 Operator : SY/MD
 Sample : N3639-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049683.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	98	rVB	113687	129498	13.65%	1.831%
2	1.809	127	146	152	rBV8	9240	19697	2.08%	0.278%
3	1.900	165	174	186	rBV	83497	110968	11.69%	1.569%
4	2.263	285	287	291	rBV4	609	395	0.04%	0.006%
5	2.562	367	380	405	rVB	172043	275782	29.06%	3.899%
6	2.674	413	415	421	rVB2	395	347	0.04%	0.005%
7	2.716	424	428	431	rBV2	374	269	0.03%	0.004%
8	2.826	457	462	468	rBV2	299	432	0.05%	0.006%
9	2.925	490	493	498	rBV2	233	185	0.02%	0.003%
10	2.964	498	505	507	rBV3	356	484	0.05%	0.007%
11	3.041	520	529	541	rVB4	2853	4782	0.50%	0.068%
12	3.176	565	571	572	rBV2	790	794	0.08%	0.011%
13	3.240	588	591	595	rVB2	295	214	0.02%	0.003%
14	3.526	674	680	684	rBV2	232	266	0.03%	0.004%
15	3.674	720	726	729	rVB2	241	202	0.02%	0.003%
16	3.716	734	739	742	rBV2	306	267	0.03%	0.004%
17	4.144	869	872	876	rBV	298	326	0.03%	0.005%
18	4.192	884	887	890	rBV	363	342	0.04%	0.005%
19	4.227	893	898	901	rVV	259	252	0.03%	0.004%
20	4.308	919	923	929	rBV2	273	299	0.03%	0.004%
21	4.620	1007	1020	1056	rBV	115407	279456	29.45%	3.951%
22	4.809	1076	1079	1083	rVB3	233	181	0.02%	0.003%
23	4.832	1083	1086	1091	rBV3	230	234	0.02%	0.003%
24	4.893	1103	1105	1109	rVB2	277	180	0.02%	0.003%
25	5.063	1141	1158	1180	rBV	170646	371864	39.19%	5.258%
26	5.202	1196	1201	1204	rVB2	269	263	0.03%	0.004%
27	5.224	1204	1208	1213	rBV3	368	365	0.04%	0.005%
28	5.285	1222	1227	1240	rVB3	596	1131	0.12%	0.016%
29	5.366	1249	1252	1261	rVB3	381	482	0.05%	0.007%
30	5.639	1334	1337	1342	rBV2	259	213	0.02%	0.003%
31	5.723	1342	1363	1386	rBV2	352084	948939	100.00%	13.417%
32	5.954	1429	1435	1438	rBV2	274	261	0.03%	0.004%
33	5.973	1438	1441	1445	rVV3	402	369	0.04%	0.005%
34	5.999	1447	1449	1453	rVV2	309	192	0.02%	0.003%
35	6.044	1458	1463	1468	rVB4	237	237	0.02%	0.003%
36	6.086	1473	1476	1479	rBV2	239	184	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071122\
 Data File : VU049683.D
 Acq On : 11 Jul 2022 18:07
 Operator : SY/MD
 Sample : N3639-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.173	1499	1503	1506	rBV2	236	166	0.02%	0.002%
38	6.247	1512	1526	1547	rBV	285270	544750	57.41%	7.702%
39	6.378	1563	1567	1574	rBV2	389	489	0.05%	0.007%
40	6.488	1598	1601	1605	rVB	494	336	0.04%	0.005%
41	6.526	1605	1613	1625	rBV5	1598	2839	0.30%	0.040%
42	6.604	1634	1637	1642	rVB3	382	302	0.03%	0.004%
43	6.690	1649	1664	1682	rBV	228900	441966	46.57%	6.249%
44	6.803	1697	1699	1703	rBV3	360	237	0.02%	0.003%
45	6.822	1703	1705	1708	rVB	356	192	0.02%	0.003%
46	7.009	1761	1763	1769	rVB	258	231	0.02%	0.003%
47	7.041	1769	1773	1779	rBV2	266	270	0.03%	0.004%
48	7.176	1813	1815	1816	rBV2	638	334	0.04%	0.005%
49	7.253	1836	1839	1847	rVV2	156	192	0.02%	0.003%
50	7.346	1864	1868	1872	rVB2	214	173	0.02%	0.002%
51	7.388	1878	1881	1887	rVB2	249	216	0.02%	0.003%
52	7.481	1907	1910	1914	rVB2	256	180	0.02%	0.003%
53	7.565	1922	1936	1957	rBV	116380	201790	21.26%	2.853%
54	7.674	1966	1970	1971	rBV	361	222	0.02%	0.003%
55	7.771	1996	2000	2002	rBV	228	205	0.02%	0.003%
56	7.896	2026	2039	2060	rBV	400026	685798	72.27%	9.696%
57	8.179	2115	2127	2141	rBV	79947	131575	13.87%	1.860%
58	8.333	2172	2175	2179	rBV	310	226	0.02%	0.003%
59	8.394	2191	2194	2197	rBV2	201	179	0.02%	0.003%
60	8.430	2200	2205	2210	rVB2	240	272	0.03%	0.004%
61	8.632	2256	2268	2304	rBV2	317883	595238	62.73%	8.416%
62	8.800	2318	2320	2326	rVB4	661	513	0.05%	0.007%
63	8.886	2343	2347	2350	rBV2	258	213	0.02%	0.003%
64	8.931	2358	2361	2365	rBV	313	194	0.02%	0.003%
65	8.996	2377	2381	2387	rVB	234	270	0.03%	0.004%
66	9.362	2490	2495	2497	rBV	270	246	0.03%	0.003%
67	9.417	2499	2512	2534	rBV	404996	664563	70.03%	9.396%
68	9.568	2553	2559	2563	rBV2	306	350	0.04%	0.005%
69	9.642	2577	2582	2585	rBV2	235	227	0.02%	0.003%
70	9.697	2592	2599	2602	rBV2	330	427	0.04%	0.006%
71	9.918	2665	2668	2676	rVB	298	310	0.03%	0.004%
72	9.960	2676	2681	2686	rBV2	159	206	0.02%	0.003%
73	10.050	2704	2709	2712	rBV2	265	245	0.03%	0.003%
74	10.111	2724	2728	2732	rBV2	261	285	0.03%	0.004%
75	10.275	2776	2779	2783	rVB2	339	239	0.03%	0.003%
76	10.488	2842	2845	2849	rVB2	260	183	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071122\
 Data File : VU049683.D
 Acq On : 11 Jul 2022 18:07
 Operator : SY/MD
 Sample : N3639-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	10.517	2850	2854	2856	rBV2	266	207	0.02%	0.003%
78	10.754	2915	2928	2951	rBV	310489	489812	51.62%	6.925%
79	11.082	3027	3030	3033	rVV3	392	270	0.03%	0.004%
80	11.269	3084	3088	3091	rBV	210	213	0.02%	0.003%
81	11.668	3208	3212	3218	rBV	294	345	0.04%	0.005%
82	11.738	3230	3234	3237	rBV	274	257	0.03%	0.004%
83	11.812	3244	3257	3283	rBV	361908	574420	60.53%	8.122%
84	11.918	3287	3290	3297	rBV2	307	400	0.04%	0.006%
85	11.999	3313	3315	3321	rVB2	353	304	0.03%	0.004%
86	12.137	3356	3358	3363	rVB	399	275	0.03%	0.004%
87	12.192	3363	3375	3398	rBV	357220	575741	60.67%	8.140%
88	12.324	3412	3416	3419	rBV2	264	205	0.02%	0.003%
89	12.372	3425	3431	3434	rBV2	324	383	0.04%	0.005%
90	12.468	3458	3461	3467	rVB	345	350	0.04%	0.005%
91	12.500	3469	3471	3474	rBV	280	171	0.02%	0.002%
92	12.751	3546	3549	3551	rBV2	269	205	0.02%	0.003%
93	12.928	3601	3604	3610	rBV	336	243	0.03%	0.003%
94	13.227	3694	3697	3701	rBV	373	267	0.03%	0.004%
95	13.513	3783	3786	3788	rBV	350	212	0.02%	0.003%
96	13.722	3849	3851	3857	rBV2	237	198	0.02%	0.003%
97	14.015	3939	3942	3944	rBV	280	196	0.02%	0.003%
98	14.092	3963	3966	3967	rBV2	364	237	0.02%	0.003%
99	14.214	4002	4004	4008	rBV2	428	346	0.04%	0.005%
100	14.298	4027	4030	4032	rBV2	395	262	0.03%	0.004%




Sum of corrected areas: 7072720

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071122\
Data File : VU049683.D
Acq On : 11 Jul 2022 18:07
Operator : SY/MD
Sample : N3639-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

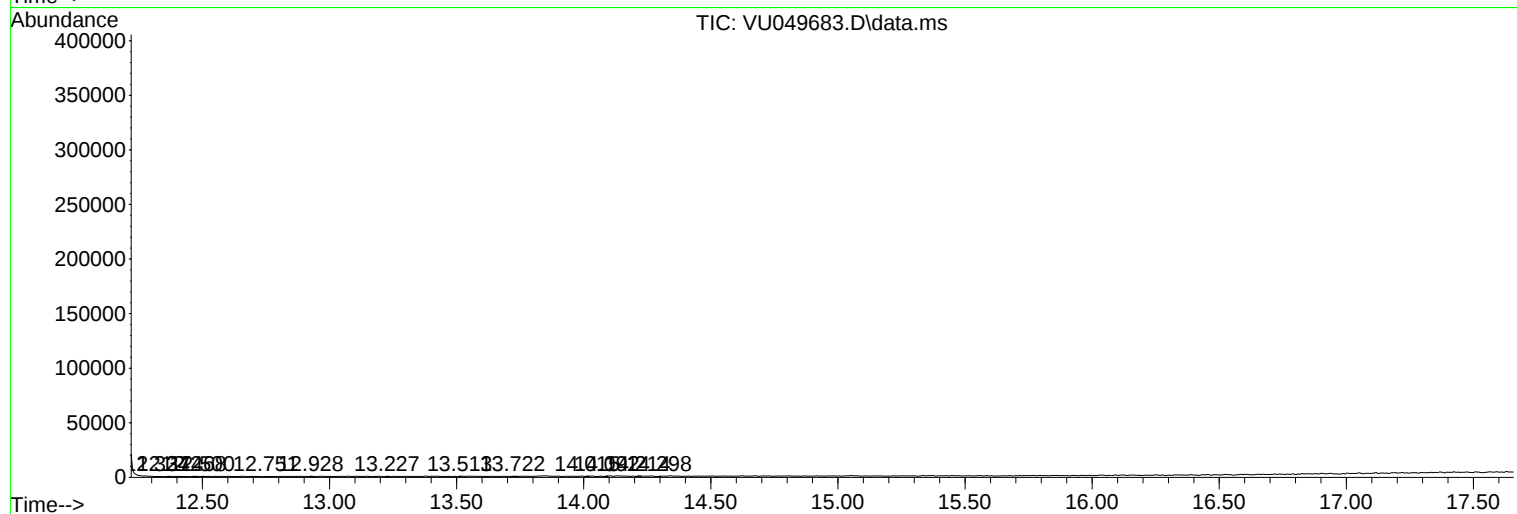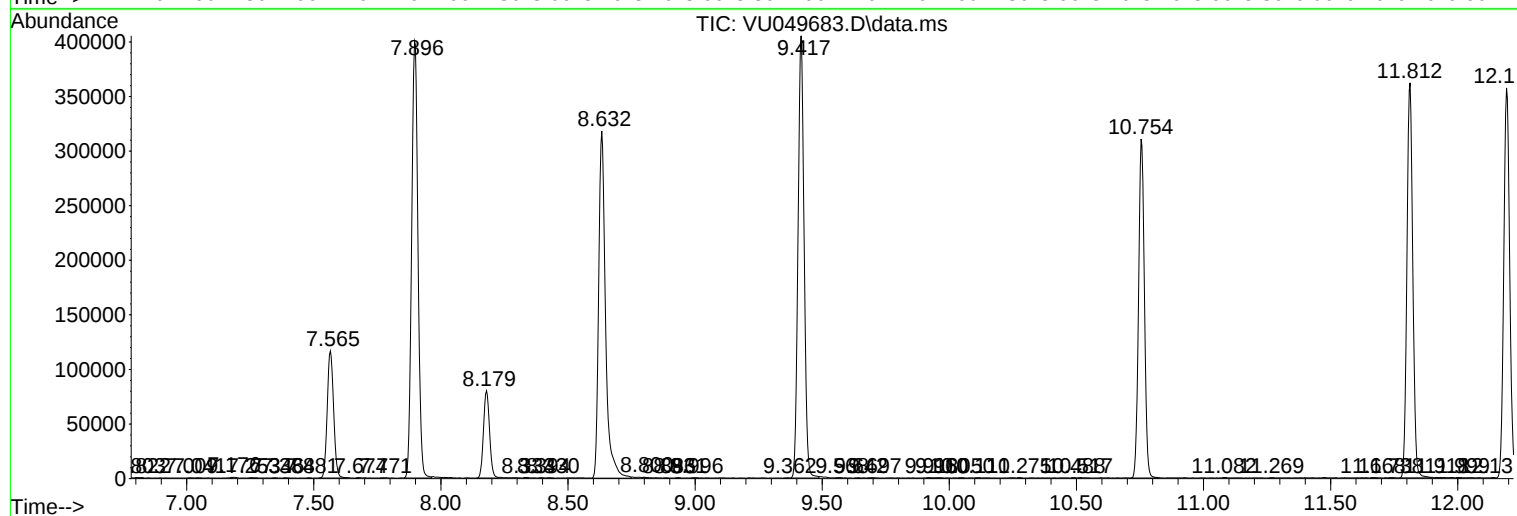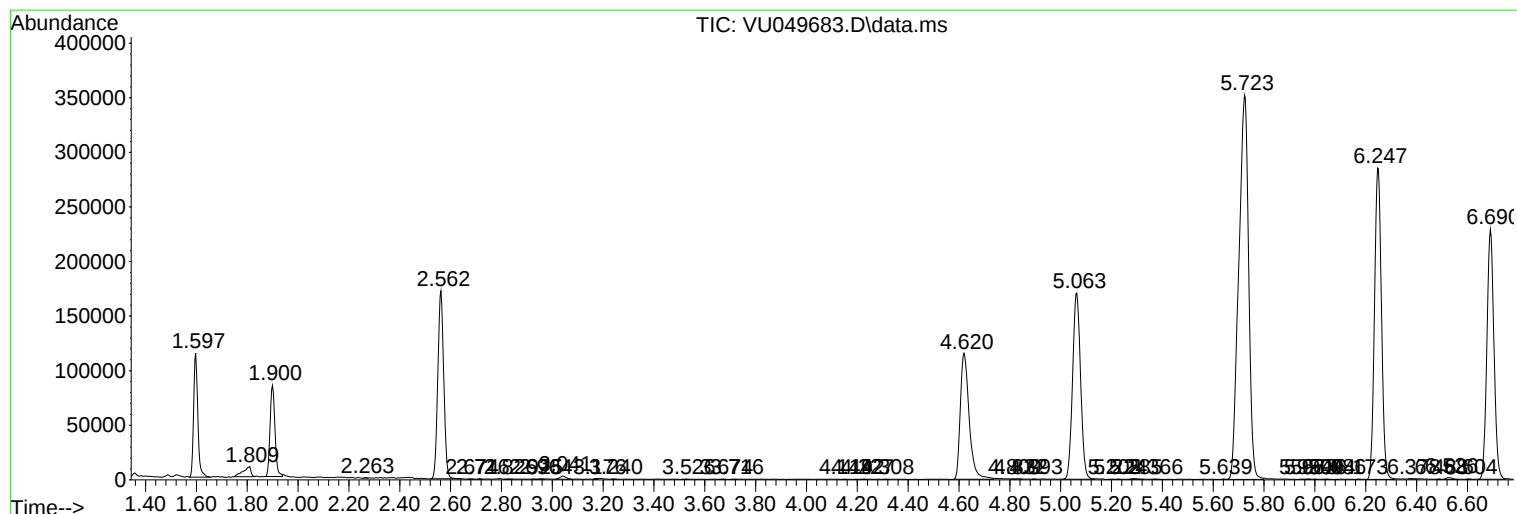

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071122\
Data File : VU049683.D
Acq On : 11 Jul 2022 18:07
Operator : SY/MD
Sample : N3639-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071122\
Data File : VU049683.D
Acq On : 11 Jul 2022 18:07
Operator : SY/MD
Sample : N3639-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------