

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071124\
 Data File : VU059897.D
 Acq On : 11 Jul 2024 09:44
 Operator : MD/SY
 Sample : VU0711WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jul 12 02:04:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 12 02:03:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	218043	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	225252	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	94989	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	71664	51.189	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	102.380%
7) Chloroethane-d5	1.904	69	62594	53.155	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	106.320%
11) 1,1-Dichloroethene-d2	2.557	63	91801	36.910	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.820%
21) 2-Butanone-d5	4.615	46	96984	99.682	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.680%
24) Chloroform-d	5.052	84	140177	51.705	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.400%
26) 1,2-Dichloroethane-d4	5.692	65	87500	54.281	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.560%
32) Benzene-d6	5.718	84	285751	49.540	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.080%
36) 1,2-Dichloropropane-d6	6.679	67	91702	51.368	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.740%
41) Toluene-d8	7.891	98	244757	44.621	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.240%
43) trans-1,3-Dichloroprop...	8.174	79	38305	45.854	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.700%
47) 2-Hexanone-d5	8.627	63	67569	89.810	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.810%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	142404	51.971	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.940%
66) 1,2-Dichlorobenzene-d4	12.187	152	92798	53.164	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.320%
Target Compounds						
60) 1,2,3-Trichloropropane	11.807	75	10063	5.582	ug/L	Qvalue # 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071124\
Data File : VU059897.D
Acq On : 11 Jul 2024 09:44
Operator : MD/SY
Sample : VU0711WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Jul 12 02:04:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 12 02:03:36 2024
Response via : Initial Calibration

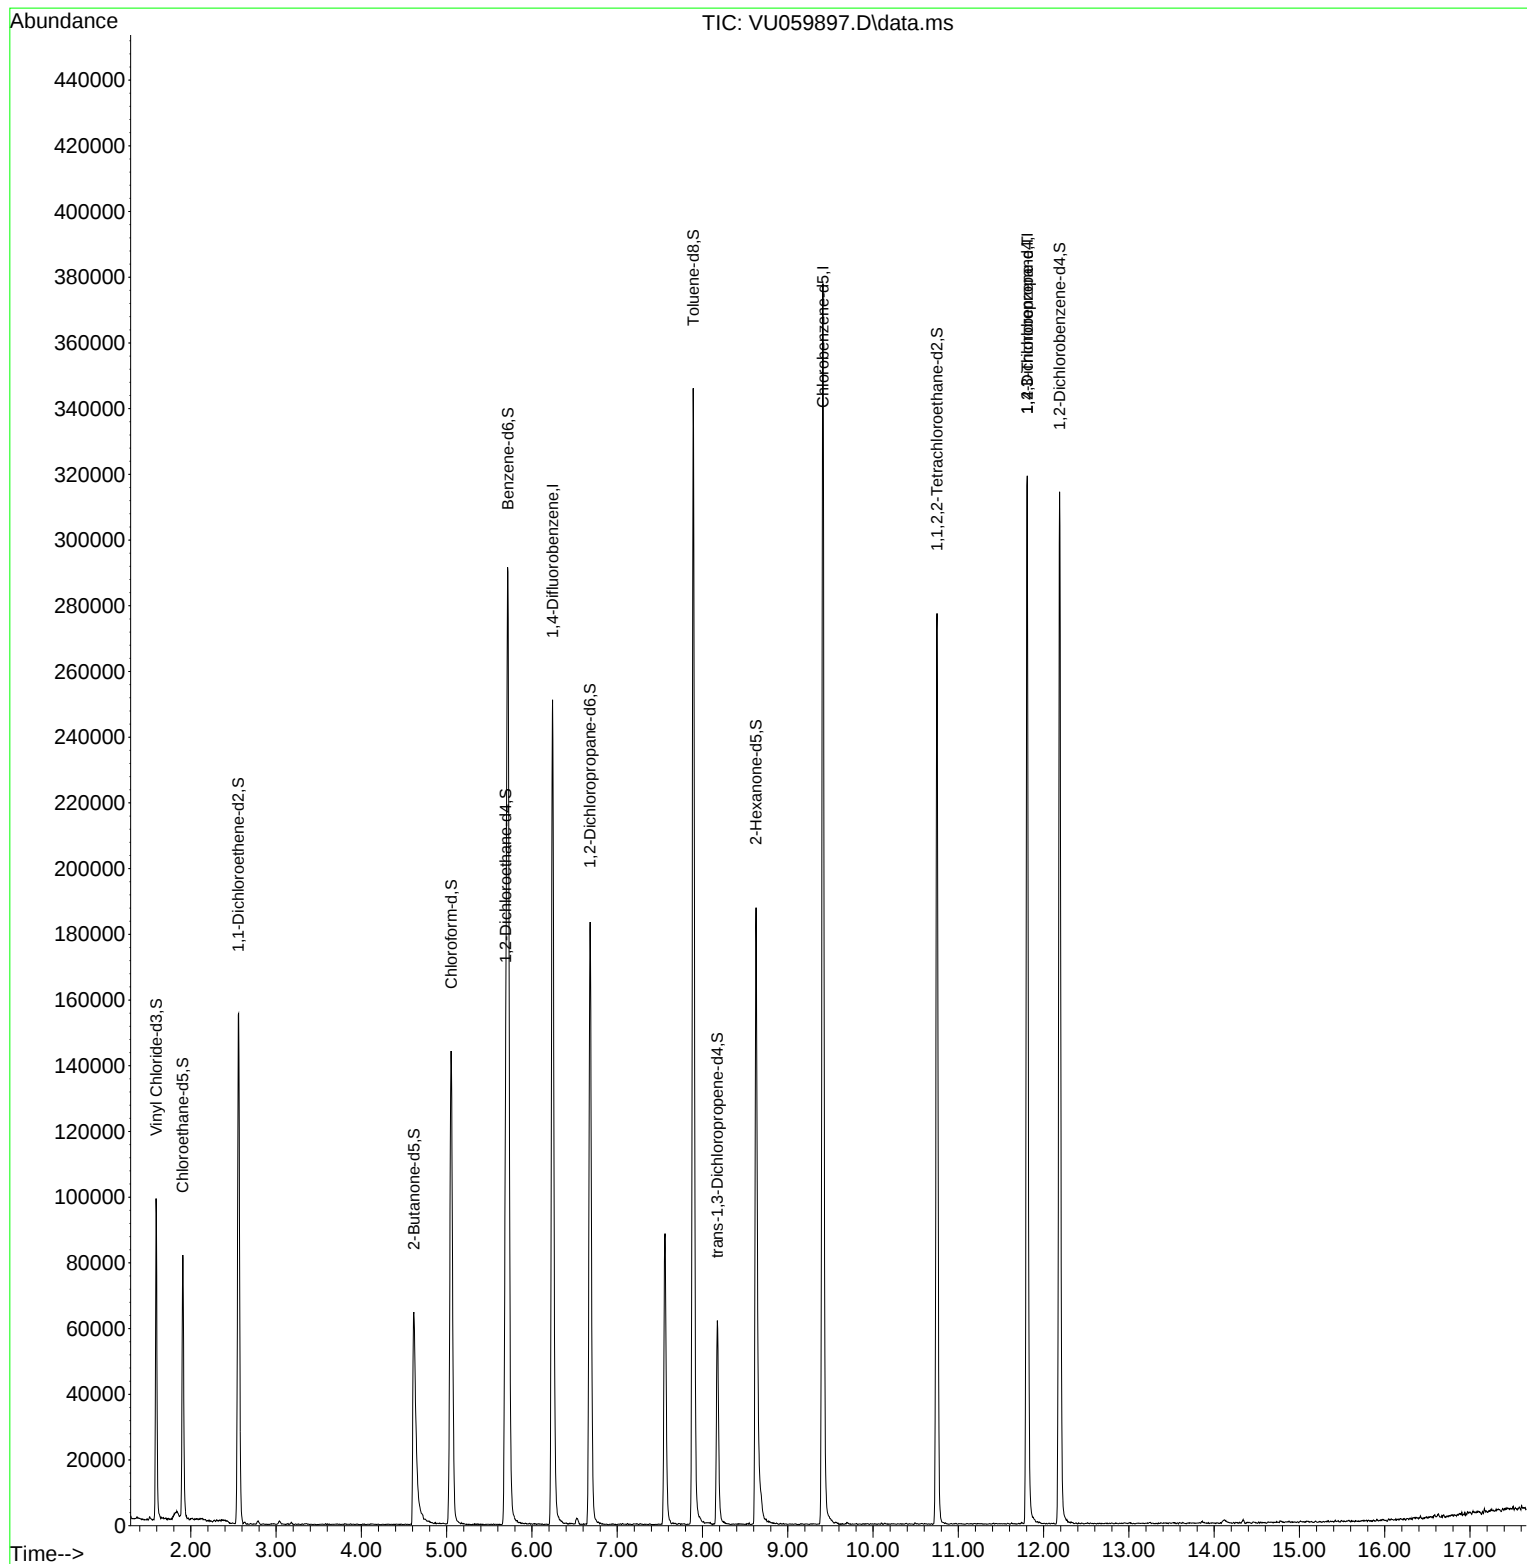

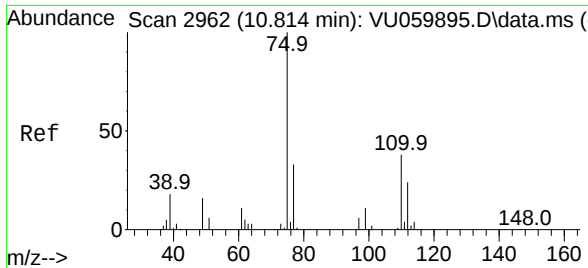

#60
 1,2,3-Trichloropropane
 Concen: 5.582 ug/L
 RT: 11.807 min Scan# 31
 Delta R.T. 0.994 min
 Lab File: VU059897.D
 Acq: 11 Jul 2024 09:44

Instrument :
 MSVOA_U
 ClientSampleId :

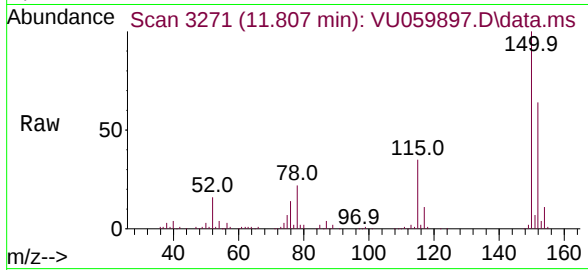

Tgt Ion:	75	Resp:	10063
Ion	Ratio	Lower	Upper
75	100		
77	29.7	25.5	38.3
110	1.6	30.7	46.1#

