
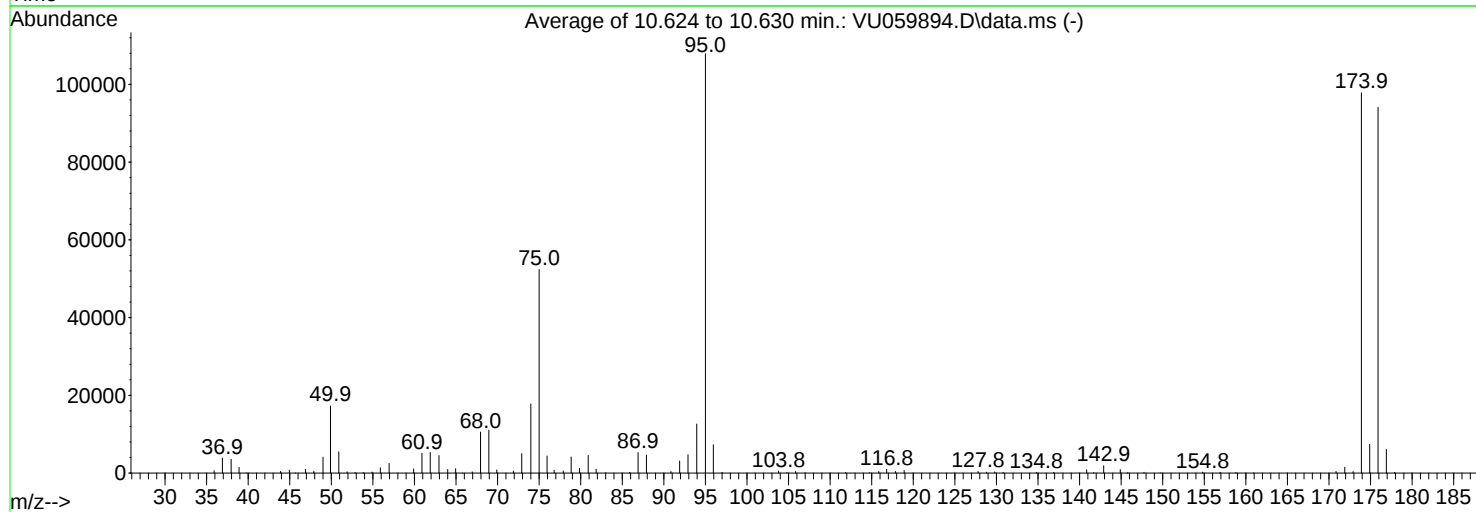


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071124\
Data File : VU059894.D
Acq On : 11 Jul 2024 07:55
Operator : MD/SY
Sample : BFB071
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB071

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Title : VOC Analysis
Last Update : Fri Jul 12 02:03:36 2024

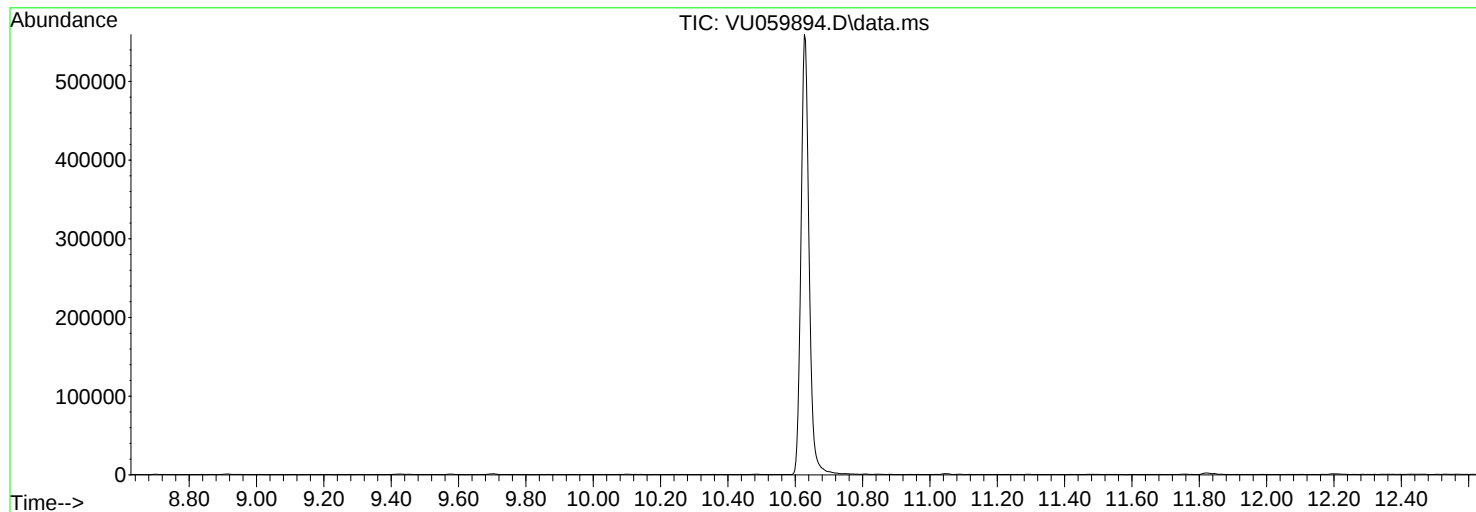

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	17283	PASS
75	95	30	80	48.5	52360	PASS
95	95	100	100	100.0	107888	PASS
96	95	5	9	6.8	7297	PASS
173	174	0.00	2	0.4	415	PASS
174	95	50	120	90.7	97840	PASS
175	174	5	9	7.5	7370	PASS
176	174	95	101	96.2	94109	PASS
177	176	5	9	6.4	6070	PASS

Scan 2891 (10.585 min): VU059894.D\data.ms
BFB071

m/z	Abundance
39.80	206.0
43.90	290.0

Instrument :
MSVOA_U
ClientSampleId :
BFB071

m/z	Abundance
35.90	627.0
36.90	3728.0
37.90	3694.0
38.90	1217.0
39.70	237.0
43.90	645.0
44.90	838.0
45.70	132.0
46.90	970.0
47.90	407.0
49.00	4065.0
49.90	16760.0
50.90	5348.0
51.90	349.0
52.90	149.0
53.80	122.0
54.90	267.0
55.90	1268.0
56.90	2454.0
59.90	993.0
60.90	4987.0
61.90	5271.0
62.90	4212.0
64.00	922.0
64.90	1030.0
66.90	346.0
68.00	9988.0
69.00	10420.0
69.90	778.0
71.90	503.0
72.90	4788.0
74.00	17168.0
75.00	50664.0
76.00	4111.0
76.80	675.0
77.90	609.0
78.90	4108.0
79.80	1189.0
80.90	4512.0
81.80	943.0
85.90	131.0
86.90	5085.0
87.90	4187.0
90.80	314.0
91.90	3002.0
92.90	4487.0
93.90	12069.0
95.00	102904.0
96.00	6938.0
97.00	185.0
103.80	493.0
104.80	132.0
105.80	399.0
107.00	143.0
111.90	105.0
114.80	128.0
115.90	458.0
116.80	912.0
117.90	451.0
118.90	721.0
127.80	390.0
128.80	215.0
129.80	253.0
130.80	201.0
134.80	144.0
136.80	149.0
140.80	812.0
141.70	163.0
142.90	1840.0
144.90	783.0
145.80	188.0
147.80	225.0
154.80	232.0
156.80	130.0
158.80	200.0
170.90	476.0
171.90	1333.0
173.90	90760.0
174.90	6901.0
175.90	88144.0
176.90	5787.0
177.90	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB071

m/z	Abundance
35.90	630.0
36.90	3966.0
38.00	3664.0
38.90	1533.0
39.80	263.0
43.90	734.0
44.90	793.0
46.90	922.0
47.90	514.0
49.00	4236.0
49.90	17800.0
50.90	5599.0
51.90	339.0
52.80	133.0
53.80	123.0
54.90	265.0
55.90	1409.0
57.00	2613.0
59.90	1152.0
60.90	5260.0
61.90	5542.0
63.00	4646.0
64.00	946.0
65.00	1153.0
66.90	327.0
68.00	10936.0
68.90	11432.0
69.90	831.0
71.90	536.0
72.90	5211.0
74.00	18288.0
75.00	53944.0
75.90	4509.0
76.80	792.0
77.90	582.0
78.90	4248.0
79.90	1211.0
80.90	4600.0
81.90	1038.0
83.00	100.0
85.90	169.0
86.90	5546.0
87.90	4789.0
90.90	411.0
91.90	3260.0
92.90	4851.0
93.90	13117.0
95.00	111624.0
95.90	7513.0
97.00	201.0
103.80	512.0
104.80	159.0
105.90	445.0
107.00	140.0
111.90	126.0
114.70	106.0
115.90	411.0
116.80	983.0
117.90	450.0
118.90	728.0
127.80	436.0
128.80	245.0
129.80	322.0
130.80	218.0
134.80	188.0
136.80	152.0
140.80	867.0
141.70	159.0
142.90	1924.0
144.90	949.0
145.80	171.0
147.80	226.0
149.70	114.0
154.80	258.0
157.00	186.0
158.80	177.0
160.90	115.0
170.90	447.0
171.90	1547.0
173.90	100976.0
174.90	7643.0
175.90	97272.0
176.90	6308.0
177.90	152.0

Instrument :
MSVOA_U
ClientSampleId :
BFB071

m/z	Abundance
35.90	610.0
36.90	3897.0
37.90	3301.0
38.90	1644.0
39.80	269.0
43.90	781.0
45.00	708.0
46.90	909.0
47.90	560.0
49.00	3995.0
49.90	17288.0
50.90	5422.0
51.90	305.0
52.80	124.0
53.90	122.0
54.90	245.0
55.90	1405.0
56.90	2468.0
59.90	1131.0
60.90	5084.0
61.90	5137.0
63.00	4723.0
64.00	914.0
65.00	1208.0
65.80	107.0
67.00	278.0
67.90	10711.0
68.90	11235.0
69.90	810.0
71.90	515.0
72.90	5005.0
74.00	17936.0
75.00	52472.0
75.90	4605.0
76.80	755.0
77.90	476.0
78.80	4088.0
79.90	1168.0
80.90	4443.0
81.90	1015.0
83.00	131.0
85.90	207.0
86.90	5234.0
87.90	4904.0
90.90	489.0
91.90	3087.0
92.90	4806.0
94.00	12661.0
95.00	109136.0
95.90	7441.0
97.00	223.0
103.80	473.0
104.80	171.0
105.90	437.0
111.80	108.0
115.80	343.0
116.80	1001.0
117.80	398.0
118.90	686.0
127.80	412.0
128.80	244.0
129.80	354.0
130.80	167.0
134.80	190.0
136.90	156.0
140.90	896.0
141.70	122.0
142.90	1871.0
144.90	1002.0
145.80	175.0
147.70	197.0
149.70	108.0
154.80	286.0
156.90	220.0
158.80	102.0
170.80	398.0
171.90	1659.0
172.90	1246.0
173.90	101784.0
174.90	7566.0
175.90	96912.0
176.90	6115.0
177.90	181.0

Instrument :
MSVOA_U
ClientSampleId :
BFB071