


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071125\
Data File : VU063482.D
Acq On : 11 Jul 2025 07:50
Operator : MD/SY
Sample : BFB
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U070825W.M
Title : SW846 8260
Last Update : Wed Jul 09 04:25:34 2025

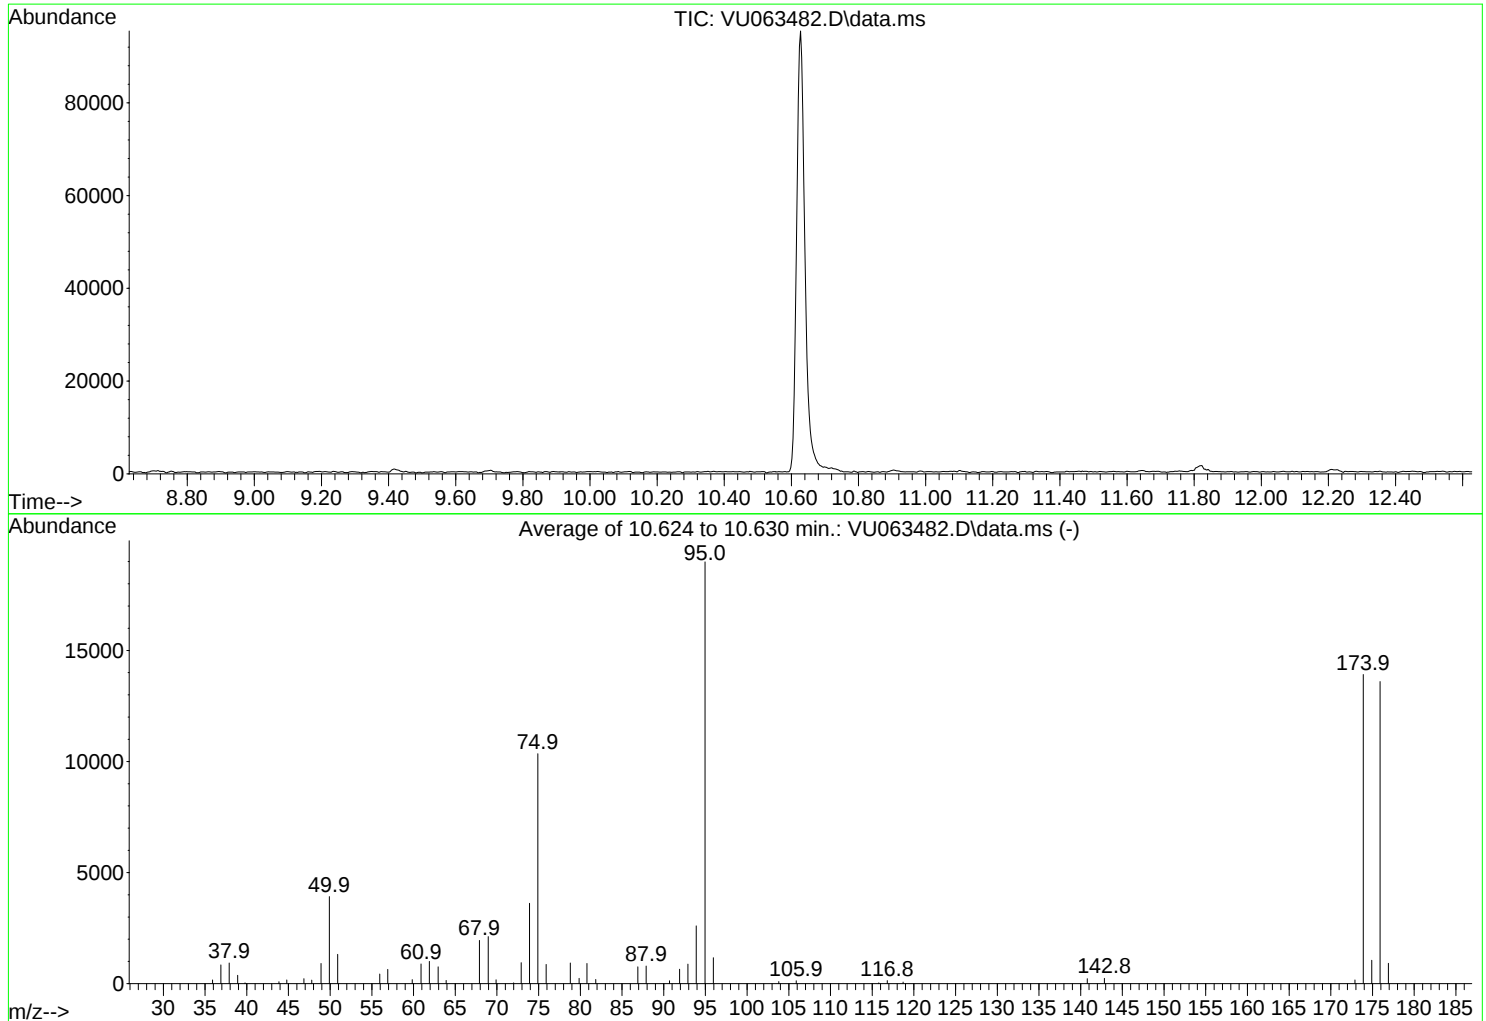

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	3920	PASS
75	95	30	60	54.5	10349	PASS
95	95	100	100	100.0	18989	PASS
96	95	5	9	6.2	1170	PASS
173	174	0.00	2	1.2	169	PASS
174	95	50	100	73.3	13918	PASS
175	174	5	9	7.6	1054	PASS
176	174	95	101	97.7	13596	PASS
177	176	5	9	6.7	913	PASS