


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU071218\
 Data File : VU025358.D
 Acq On : 12 Jul 2018 23:12
 Operator : MD/SY
 Sample : BFB
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U070918W.M
 Title : SW846 8260
 Last Update : Tue Jul 10 09:34:16 2018

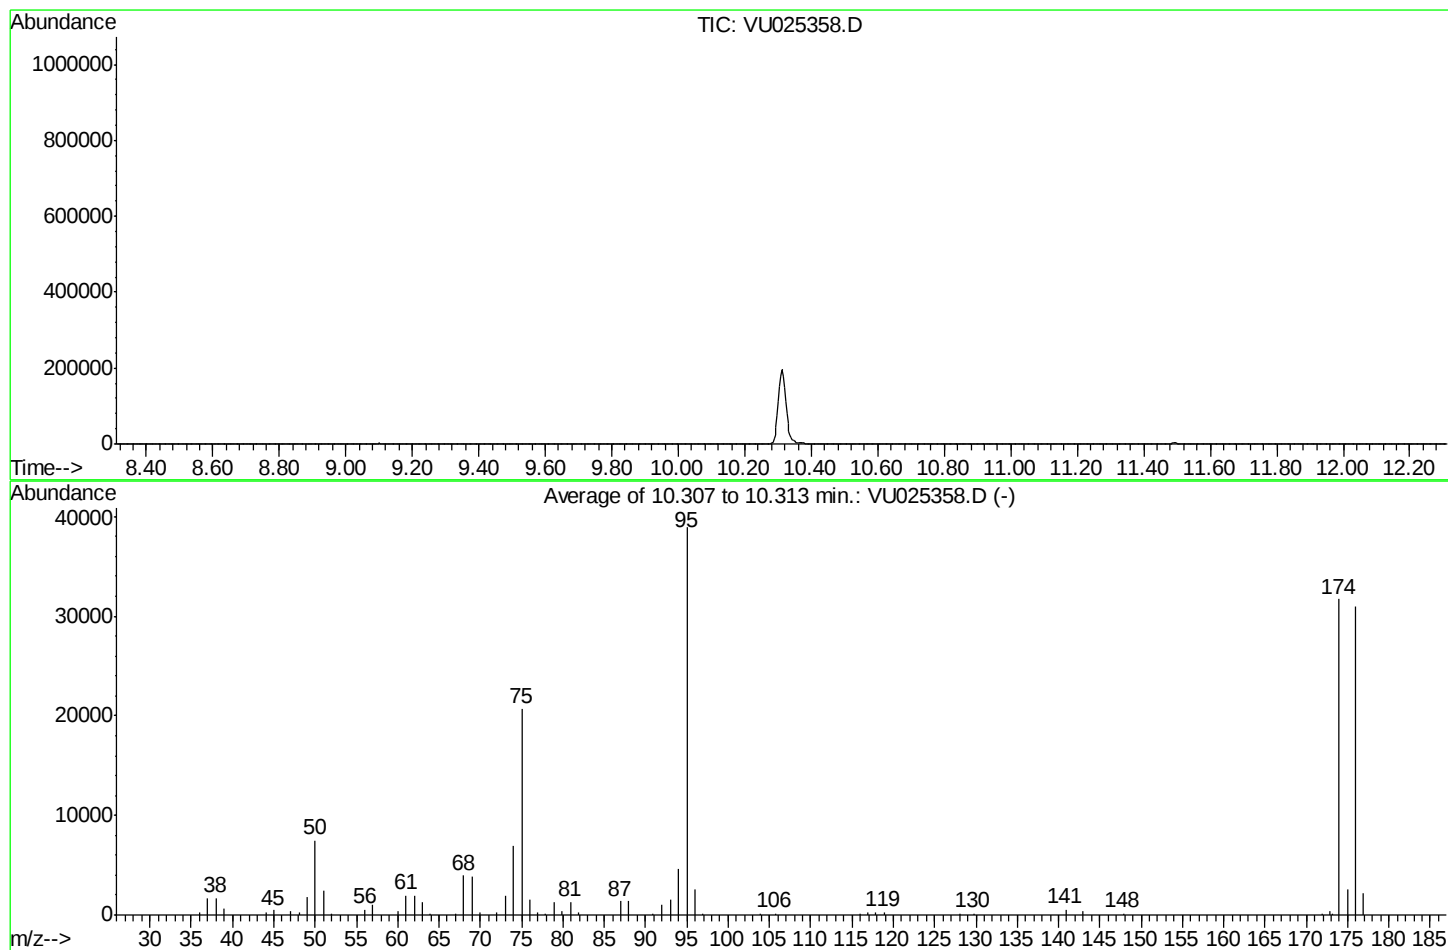

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	7502	PASS
75	95	30	60	53.2	20720	PASS
95	95	100	100	100.0	38912	PASS
96	95	5	9	6.8	2627	PASS
173	174	0.00	2	1.1	338	PASS
174	95	50	100	81.5	31730	PASS
175	174	5	9	8.0	2526	PASS
176	174	95	101	97.4	30914	PASS
177	176	5	9	6.9	2140	PASS