


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU071219\
Data File : VU033208.D
Acq On : 12 Jul 2019 08:18
Operator : JC/SP
Sample : BFB34
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB34

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
Title : VOC Analysis
Last Update : Sat Jul 13 00:05:57 2019

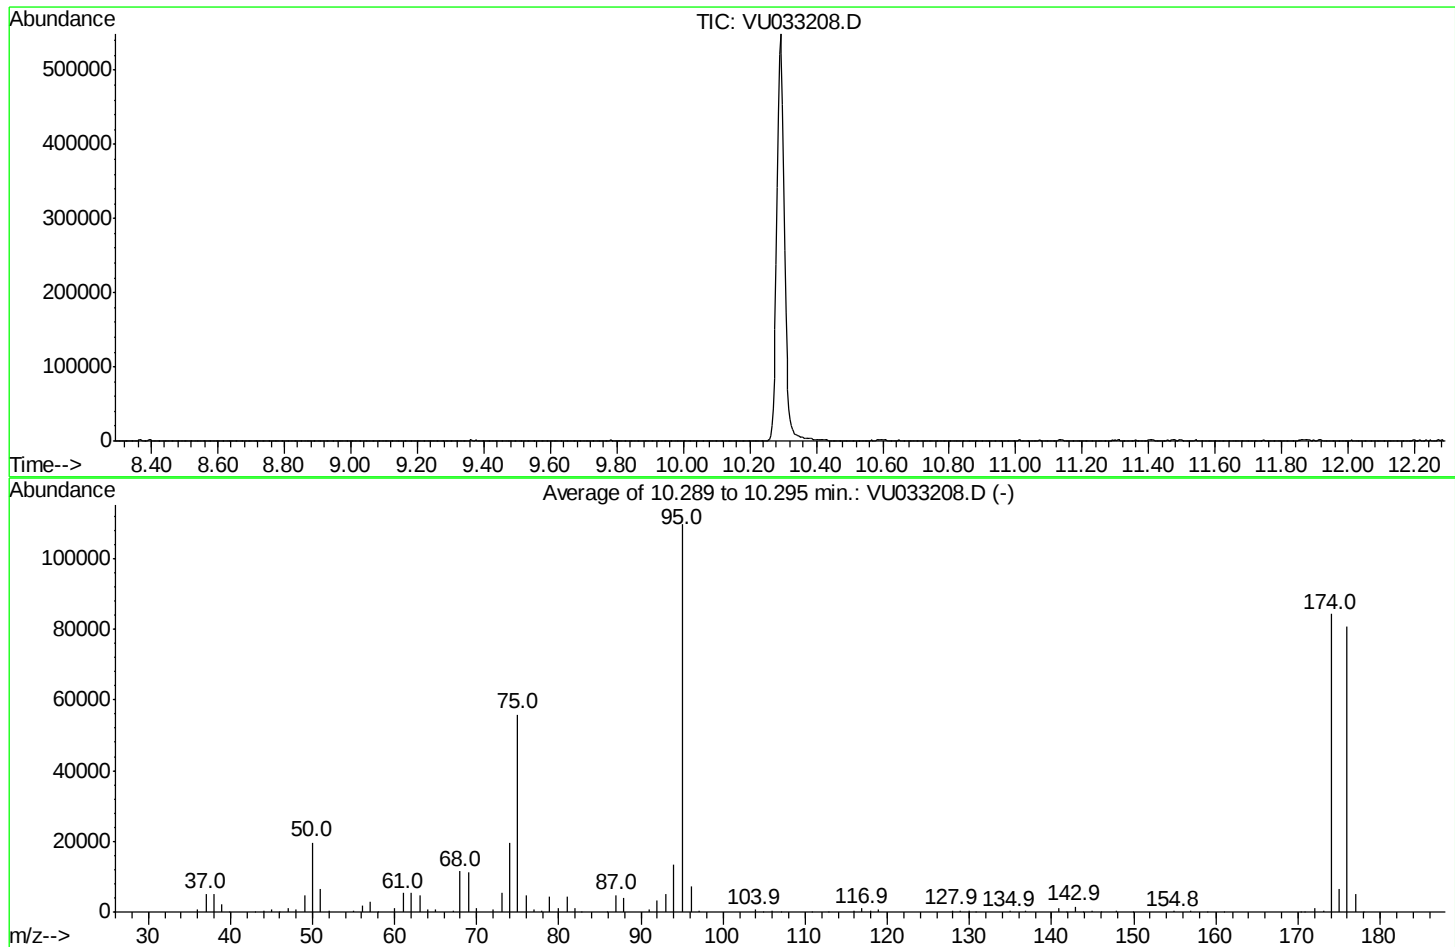

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2849

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	19629	PASS
75	95	30	80	50.9	55813	PASS
95	95	100	100	100.0	109672	PASS
96	95	5	9	6.6	7259	PASS
173	174	0.00	2	0.6	487	PASS
174	95	50	120	76.8	84277	PASS
175	174	5	9	7.7	6470	PASS
176	174	95	101	96.0	80901	PASS
177	176	5	9	6.3	5090	PASS

Scan 2849 (10.250 min): VU033208.D
BFB34

m/z	Abundance
39.80	204.0
44.00	427.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

m/z	Abundance
36.00	897.0
37.00	5190.0
38.00	5058.0
39.00	1856.0
39.90	312.0
43.00	118.0
44.00	973.0
45.00	876.0
45.90	151.0
47.10	1149.0
48.00	656.0
49.00	4529.0
50.00	19344.0
51.00	6619.0
52.00	344.0
54.90	381.0
56.00	1749.0
57.00	3146.0
57.90	111.0
60.00	968.0
61.00	5327.0
62.00	5319.0
63.00	4488.0
64.00	608.0
65.00	565.0
67.10	398.0
68.00	11554.0
69.00	11237.0
70.00	988.0
72.10	630.0
73.00	5410.0
74.00	19416.0
75.00	55200.0
76.00	4752.0
77.00	856.0
77.90	375.0
78.90	4503.0
80.00	988.0
81.00	4373.0
81.90	962.0
82.80	137.0
85.90	215.0
87.00	4411.0
87.90	4107.0
91.00	538.0
92.00	3192.0
93.00	5107.0
94.00	13811.0
95.00	108416.0
96.10	7365.0
97.00	308.0
103.90	569.0
104.80	166.0
105.90	509.0
107.00	102.0
110.90	102.0
112.80	135.0
115.90	338.0
116.90	1010.0
117.90	556.0
118.90	729.0
127.90	416.0
128.90	184.0
129.90	393.0
130.70	141.0
134.90	212.0
136.80	228.0
140.90	1168.0
142.90	1520.0
143.90	186.0
145.00	366.0
146.00	133.0
147.90	269.0
154.80	253.0
156.90	171.0
159.00	100.0
161.00	126.0
170.80	214.0
172.00	906.0
173.10	1461.0
174.00	79032.0
175.00	6398.0
176.00	77384.0
177.00	5050.0
178.00	167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

m/z	Abundance
36.00	930.0
37.00	5374.0
38.00	5237.0
39.00	2101.0
39.90	292.0
43.00	114.0
44.00	972.0
45.00	786.0
47.10	1117.0
48.00	603.0
49.00	4785.0
50.00	20272.0
51.00	6655.0
52.00	341.0
55.00	423.0
56.10	1850.0
57.00	3030.0
58.00	144.0
60.00	940.0
61.00	5577.0
62.00	5799.0
63.10	4704.0
64.00	677.0
65.00	616.0
67.10	373.0
68.00	11833.0
69.00	11748.0
70.00	1034.0
72.10	605.0
73.00	5636.0
74.00	20272.0
75.00	57712.0
76.00	4905.0
76.90	805.0
77.90	410.0
78.90	4782.0
80.00	1080.0
80.90	4462.0
81.90	957.0
82.80	144.0
85.90	204.0
87.00	4930.0
87.90	4257.0
91.00	584.0
92.00	3264.0
93.00	5440.0
94.00	14001.0
95.00	113560.0
96.10	7540.0
97.00	299.0
103.90	643.0
104.80	152.0
105.90	552.0
107.00	104.0
110.90	105.0
112.90	117.0
115.90	401.0
116.90	1021.0
117.90	484.0
118.90	747.0
127.90	472.0
128.90	239.0
130.00	424.0
130.80	108.0
134.90	231.0
136.80	223.0
140.90	1304.0
141.80	109.0
142.90	1572.0
143.90	160.0
145.00	348.0
145.90	150.0
147.90	271.0
149.90	100.0
154.90	264.0
156.90	212.0
161.00	137.0
170.90	195.0
172.00	964.0
174.00	87136.0
175.00	6630.0
176.00	83816.0
177.00	5240.0
178.00	164.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34

m/z	Abundance
36.00	858.0
37.00	5163.0
38.00	4873.0
39.00	2069.0
39.90	270.0
44.00	958.0
45.10	668.0
47.10	1009.0
48.00	570.0
49.00	4570.0
50.00	19272.0
51.00	6154.0
52.00	304.0
55.00	388.0
56.10	1863.0
57.00	2843.0
58.10	164.0
60.00	891.0
61.00	5225.0
62.00	5649.0
63.10	4454.0
64.00	657.0
65.00	561.0
67.10	288.0
68.00	10954.0
69.00	11221.0
70.00	995.0
72.00	535.0
73.00	5229.0
74.00	19000.0
75.00	54528.0
76.00	4649.0
76.90	739.0
77.90	418.0
78.90	4305.0
80.00	1150.0
80.90	4229.0
81.90	841.0
82.80	147.0
85.90	166.0
87.00	4908.0
88.00	4002.0
91.00	547.0
92.00	3217.0
93.00	5039.0
94.00	12928.0
95.00	107040.0
96.10	6872.0
97.00	244.0
103.90	585.0
104.90	141.0
105.90	476.0
110.80	100.0
115.90	473.0
116.90	901.0
117.90	390.0
118.90	706.0
127.90	479.0
128.90	253.0
129.90	390.0
134.90	234.0
136.90	192.0
140.90	1316.0
141.80	148.0
142.90	1401.0
143.90	111.0
145.00	283.0
145.90	158.0
147.80	224.0
154.90	247.0
156.90	206.0
161.00	113.0
170.40	108.0
170.90	129.0
172.00	947.0
174.00	86664.0
175.00	6384.0
176.00	81504.0
177.00	4980.0
177.90	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB34