

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071224\
 Data File : VU059918.D
 Acq On : 12 Jul 2024 13:52
 Operator : MD/SY
 Sample : P3230-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHB69

Quant Time: Jul 13 03:55:37 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jul 13 03:52:33 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	154339	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	156695	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	72811	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	50090	4.667	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.400%
7) Chloroethane-d5	1.911	69	41930	4.061	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.200%
11) 1,1-Dichloroethene-d2	2.560	65	19285	4.331	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.600%
20) 2-Butanone-d5	4.628	46	93841	42.450	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.900%
24) Chloroform-d	5.055	84	86945	3.947	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.000%
26) 1,2-Dichloroethane-d4	5.698	65	42954	4.048	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.000%
32) Benzene-d6	5.721	84	180224	4.179	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.600%
36) 1,2-Dichloropropane-d6	6.685	67	55245	4.181	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.600%
41) Toluene-d8	7.891	98	152751	3.810	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.200%
43) trans-1,3-Dichloroprop...	8.177	79	18046	4.361	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.200%
46) 2-Hexanone-d5	8.627	63	71344	41.496	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.000%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	44025	4.032	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	80.600%
66) 1,2-Dichlorobenzene-d4	12.187	152	58394	4.506	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.200%
Target Compounds						
					Qvalue	
13) Acetone	2.640	43	16556	11.545	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071224\
Data File : VU059918.D
Acq On : 12 Jul 2024 13:52
Operator : MD/SY
Sample : P3230-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHB69

Quant Time: Jul 13 03:55:37 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jul 13 03:52:33 2024
Response via : Initial Calibration

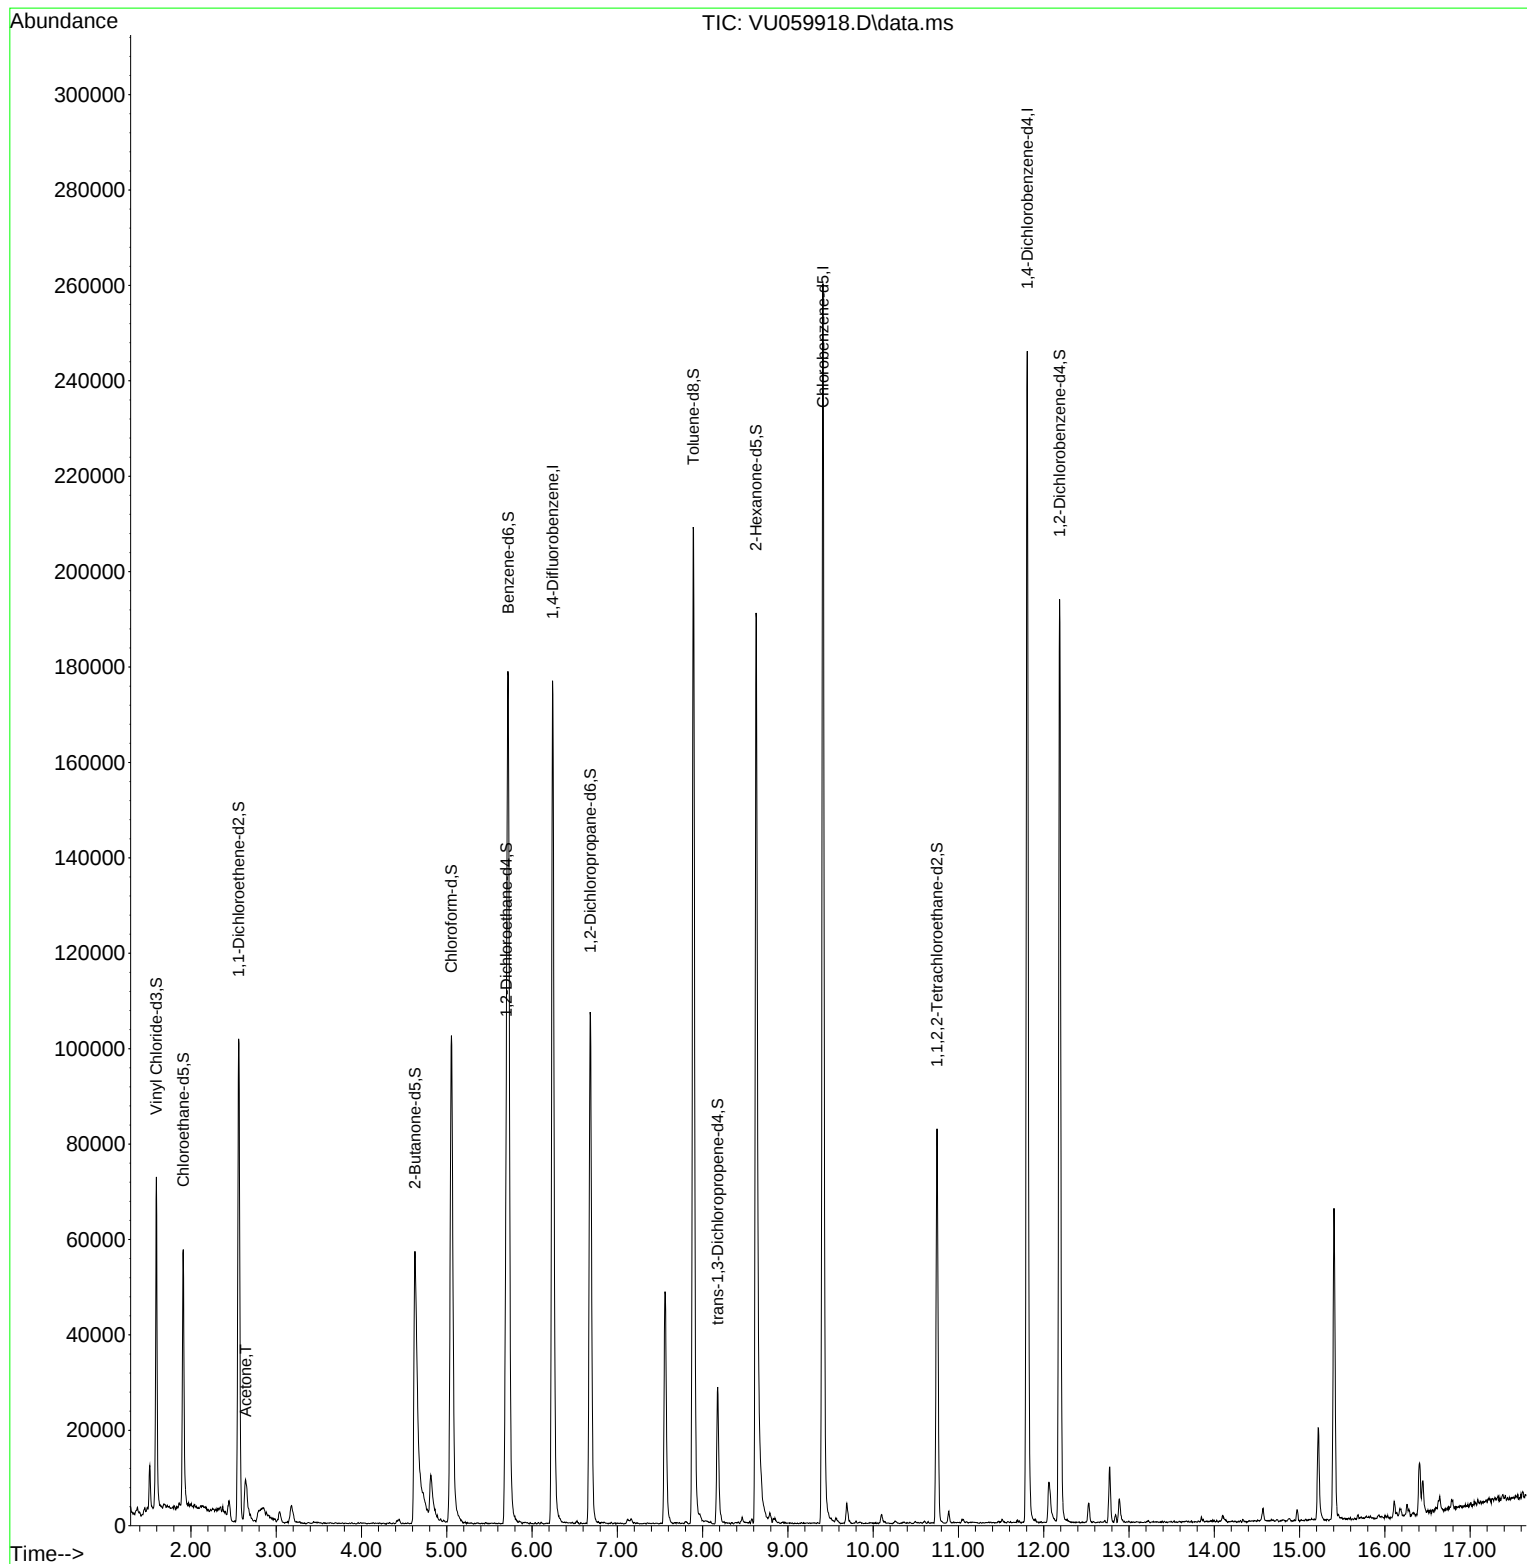

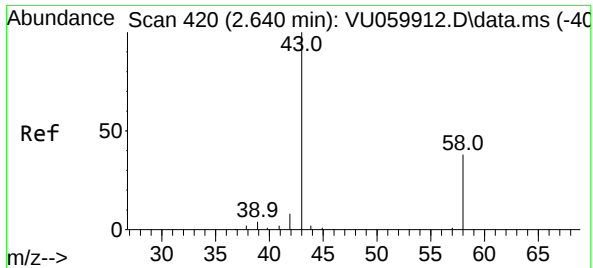

#13
 Acetone
 Concen: 11.545 ug/L
 RT: 2.640 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: VU059918.D
 Acq: 12 Jul 2024 13:52

Instrument :
 MSVOA_U
 ClientSampleId :
 BHB69

Tgt Ion: 43 Resp: 16556
 Ion Ratio Lower Upper
 43 100
 58 29.3 0.0 68.0

