

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071224\
 Data File : VU059924.D
 Acq On : 12 Jul 2024 16:12
 Operator : MD/SY
 Sample : P3217-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YDZG5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU059924.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.075	234	244	262	rBV	224379	326537	1.22%	0.543%
2	2.560	382	395	414	rVB3	161300	302556	1.13%	0.503%
3	3.345	623	639	661	rBV	454433	917430	3.44%	1.525%
4	4.653	1028	1046	1087	rBV	7366222	16624743	62.27%	27.633%
5	5.718	1356	1377	1388	rBV2	234608	607826	2.28%	1.010%
6	6.242	1526	1540	1564	rBV	240640	463553	1.74%	0.771%
7	6.534	1613	1631	1665	rBV	4351287	8111629	30.38%	13.483%
8	7.891	2040	2053	2068	rBV	294804	509064	1.91%	0.846%
9	8.547	2242	2257	2273	rBV	1322918	2217651	8.31%	3.686%
10	8.631	2273	2283	2310	rVV	286050	570126	2.14%	0.948%
11	9.441	2514	2535	2585	rBV	15920181	26697223	100.00%	44.375%
12	11.807	3259	3271	3290	rBV2	383961	807524	3.02%	1.342%
13	12.203	3377	3394	3414	rBV2	553090	1250832	4.69%	2.079%
14	15.216	4319	4331	4352	rBV	274694	451280	1.69%	0.750%
15	15.402	4376	4389	4405	rBV	179415	304455	1.14%	0.506%




Sum of corrected areas: 60162429

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071224\
Data File : VU059924.D
Acq On : 12 Jul 2024 16:12
Operator : MD/SY
Sample : P3217-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YDZG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

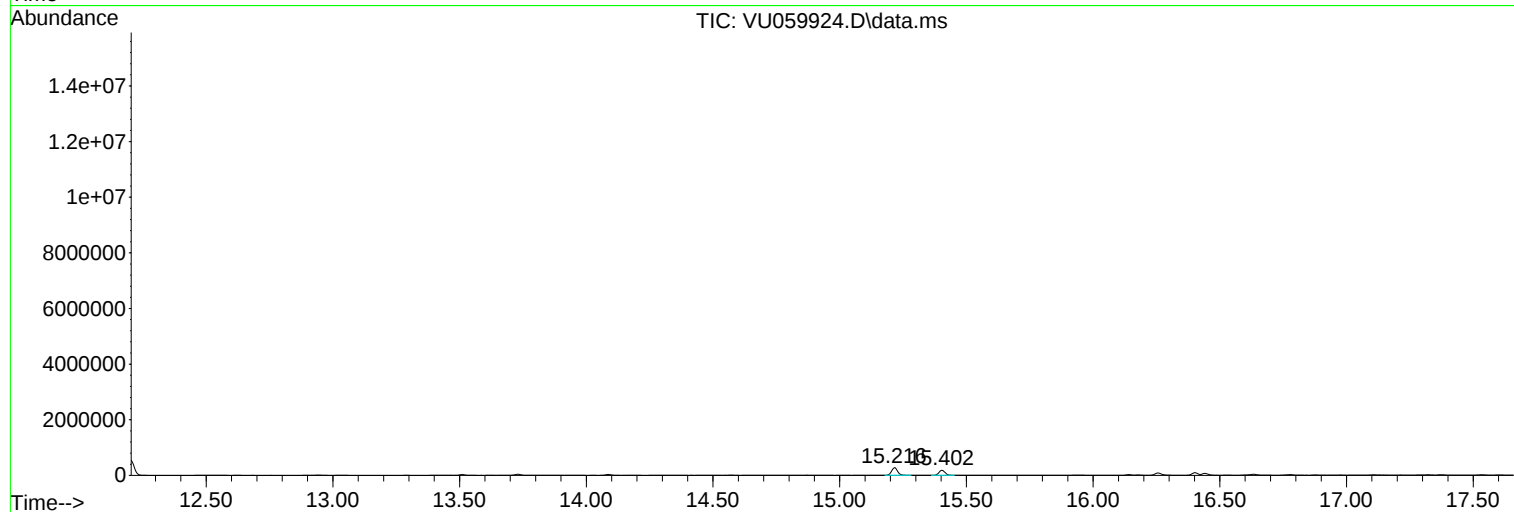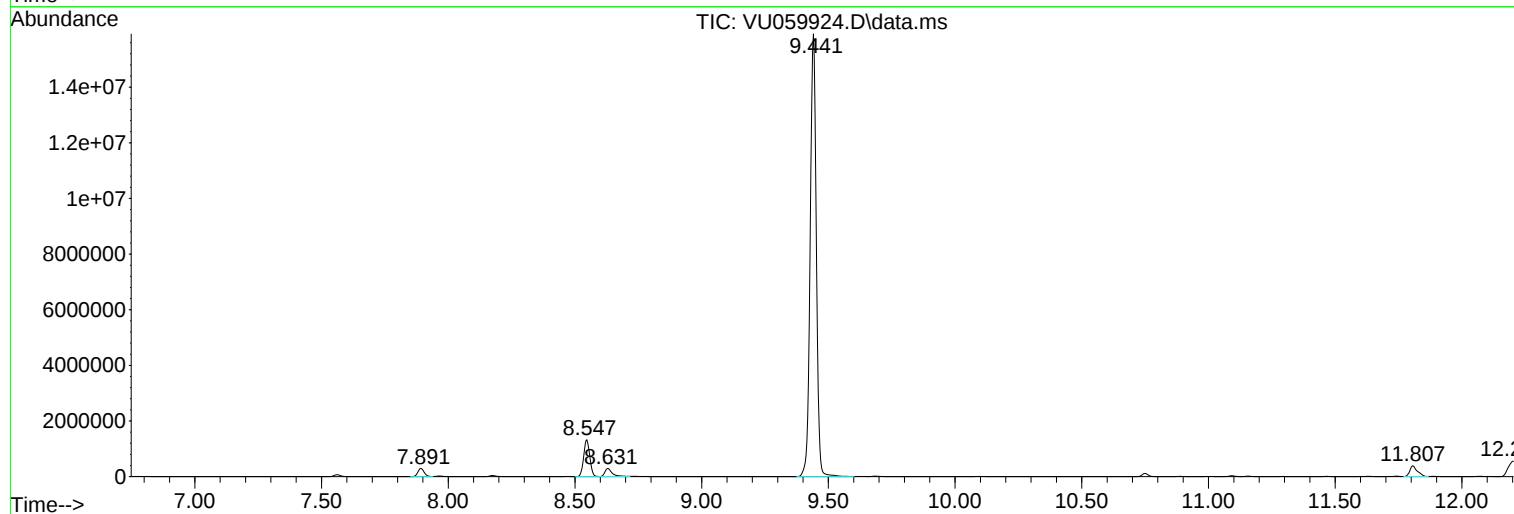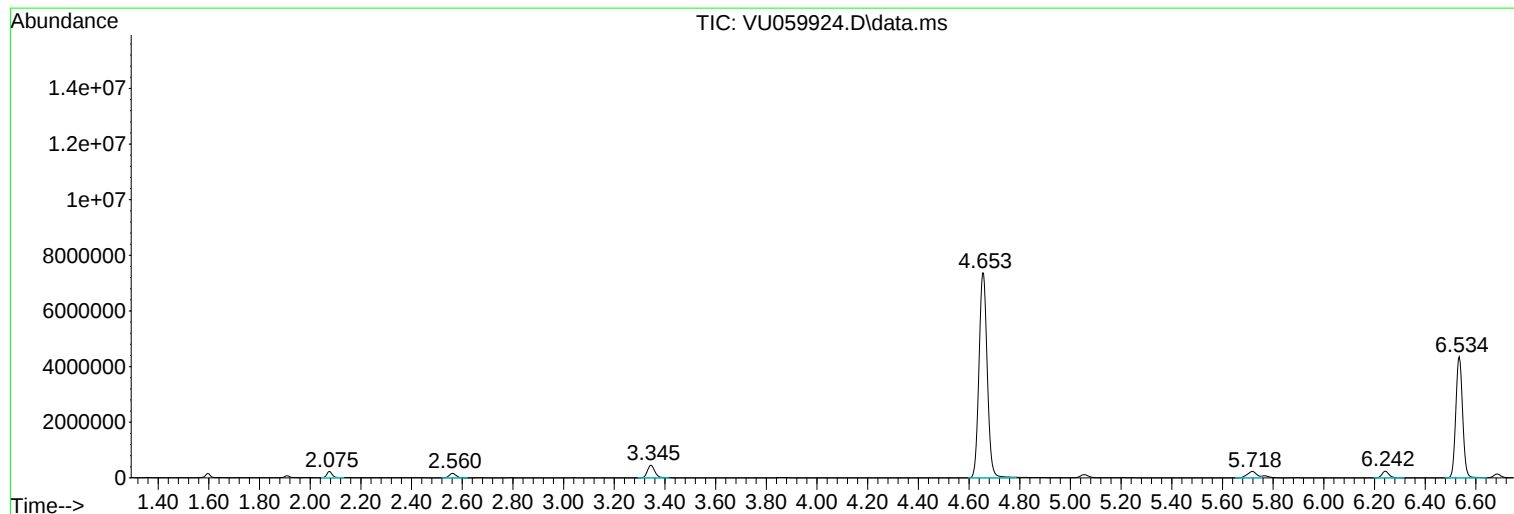

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071224\
Data File : VU059924.D
Acq On : 12 Jul 2024 16:12
Operator : MD/SY
Sample : P3217-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YDZG5










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.075	3.52 ug/L	326537	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
2			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
3			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
4			1-Butyne, 3,3-dimethyl-	82	C6H10	000917-92-0	7
5			Methanamine, N,N-difluoro-	67	CH3F2N	000753-58-2	4

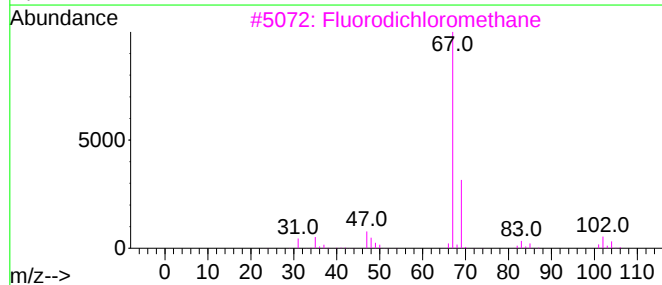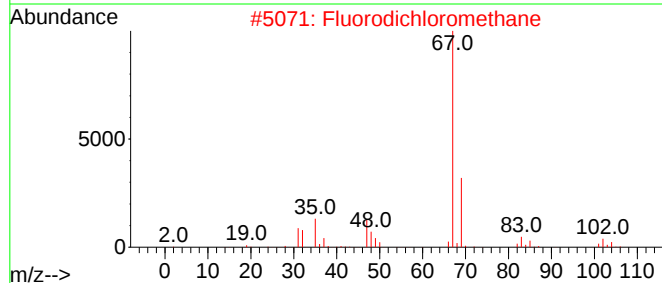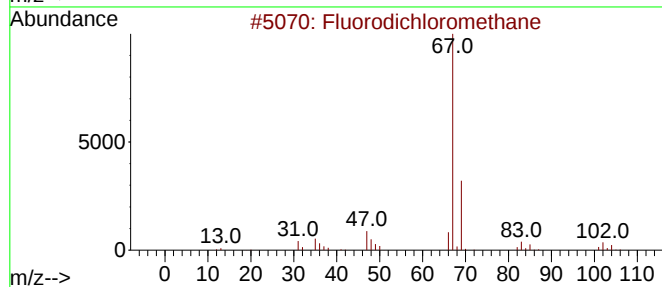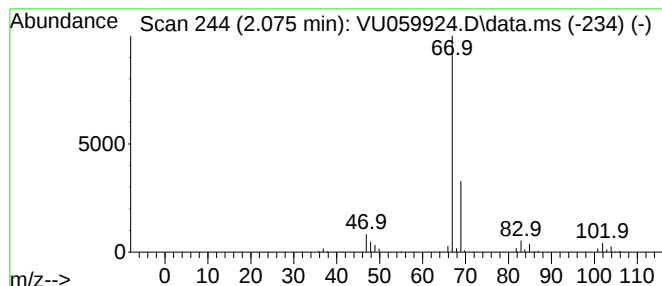

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071224\
Data File : VU059924.D
Acq On : 12 Jul 2024 16:12
Operator : MD/SY
Sample : P3217-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YDZG5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorodichlorom...	2.075	3.5	ug/L	326537	1	6.242	463553	5.0