


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071224\
Data File : VU059911.D
Acq On : 12 Jul 2024 10:22
Operator : MD/SY
Sample : BFB173
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB173

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Jul 13 03:52:33 2024

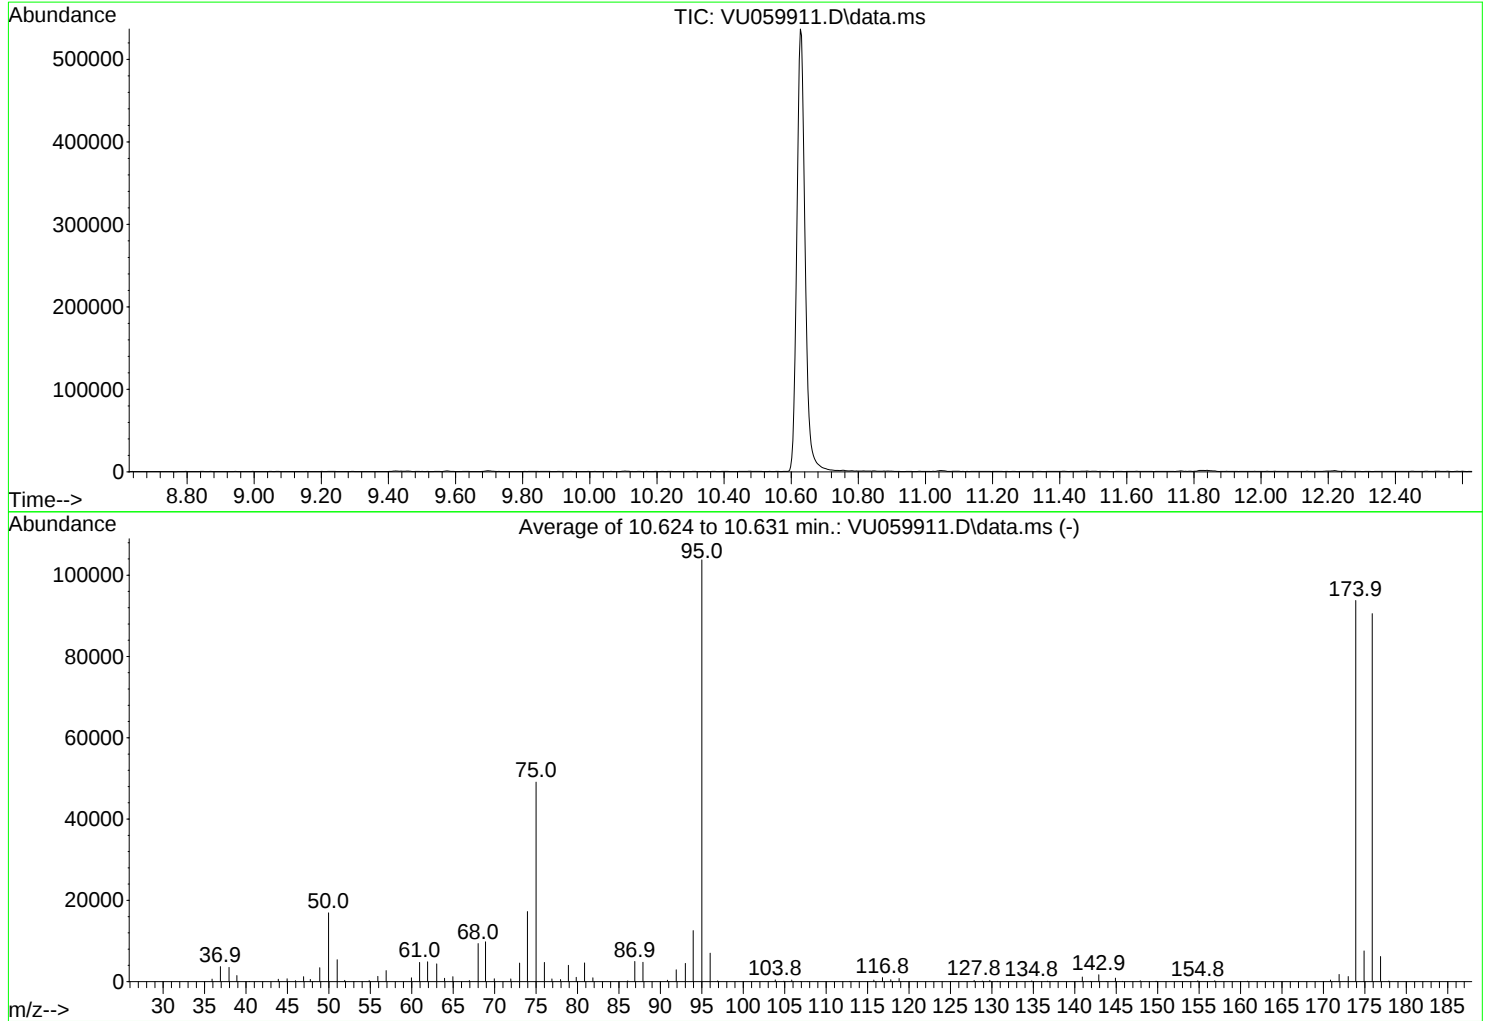

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.3	16913	PASS
75	95	30	80	47.3	49093	PASS
95	95	100	100	100.0	103781	PASS
96	95	5	9	6.7	6995	PASS
173	174	0.00	2	1.4	1276	PASS
174	95	50	120	90.4	93795	PASS
175	174	5	9	8.1	7565	PASS
176	174	95	101	96.6	90563	PASS
177	176	5	9	6.8	6171	PASS

Scan 2890 (10.582 min): VU059911.D\data.ms
BFB173

m/z	Abundance
39.80	356.0
43.90	278.0

Instrument :
MSVOA_U
ClientSampleId :
BFB173

m/z	Abundance
35.90	684.0
36.90	3702.0
38.00	3412.0
38.90	1442.0
39.90	351.0
43.90	790.0
45.00	678.0
46.00	254.0
46.90	1155.0
47.80	499.0
48.90	3286.0
50.00	16292.0
51.00	5138.0
51.90	270.0
53.00	120.0
54.90	250.0
55.90	1250.0
56.90	2603.0
59.90	882.0
60.90	4465.0
61.90	4836.0
63.00	4389.0
63.90	789.0
65.00	1086.0
67.00	249.0
68.00	8831.0
68.90	9874.0
70.00	647.0
71.90	662.0
73.00	4456.0
73.90	16904.0
75.00	47120.0
76.00	4408.0
76.90	685.0
77.90	544.0
78.90	3981.0
79.80	1061.0
80.90	4531.0
81.80	936.0
86.10	189.0
86.90	5240.0
87.90	4769.0
90.80	305.0
91.90	2850.0
93.00	4288.0
94.00	11999.0
95.00	99776.0
96.00	6859.0
96.90	156.0
103.90	400.0
105.00	107.0
105.80	406.0
107.80	121.0
115.80	447.0
116.80	967.0
117.80	389.0
118.80	717.0
127.90	263.0
128.80	122.0
129.80	322.0
130.70	123.0
134.80	191.0
136.70	172.0
140.90	1056.0
142.90	1627.0
144.90	915.0
147.90	251.0
149.80	129.0
154.80	240.0
156.90	262.0
160.80	103.0
170.80	421.0
171.90	1581.0
173.00	1274.0
173.90	88480.0
174.90	7315.0
175.90	85240.0
176.90	5721.0
177.90	156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB173

m/z	Abundance
35.90	644.0
36.90	3844.0
37.90	3541.0
38.90	1559.0
39.90	277.0
43.90	901.0
45.00	716.0
45.90	256.0
47.00	1243.0
47.70	599.0
48.90	3536.0
50.00	17376.0
51.00	5547.0
51.90	351.0
54.80	286.0
55.90	1327.0
56.90	2787.0
59.90	971.0
60.90	4896.0
61.90	5092.0
63.00	4438.0
64.00	870.0
64.90	1306.0
66.90	270.0
68.00	9627.0
68.90	10047.0
69.90	721.0
72.00	734.0
73.00	4717.0
74.00	17928.0
75.00	50504.0
76.00	4929.0
76.90	687.0
78.00	556.0
78.90	4090.0
79.90	1054.0
80.90	4743.0
81.80	948.0
86.00	231.0
86.90	5115.0
87.90	4902.0
90.80	328.0
91.90	2948.0
93.00	4585.0
94.00	12948.0
95.00	106696.0
96.00	7262.0
96.90	226.0
103.80	420.0
104.90	125.0
105.90	393.0
112.90	115.0
115.80	440.0
116.80	1046.0
117.80	515.0
118.80	780.0
127.90	331.0
128.90	152.0
129.70	328.0
130.70	122.0
134.80	189.0
136.70	161.0
140.90	1184.0
141.90	109.0
142.90	1769.0
144.90	919.0
145.80	124.0
147.90	221.0
149.80	141.0
154.80	276.0
156.90	248.0
160.90	114.0
170.90	424.0
171.90	1857.0
173.00	1309.0
173.90	96168.0
174.90	7877.0
175.90	93264.0
176.90	6366.0
177.90	187.0

Instrument :
MSVOA_U
ClientSampleId :
BFB173

m/z	Abundance
35.90	530.0
36.90	3588.0
37.90	3520.0
38.90	1480.0
39.80	259.0
40.40	106.0
43.90	876.0
44.90	702.0
45.90	198.0
46.90	1222.0
47.80	547.0
48.90	3450.0
49.90	17072.0
51.00	5507.0
51.90	356.0
54.80	263.0
55.90	1315.0
56.90	2711.0
60.00	969.0
61.00	4864.0
61.90	4664.0
63.00	4264.0
64.00	845.0
64.90	1294.0
66.90	287.0
68.00	9653.0
68.90	9481.0
69.90	721.0
71.90	675.0
73.00	4589.0
74.00	16944.0
75.00	49656.0
76.00	4847.0
76.90	625.0
77.90	503.0
78.90	3984.0
79.90	1034.0
80.80	4519.0
81.90	908.0
86.00	190.0
86.90	4570.0
87.90	4687.0
90.90	379.0
91.90	3001.0
93.00	4636.0
93.90	12712.0
95.00	104872.0
96.00	6863.0
96.90	227.0
103.80	436.0
104.80	123.0
105.90	393.0
106.90	118.0
112.80	108.0
115.70	322.0
116.80	1009.0
117.80	563.0
118.80	825.0
127.80	373.0
128.80	164.0
129.70	287.0
134.80	168.0
136.90	158.0
140.90	1171.0
141.90	132.0
142.90	1726.0
143.80	105.0
144.90	795.0
145.80	164.0
147.90	201.0
149.80	128.0
154.90	252.0
156.90	213.0
160.90	141.0
170.90	388.0
171.90	1923.0
173.00	1246.0
173.90	96736.0
174.90	7502.0
175.90	93184.0
176.90	6426.0
177.90	190.0

Instrument :
MSVOA_U
ClientSampleId :
BFB173