

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071318\
 Data File : VU025387.D
 Acq On : 13 Jul 2018 12:26
 Operator : MD/SY
 Sample : J3937-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jul 13 14:44:09 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 13 14:43:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	292688	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	260447	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	114968	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	80707	46.13	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.26%
7) Chloroethane-d5	1.68	69	66352	45.98	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.96%
11) 1,1-Dichloroethene-d2	2.27	63	130268	34.13	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.26%
21) 2-Butanone-d5	4.18	46	141493	96.75	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.75%
24) Chloroform-d	4.65	84	172310	45.98	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.96%
26) 1,2-Dichloroethane-d4	5.31	65	125254	47.14	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.28%
32) Benzene-d6	5.35	84	341130	47.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.48%
36) 1,2-Dichloropropane-d6	6.33	67	109757	48.22	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.44%
41) Toluene-d8	7.57	98	328468	46.98	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.96%
43) trans-1,3-Dichloropropene-	7.85	79	48801	42.76	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.52%
47) 2-Hexanone-d5	8.31	63	102303	98.48	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	98.48%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	145808	45.21	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.42%
64) 1,2-Dichlorobenzene-d4	11.86	152	123878	49.45	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.90%

Target Compounds


					Ovalue
13) Acetone	2.32	43	4678	3.112 ug/L	85
15) Methyl Acetate	2.62	43	2864	1.245 ug/L #	65
37) 1,2-Dichloropropane	6.34	63	12944	6.137 ug/L #	88
48) 2-Hexanone	8.31	43	13404	5.544 ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU071318\
Data File : VU025387.D
Acq On : 13 Jul 2018 12:26
Operator : MD/SY
Sample : J3937-04
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jul 13 14:44:09 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 13 14:43:42 2018
Response via : Initial Calibration

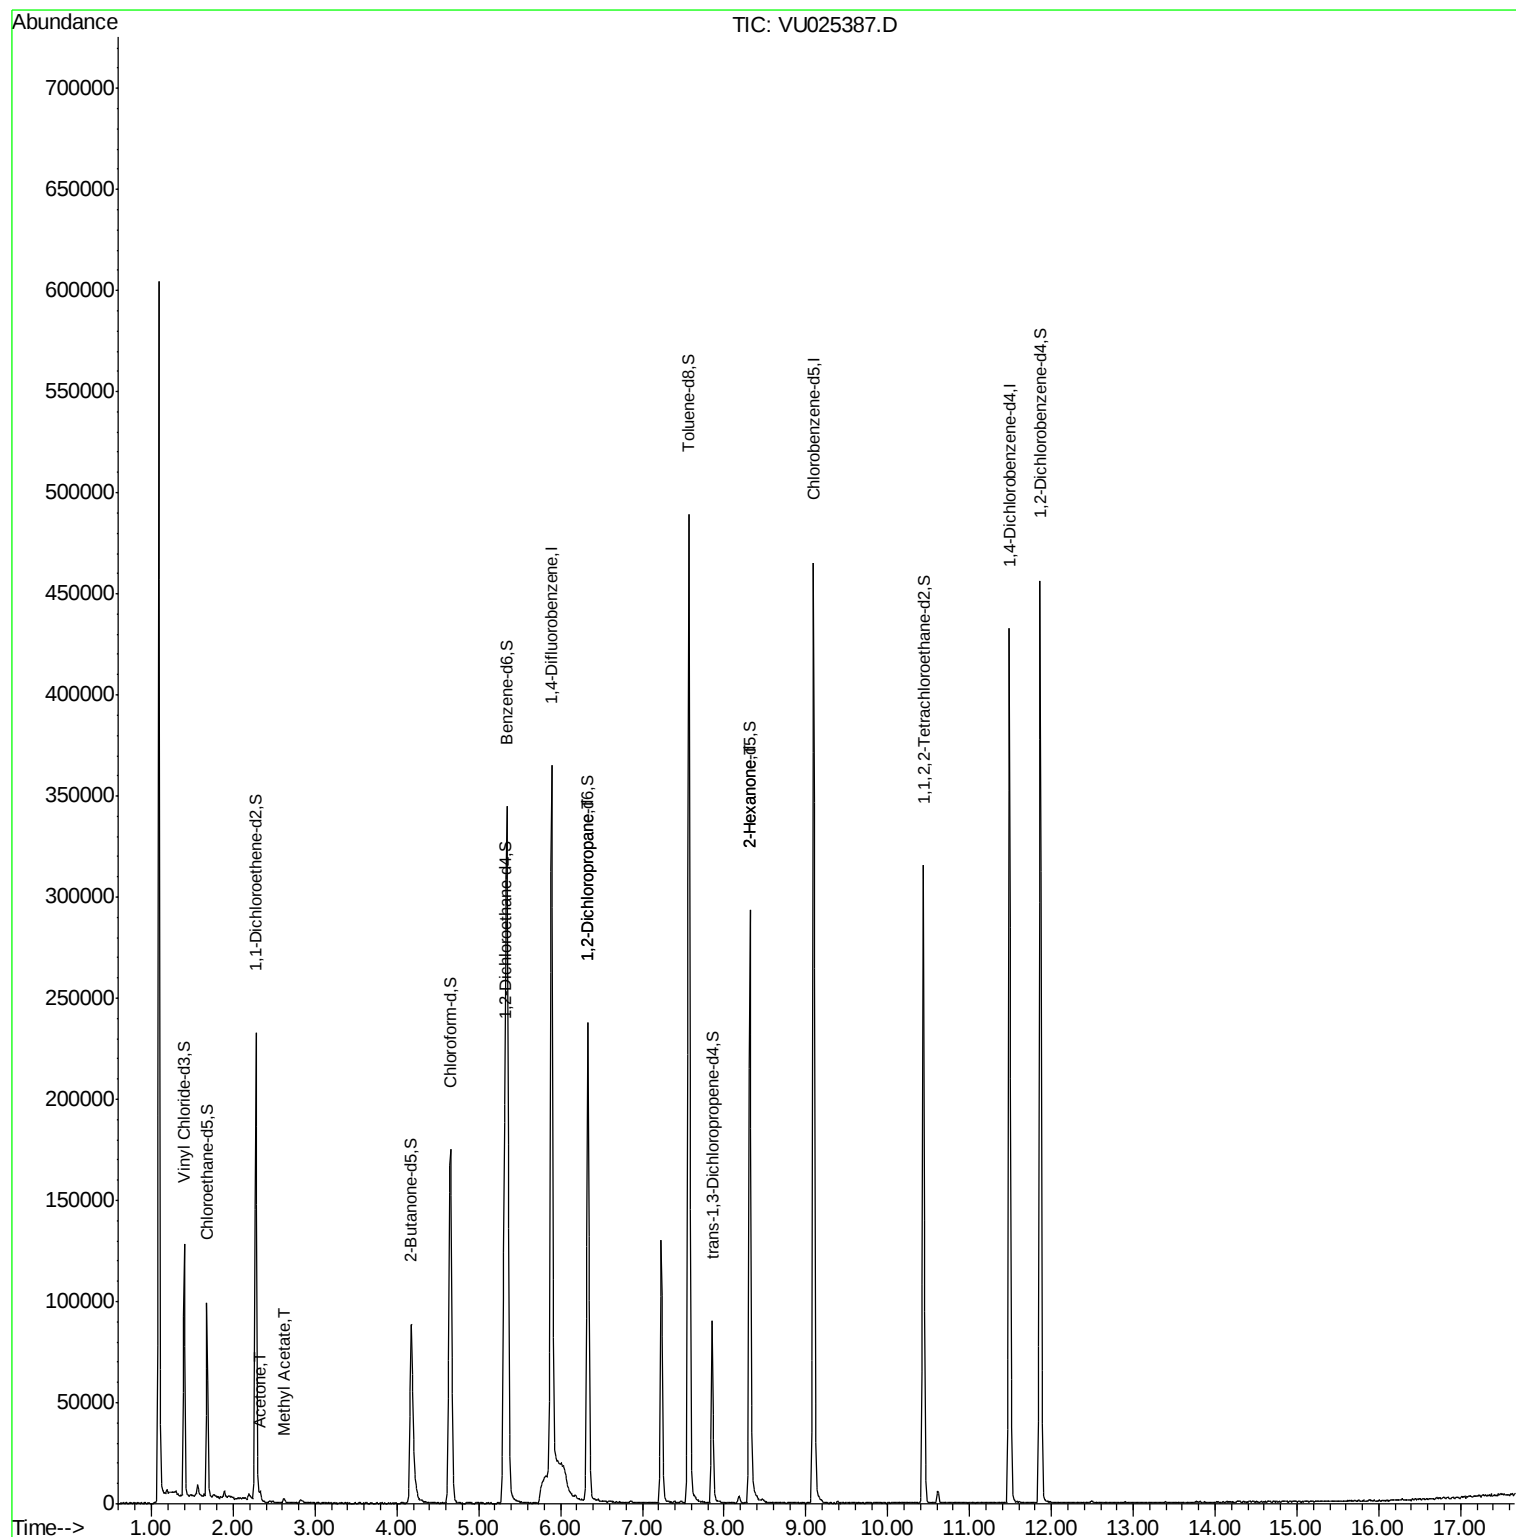

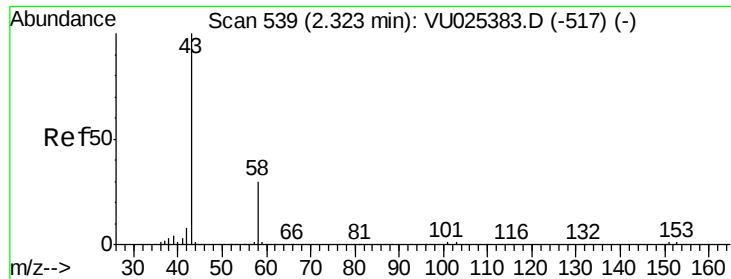

#13

Acetone

Concen: 3.112 ug/L

RT: 2.32 min Scan# 538

Delta R.T. -0.00 min

Lab File: VU025387.D

Acq: 13 Jul 2018 12:26

Instrument :

MSVOA_U


ClientSampled :

Tot Ion: 43 Resp: 4678

Ion Ratio Lower Upper




43 100

58 21.4 0.0 59.4

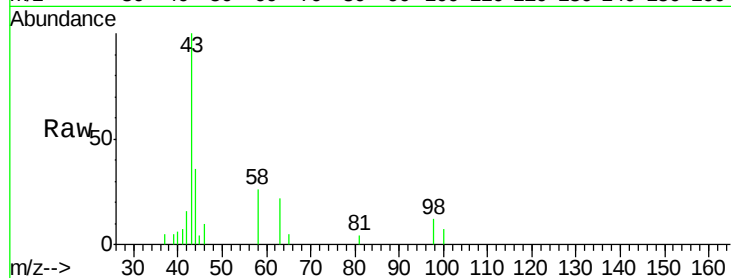

Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0

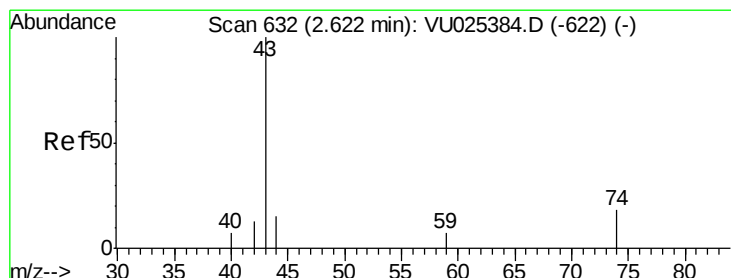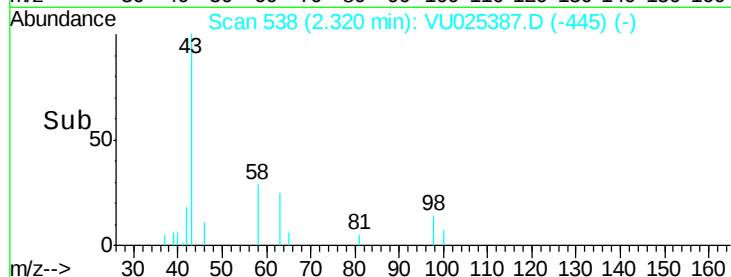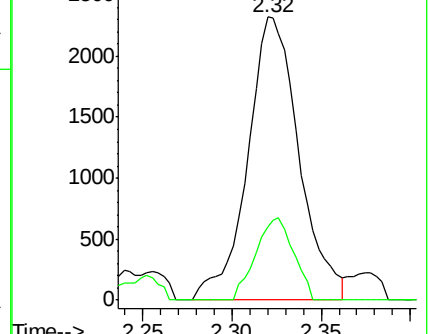

#15

Methyl Acetate

Concen: 1.245 ug/L

RT: 2.62 min Scan# 631

Delta R.T. 0.00 min

Lab File: VU025387.D


Acq: 13 Jul 2018 12:26

Tgt Ion: 43 Resp: 2864

Ion Ratio Lower Upper



43 100


74 6.4 18.6 28.0#

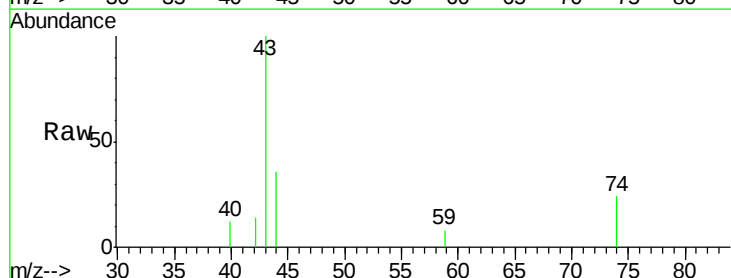

Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 74.00 (73.70 to 74.70): VU0



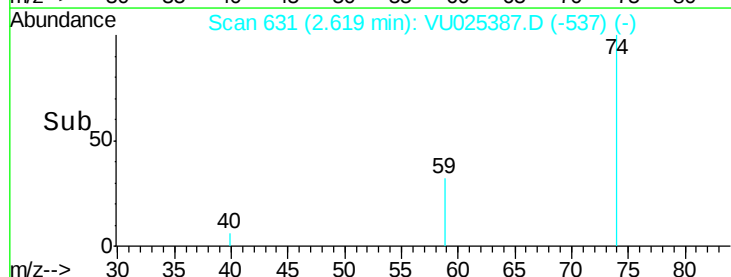
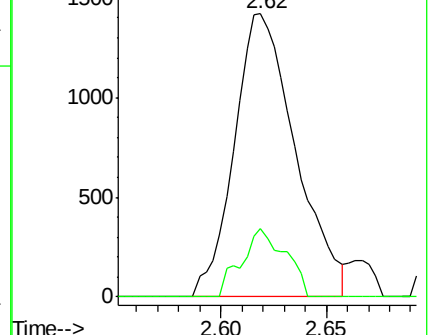


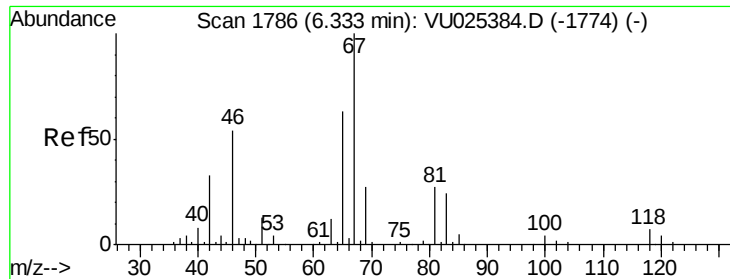

#37
 1,2-Dichloropropane
 Concen: 6.137 ug/L
 RT: 6.34 min Scan# 1787
 Delta R.T. -0.10 min
 Lab File: VU025387.D
 Acq: 13 Jul 2018 12:26

Instrument :
 MSVOA_U
 ClientSampleId :

Tot Ion: 63 Resp: 12944
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.2 4.8#

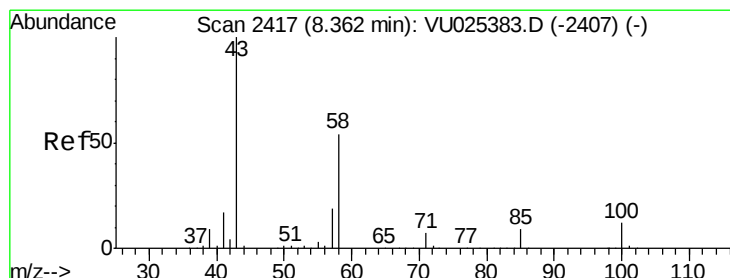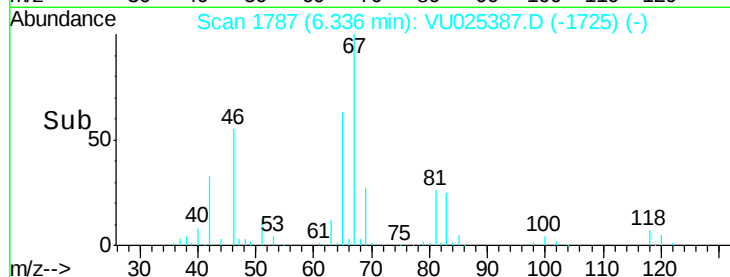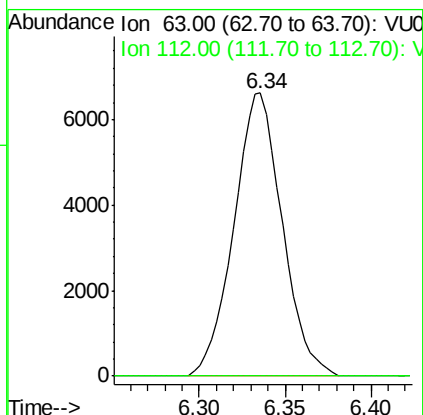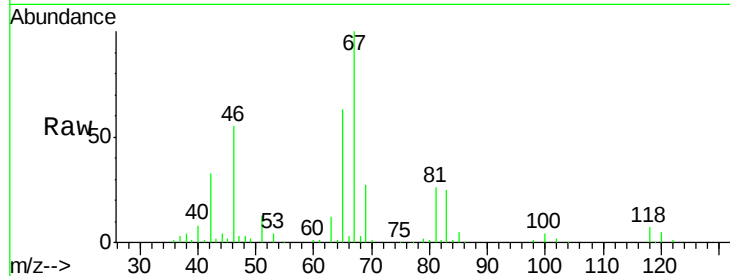

#48
 2-Hexanone
 Concen: 5.544 ug/L
 RT: 8.31 min Scan# 2402
 Delta R.T. -0.05 min
 Lab File: VU025387.D
 Acq: 13 Jul 2018 12:26

Tgt Ion: 43 Resp: 13404
 Ion Ratio Lower Upper
 43 100
 58 22.3 43.2 64.8#
 57 20.1 15.8 23.8
 100 0.0 9.4 14.0#

