

Data File : VU025387.D
Acq On : 13 Jul 2018 12:26
Operator : MD/SY
Sample : J3937-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEMG2

Manual Integrations
APPROVED

sam
7/16/2018 2:15:50 PM

Quant Time: Jul 13 15:01:44 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 13 14:43:42 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	292688	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	260447	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	114968	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	80707	46.13	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.26%
7) Chloroethane-d5	1.68	69	66352	45.98	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.96%
11) 1,1-Dichloroethene-d2	2.27	63	130268	34.13	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.26%
21) 2-Butanone-d5	4.18	46	141493	96.75	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.75%
24) Chloroform-d	4.65	84	172310	45.98	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.96%
26) 1,2-Dichloroethane-d4	5.31	65	125254	47.14	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.28%
32) Benzene-d6	5.35	84	341130	47.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.48%
36) 1,2-Dichloropropane-d6	6.33	67	109757	48.22	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.44%
41) Toluene-d8	7.57	98	328468	46.98	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.96%
43) trans-1,3-Dichloropropene-	7.85	79	48801	42.76	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.52%
47) 2-Hexanone-d5	8.31	63	102303	98.48	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	98.48%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	145808	45.21	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.42%
64) 1,2-Dichlorobenzene-d4	11.86	152	123878	49.45	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.90%

Target Compounds					Qvalue
13) Acetone	2.32	43	4944m	3.289	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data File : VU025387.D
Acq On : 13 Jul 2018 12:26
Operator : MD/SY
Sample : J3937-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
BEMG2

Manual Integrations
APPROVED

sam
7/16/2018 2:15:50 PM

Quant Time: Jul 13 15:01:44 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 13 14:43:42 2018
Response via : Initial Calibration

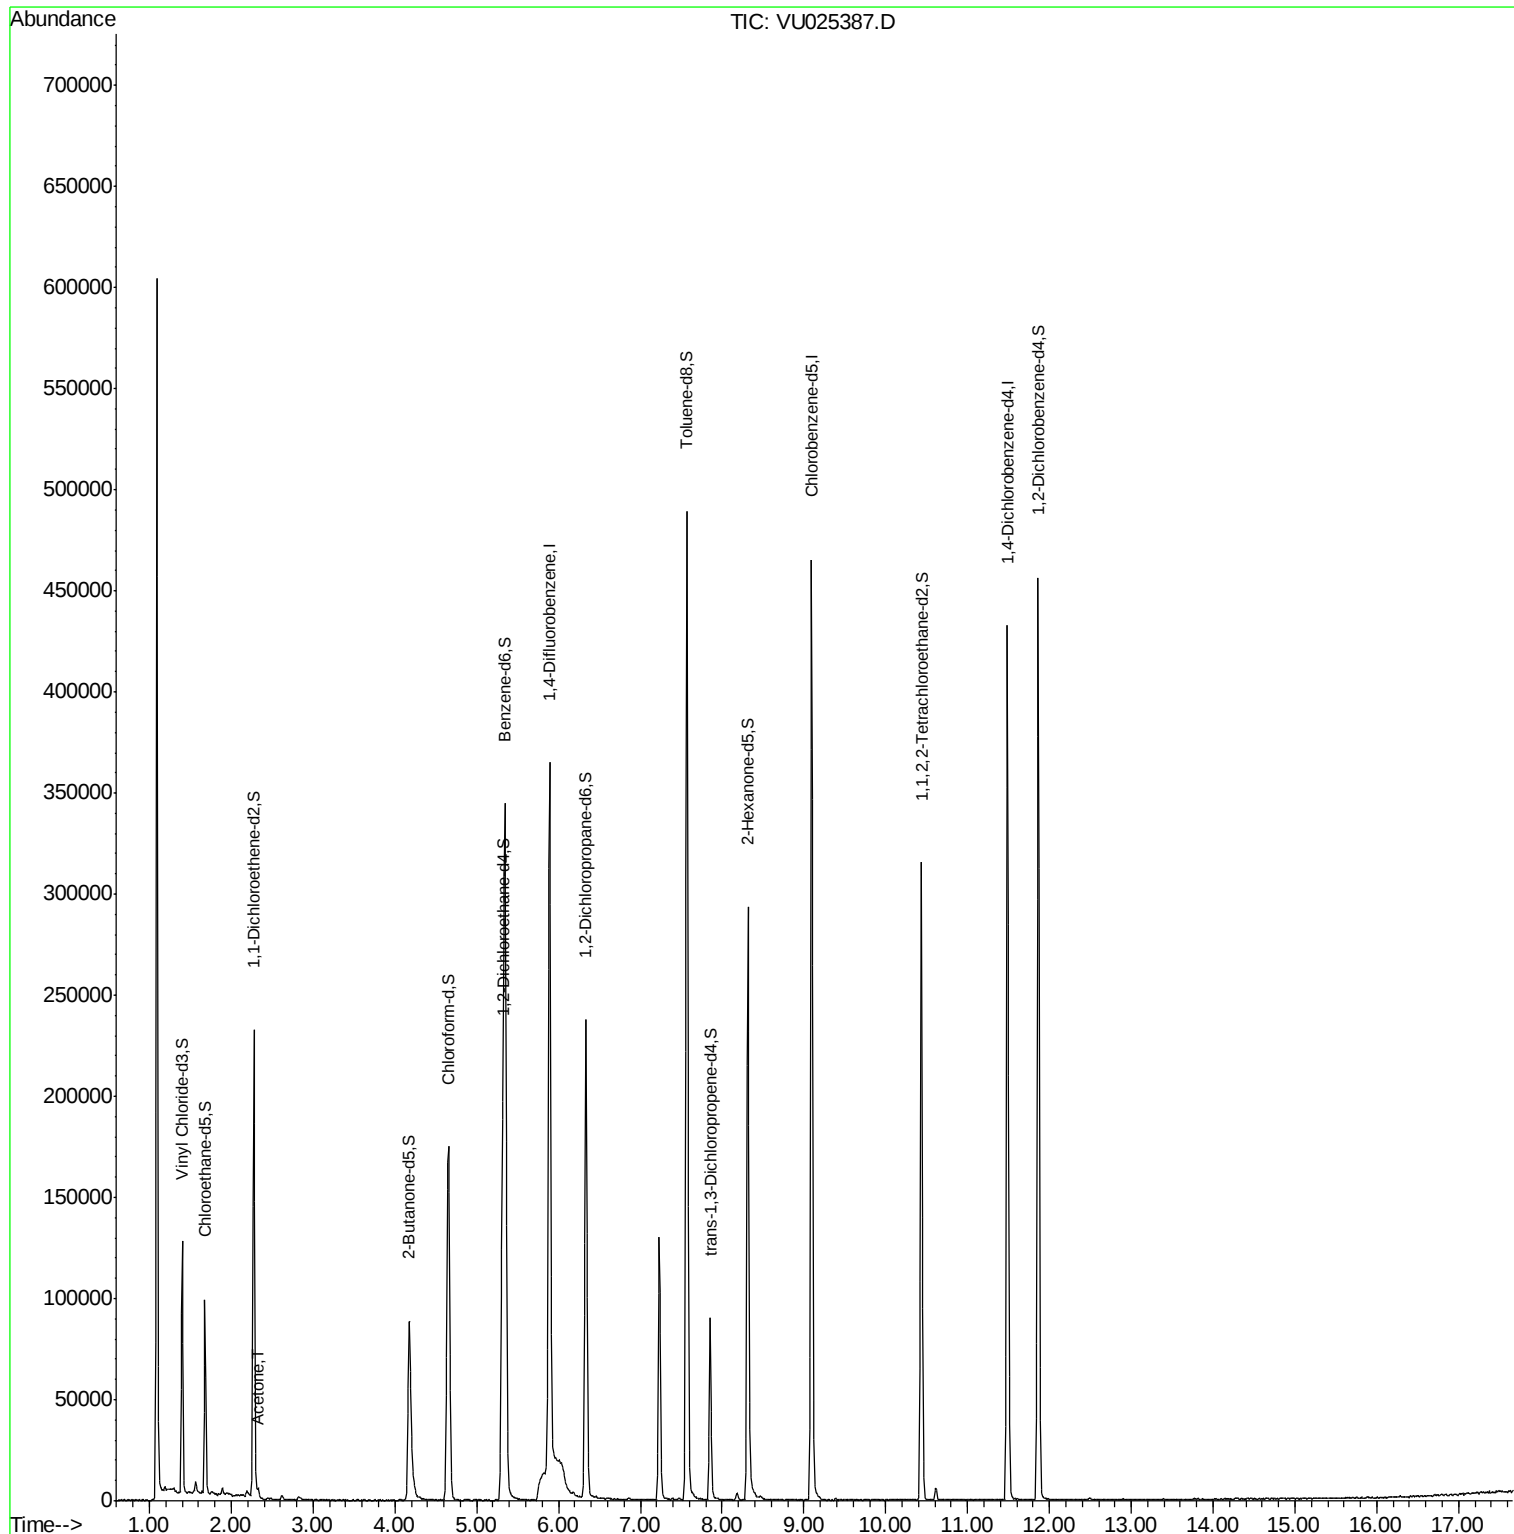

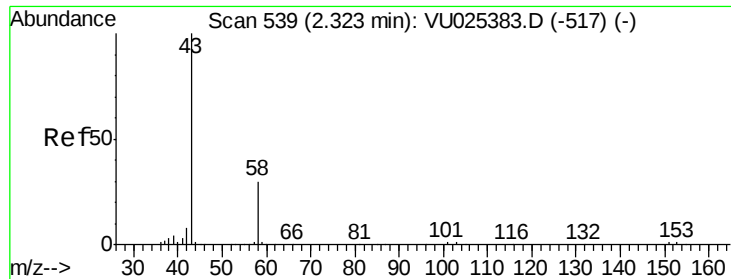

#13

Acetone

Concen: 3.289 ug/L m

RT: 2.32 min Scan# 538

Delta R.T. -0.00 min

Lab File: VU025387.D

Acq: 13 Jul 2018 12:26

Instrument :

MSVOA_U

ClientSampleId :

BEMG2

Tgt Ion: 43 Resp: 4944

Ion Ratio Lower Upper

43 100

58 20.3 0.0 59.4

Manual Integrations

APPROVED

sam

7/16/2018 2:15:50 PM

