

Data File : VU025397.D
Acq On : 13 Jul 2018 17:29
Operator : MD/SY
Sample : J3984-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB177

Quant Time: Jul 13 19:07:19 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 13 14:43:42 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	329809	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	298956	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	144566	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	83454	42.33	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.66%
7) Chloroethane-d5	1.68	69	69365	42.66	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.32%
11) 1,1-Dichloroethene-d2	2.27	63	137784	32.04	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.08%
21) 2-Butanone-d5	4.18	46	160566	97.43	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.43%
24) Chloroform-d	4.65	84	181659	43.02	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.04%
26) 1,2-Dichloroethane-d4	5.31	65	129793	43.35	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.70%
32) Benzene-d6	5.35	84	353903	43.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.30%
36) 1,2-Dichloropropane-d6	6.33	67	114369	43.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	87.56%
41) Toluene-d8	7.57	98	339267	42.27	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.54%
43) trans-1,3-Dichloropropene-	7.85	79	50817	38.79	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.58%
47) 2-Hexanone-d5	8.31	63	122076	102.38	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	102.38%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	162557	43.91	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.82%
64) 1,2-Dichlorobenzene-d4	11.86	152	138487	43.96	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.92%

Target Compounds


						Qvalue
3) Chloromethane	1.33	50	4679	1.893	ug/L	99
5) Vinyl chloride	1.40	62	31787	12.427	ug/L	89
13) Acetone	2.32	43	14604	8.622	ug/L	99
17) trans-1,2-Dichloroethene	3.00	96	59405	27.122	ug/L	97
20) cis-1,2-Dichloroethene	4.23	96	5874371	2322.261	ug/L	97
34) Trichloroethene	6.19	95	78710	32.635	ug/L	99
46) Tetrachloroethene	8.23	164	191685	93.890	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU025397.D
Acq On : 13 Jul 2018 17:29
Operator : MD/SY
Sample : J3984-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB177

Quant Time: Jul 13 19:07:19 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 13 14:43:42 2018
Response via : Initial Calibration

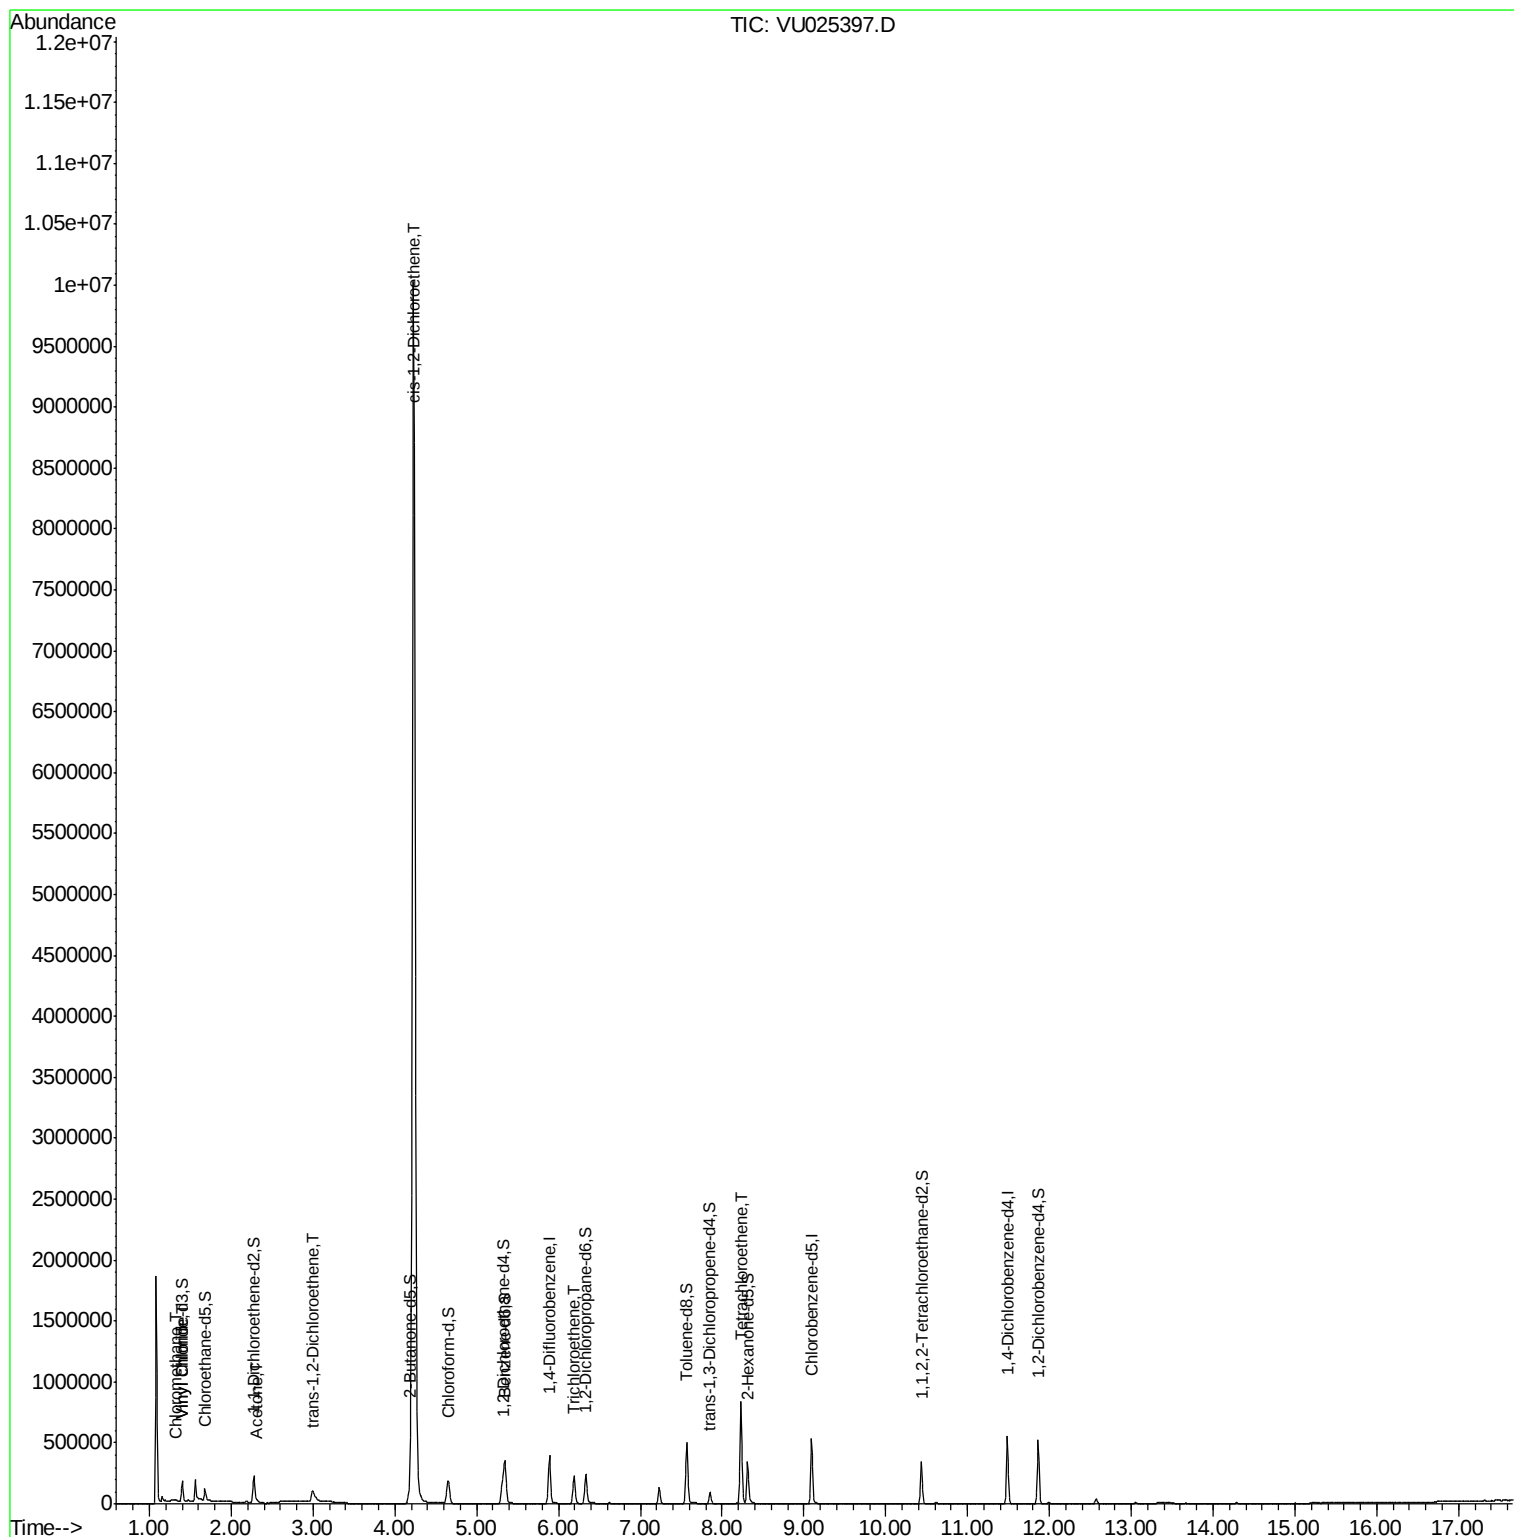

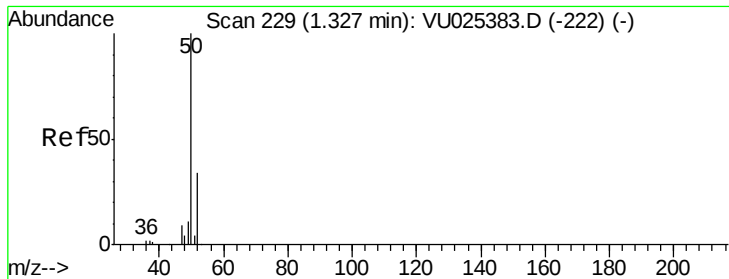

#3

Chloromethane

Concen: 1.893 ug/L

RT: 1.33 min Scan# 230

Delta R.T. 0.00 min

Lab File: VU025397.D

Acq: 13 Jul 2018 17:29

Instrument :

MSVOA_U

ClientSampleId :


DB177

Tgt Ion: 50 Resp: 4679

Ion Ratio Lower Upper




50 100

52 32.3 23.1 42.9

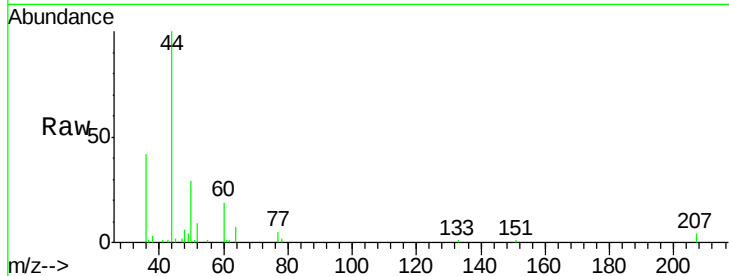

Abundance Ion 50.00 (49.70 to 50.70): VU0

Ion 52.00 (51.70 to 52.70): VU0

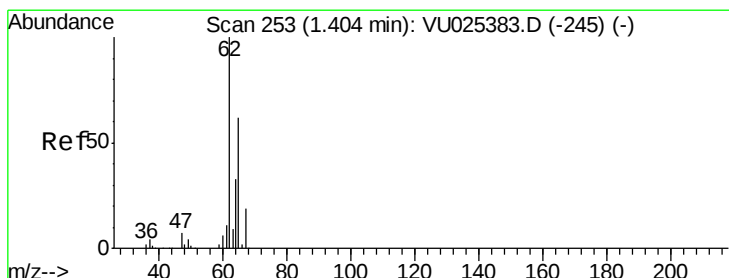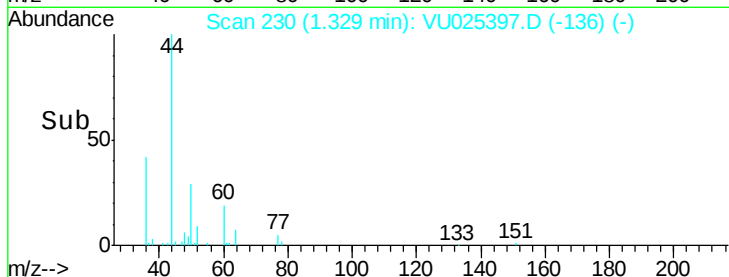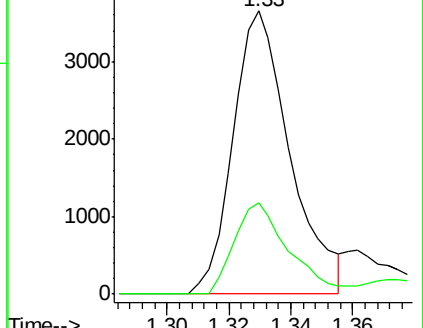

#5

Vinyl chloride

Concen: 12.427 ug/L

RT: 1.40 min Scan# 253

Delta R.T. -0.00 min

Lab File: VU025397.D


Acq: 13 Jul 2018 17:29

Tgt Ion: 62 Resp: 31787

Ion Ratio Lower Upper



62 100


64 39.0 23.0 42.8

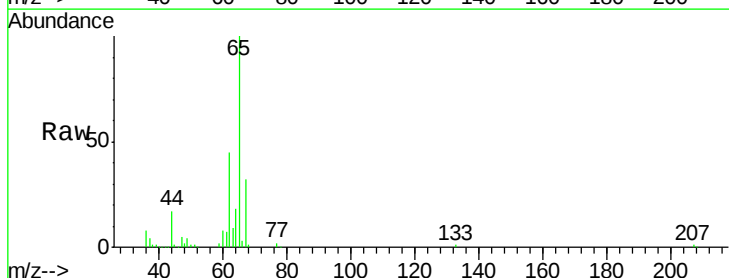

Abundance Ion 62.00 (61.70 to 62.70): VU0

Ion 64.00 (63.70 to 64.70): VU0

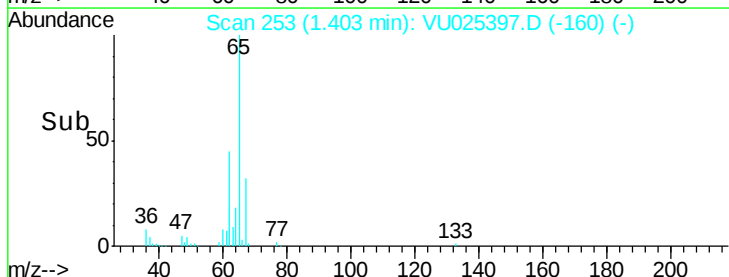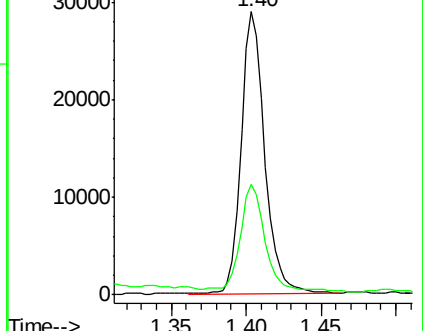

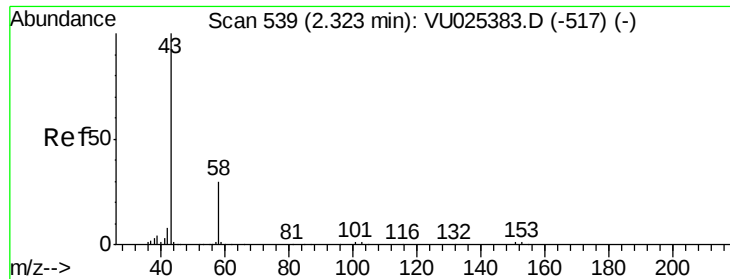

#13

Acetone

Concen: 8.622 ug/L

RT: 2.32 min Scan# 538

Delta R.T. -0.00 min

Lab File: VU025397.D

Acq: 13 Jul 2018 17:29

Instrument :

MSVOA_U

ClientSampleId :


DB177

Tgt Ion: 43 Resp: 14604

Ion Ratio Lower Upper

43 100

58 30.1 0.0 59.4

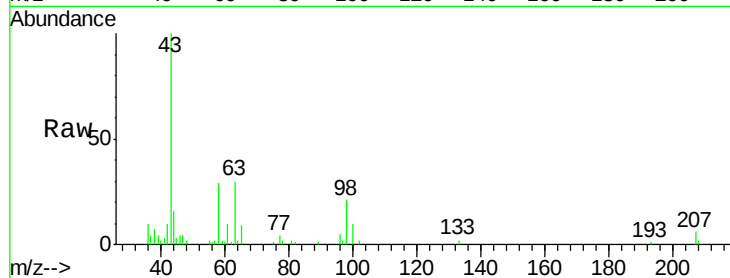

Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0

2.32

10000

8000



6000

4000

2000

0

Time--> 2.25 2.30 2.35

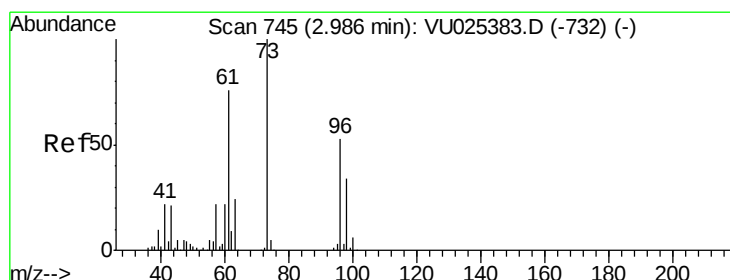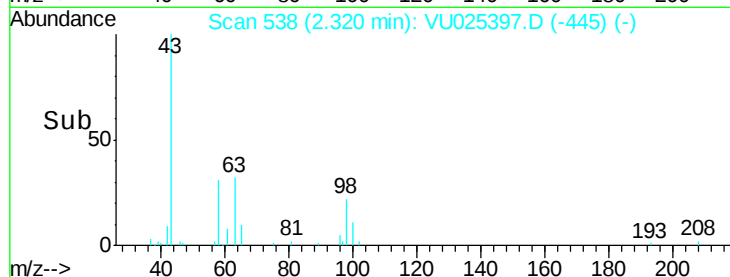

#17

trans-1,2-Dichloroethene

Concen: 27.122 ug/L

RT: 3.00 min Scan# 748

Delta R.T. 0.01 min

Lab File: VU025397.D

Acq: 13 Jul 2018 17:29


Tgt Ion: 96 Resp: 59405

Ion Ratio Lower Upper

96 100

61 143.2 102.7 190.7

98 61.7 44.4 82.5

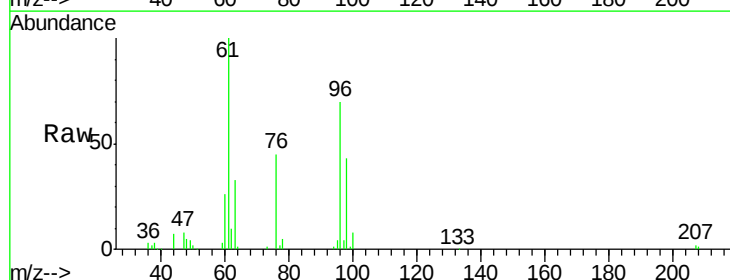

Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 61.00 (60.70 to 61.70): VU0

Ion 98.00 (97.70 to 98.70): VU0

3.00


30000


20000

10000

0

Time--> 2.90 3.00 3.10




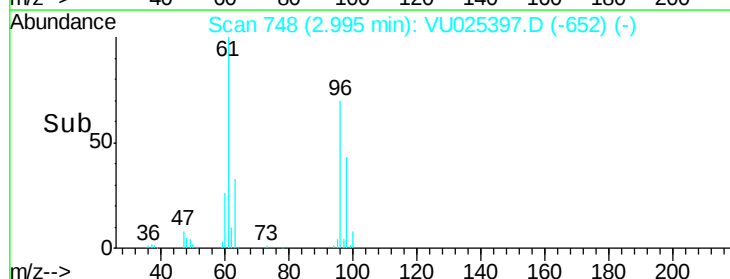


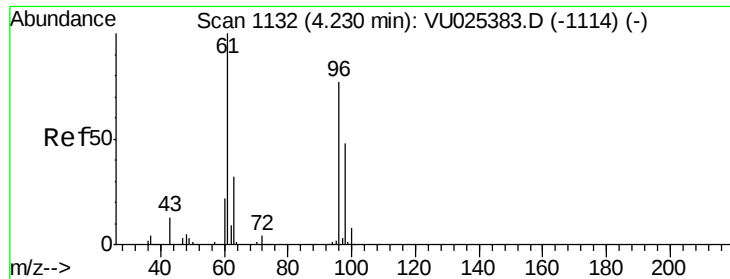

#20
 cis-1,2-Dichloroethene
 Concen: 2322.261 ug/L
 RT: 4.23 min Scan# 1132
 Delta R.T. 0.00 min
 Lab File: VU025397.D
 Acq: 13 Jul 2018 17:29




Instrument :
 MSVOA_U
 ClientSampleId :
 DB177


Tgt Ion: 96 Resp: 5874371
 Ion Ratio Lower Upper
 96 100
 61 130.4 93.4 173.6
 68 0.0 0.0 0.0

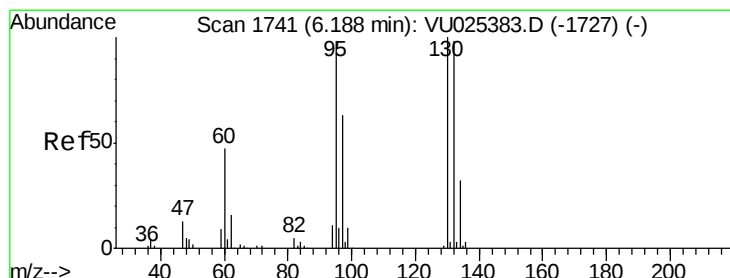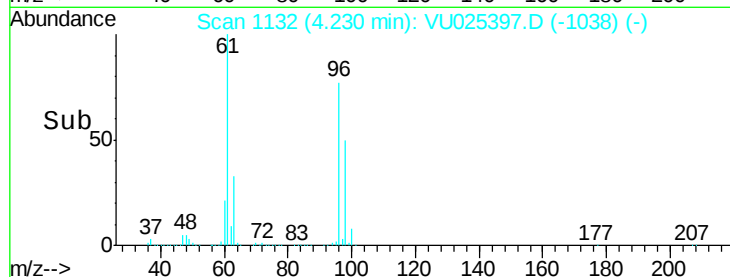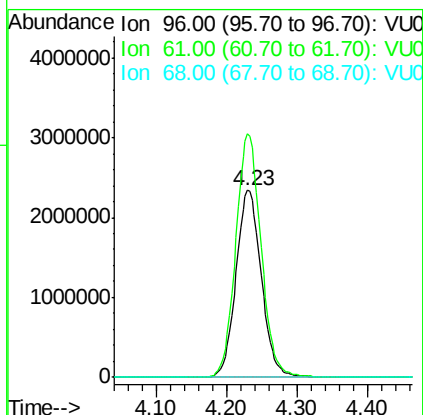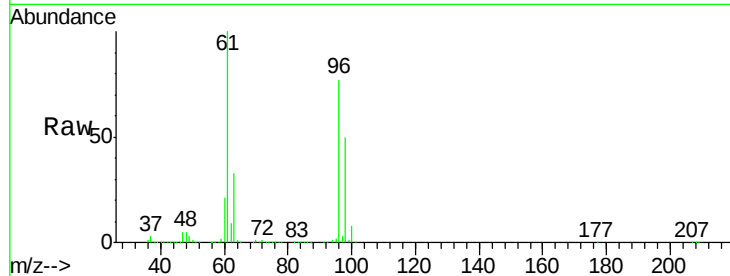

#34
 Trichloroethene
 Concen: 32.635 ug/L
 RT: 6.19 min Scan# 1741
 Delta R.T. -0.00 min
 Lab File: VU025397.D
 Acq: 13 Jul 2018 17:29

Tgt Ion: 95 Resp: 78710
 Ion Ratio Lower Upper
 95 100
 97 62.3 44.1 81.9
 132 101.3 70.2 130.4
 130 100.4 71.7 133.1

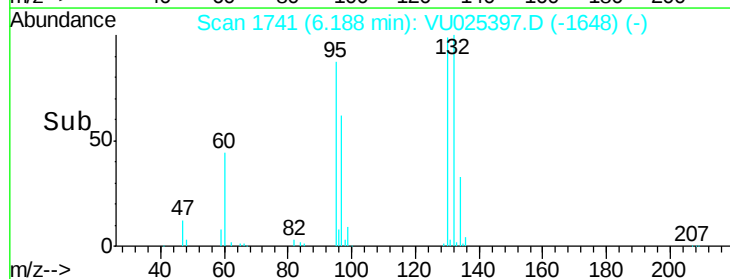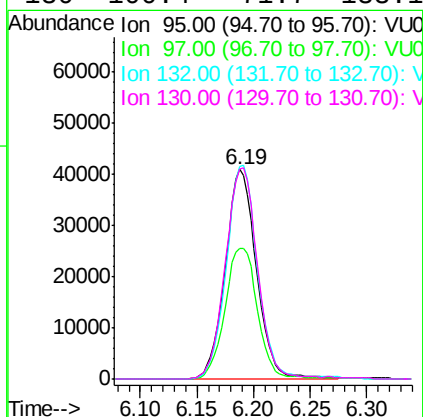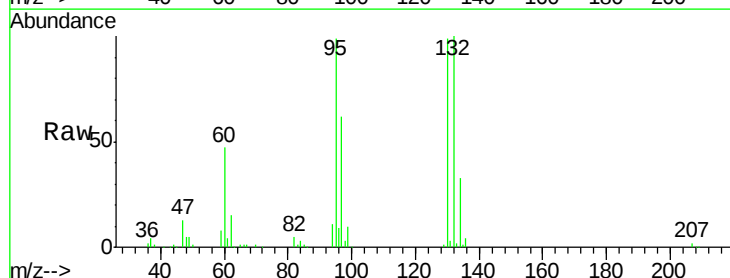

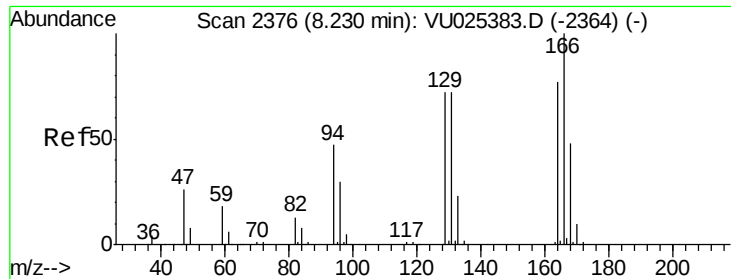

#46

Tetrachloroethene

Concen: 93.890 ug/L

RT: 8.23 min Scan# 2376

Delta R.T. -0.00 min

Lab File: VU025397.D

Acq: 13 Jul 2018 17:29

Instrument :
MSVOA_U
ClientSampleId :
DB177

Tgt Ion:164 Resp: 191685


Ion Ratio Lower Upper

164 100

129 95.1 66.1 122.8

131 91.7 62.7 116.5

166 127.2 88.8 165.0

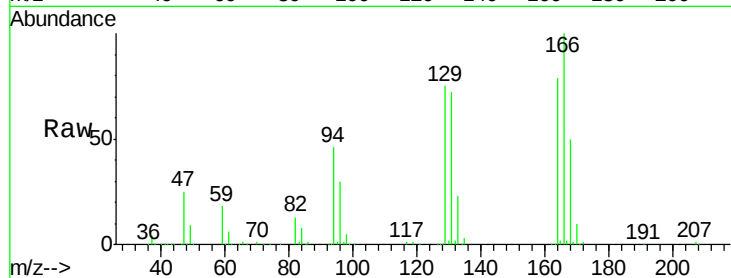

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

