

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU071318\
 Data File : VU025386.D
 Acq On : 13 Jul 2018 12:02
 Operator : MD/SY
 Sample : J3937-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEMG1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.645	14	17	20	rBV	192	104	0.01%	0.001%
2	0.674	24	26	28	rBV	159	100	0.01%	0.001%
3	0.725	39	42	45	rBV	140	95	0.01%	0.001%
4	0.761	52	53	54	rBV	124	33	0.00%	0.000%
5	0.793	59	63	64	rBV	226	164	0.02%	0.002%
6	0.876	88	89	93	rVB	99	39	0.00%	0.000%
7	0.896	93	95	97	rVB	196	102	0.01%	0.001%
8	0.912	97	100	103	rBV2	310	269	0.03%	0.003%
9	0.976	118	120	122	rBV	145	92	0.01%	0.001%
10	1.027	134	136	137	rBV	103	35	0.00%	0.000%
11	1.088	147	155	177	rBV	713164	826983	77.48%	9.327%
12	1.400	245	252	266	rVB	122496	134304	12.58%	1.515%
13	1.680	332	339	350	rVB	99461	123226	11.55%	1.390%
14	2.275	514	524	537	rBV	241291	363985	34.10%	4.105%
15	2.442	573	576	580	rBV2	550	472	0.04%	0.005%
16	2.619	621	631	644	rBV2	2778	4968	0.47%	0.0056%
17	2.703	652	657	663	rBV3	942	1141	0.11%	0.0013%
18	2.902	717	719	723	rVB	301	179	0.02%	0.0002%
19	2.921	723	725	730	rVV	135	90	0.01%	0.0001%
20	2.944	730	732	734	rVB	291	113	0.01%	0.0001%
21	2.982	741	744	746	rBV3	528	380	0.04%	0.0004%
22	3.079	767	774	775	rBV2	303	340	0.03%	0.0004%
23	3.204	812	813	816	rVB	235	99	0.01%	0.0001%
24	3.223	816	819	823	rBV	333	218	0.02%	0.0002%
25	3.275	833	835	838	rVB	254	105	0.01%	0.0001%
26	3.313	844	847	849	rBV2	372	193	0.02%	0.0002%
27	3.358	858	861	863	rBV	170	101	0.01%	0.0001%
28	3.394	867	872	878	rBV2	432	566	0.05%	0.0006%
29	3.445	885	888	891	rVB2	215	135	0.01%	0.0002%
30	3.500	901	905	906	rBV	172	107	0.01%	0.0001%
31	3.532	913	915	916	rBV	172	56	0.01%	0.0001%
32	3.580	928	930	932	rBV	137	81	0.01%	0.0001%
33	3.609	936	939	942	rVB	230	137	0.01%	0.0002%
34	3.658	951	954	955	rBV	189	113	0.01%	0.0001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU071318\
 Data File : VU025386.D
 Acq On : 13 Jul 2018 12:02
 Operator : MD/SY
 Sample : J3937-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEMG1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
 Title : VOC Analysis

35	3.841	1010	1011	1015	rBV	127	65	0.01%	0.001%
36	3.912	1030	1033	1036	rVB	176	84	0.01%	0.001%
37	3.950	1042	1045	1048	rBV2	282	183	0.02%	0.002%
38	4.066	1079	1081	1082	rBV2	134	35	0.00%	0.000%
39	4.108	1091	1094	1100	rBV	102	119	0.01%	0.001%
40	4.178	1100	1116	1127	rBV	87620	227338	21.30%	2.564%
41	4.458	1201	1203	1205	rBV	322	156	0.01%	0.002%
42	4.494	1209	1214	1217	rBV2	423	347	0.03%	0.004%
43	4.513	1217	1220	1222	rVB2	317	185	0.02%	0.002%
44	4.555	1231	1233	1238	rBV	140	57	0.01%	0.001%
45	4.580	1239	1241	1246	rVV	200	106	0.01%	0.001%
46	4.651	1246	1263	1293	rBV	179967	420944	39.44%	4.748%
47	4.799	1307	1309	1311	rBV	298	161	0.02%	0.002%
48	4.854	1323	1326	1329	rBV2	285	201	0.02%	0.002%
49	4.886	1329	1336	1351	rVV2	1074	2488	0.23%	0.028%
50	4.985	1362	1367	1368	rBV	564	478	0.04%	0.005%
51	5.079	1393	1396	1398	rBV	313	181	0.02%	0.002%
52	5.153	1415	1419	1423	rVB2	206	184	0.02%	0.002%
53	5.172	1423	1425	1426	rBV	125	48	0.00%	0.001%
54	5.346	1453	1479	1516	rBV2	355551	1067318	100.00%	12.038%
55	5.641	1568	1571	1576	rVB	407	294	0.03%	0.003%
56	5.674	1576	1581	1586	rBV2	295	396	0.04%	0.004%
57	5.802	1601	1621	1623	rBV4	10090	27816	2.61%	0.314%
58	5.889	1639	1648	1666	rVB	345142	653531	61.23%	7.371%
59	6.333	1773	1786	1809	rVB	236783	471529	44.18%	5.318%
60	7.014	1994	1998	2000	rBV2	472	383	0.04%	0.004%
61	7.082	2016	2019	2022	rBV2	239	175	0.02%	0.002%
62	7.165	2044	2045	2048	rVB	207	87	0.01%	0.001%
63	7.230	2053	2065	2082	rBV	133179	237234	22.23%	2.676%
64	7.333	2095	2097	2099	rBV	569	261	0.02%	0.003%
65	7.378	2107	2111	2112	rBV2	665	389	0.04%	0.004%
66	7.439	2127	2130	2132	rBV	417	203	0.02%	0.002%
67	7.468	2134	2139	2141	rBV4	1172	1086	0.10%	0.012%
68	7.503	2148	2150	2154	rBV2	366	198	0.02%	0.002%
69	7.567	2157	2170	2189	rBV	499850	867746	81.30%	9.787%
70	7.854	2248	2259	2275	rBV	90751	152996	14.33%	1.726%
71	8.043	2315	2318	2320	rBV	307	170	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU071318\
 Data File : VU025386.D
 Acq On : 13 Jul 2018 12:02
 Operator : MD/SY
 Sample : J3937-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEMG1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
 Title : VOC Analysis

72	8.124	2341	2343	2347	rBV	311	120	0.01%	0.001%
73	8.143	2347	2349	2351	rVV2	368	222	0.02%	0.003%
74	8.181	2354	2361	2372	rVB3	4697	8653	0.81%	0.098%
75	8.230	2372	2376	2377	rBV	134	102	0.01%	0.001%
76	8.239	2377	2379	2380	rBV	204	100	0.01%	0.001%
77	8.310	2390	2401	2432	rBV	292726	512865	48.05%	5.784%
78	8.606	2490	2493	2497	rBV	280	219	0.02%	0.002%
79	8.628	2498	2500	2504	rVB	334	167	0.02%	0.002%
80	8.648	2504	2506	2507	rBV	169	66	0.01%	0.001%
81	8.664	2507	2511	2513	rBV2	279	206	0.02%	0.002%
82	8.709	2522	2525	2528	rBV3	369	217	0.02%	0.002%
83	8.738	2531	2534	2535	rBV	103	59	0.01%	0.001%
84	8.892	2578	2582	2584	rBV	177	133	0.01%	0.002%
85	8.963	2602	2604	2605	rBV	266	128	0.01%	0.001%
86	9.091	2631	2644	2681	rBV	464809	779946	73.08%	8.797%
87	9.374	2727	2732	2735	rBV2	784	677	0.06%	0.008%
88	9.612	2804	2806	2809	rBV	222	107	0.01%	0.001%
89	10.175	2979	2981	2983	rBV	226	120	0.01%	0.001%
90	10.230	2996	2998	3000	rBV	123	59	0.01%	0.001%
91	10.435	3050	3062	3084	rVB	320147	514571	48.21%	5.804%
92	10.612	3108	3117	3127	rBV2	7067	11297	1.06%	0.127%
93	10.982	3229	3232	3238	rBV2	324	444	0.04%	0.005%
94	11.021	3243	3244	3245	rBV	415	81	0.01%	0.001%
95	11.037	3245	3249	3253	rBV	342	335	0.03%	0.004%
96	11.255	3315	3317	3319	rBV	230	138	0.01%	0.002%
97	11.487	3377	3389	3415	rVB	426467	688591	64.52%	7.766%
98	11.863	3493	3506	3529	rBV	468511	752482	70.50%	8.487%


Sum of corrected areas: 8866402

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071318\
Data File : VU025386.D
Acq On : 13 Jul 2018 12:02
Operator : MD/SY
Sample : J3937-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
BEMG1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

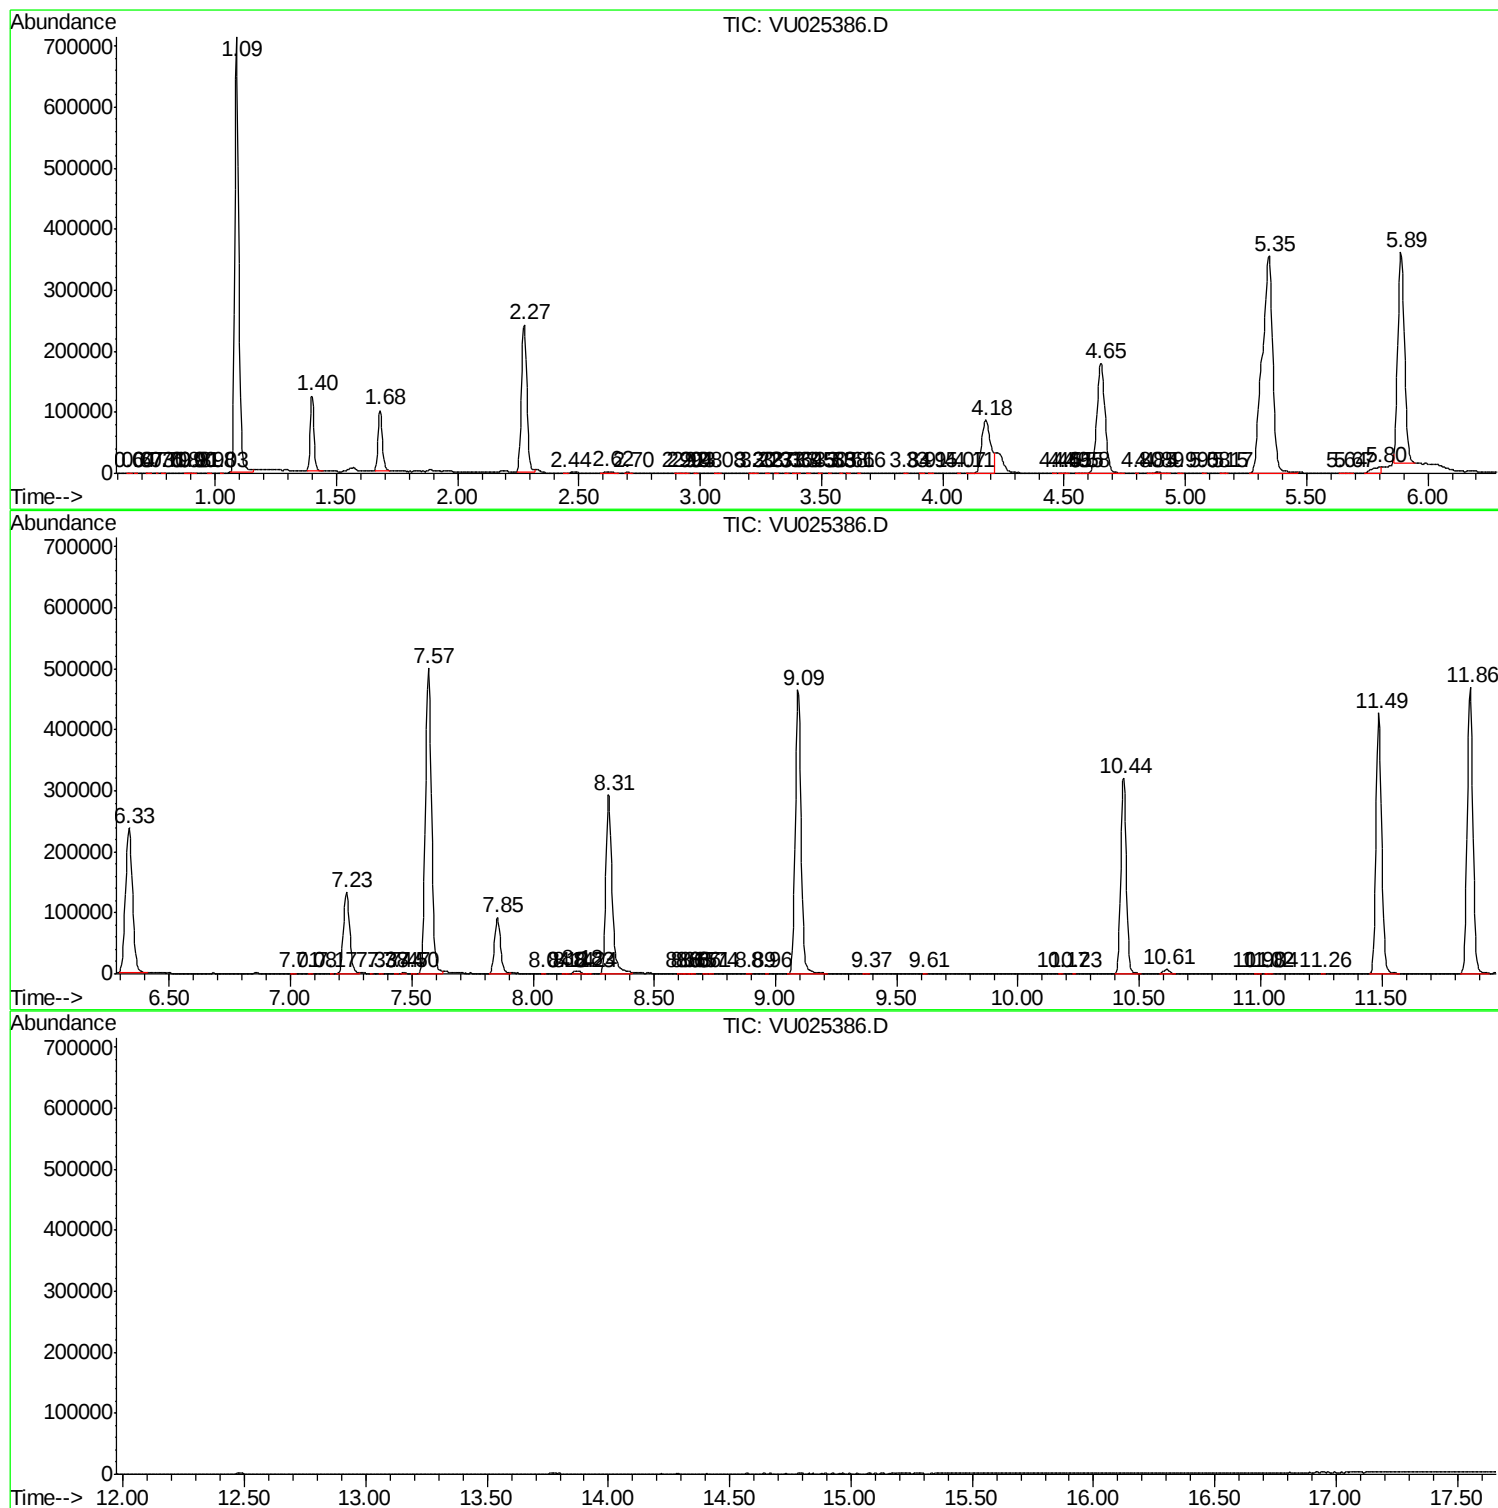

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071318\
Data File : VU025386.D
Acq On : 13 Jul 2018 12:02
Operator : MD/SY
Sample : J3937-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEMG1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071318\
Data File : VU025386.D
Acq On : 13 Jul 2018 12:02
Operator : MD/SY
Sample : J3937-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEMG1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc