


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU071318\
 Data File : VU025382.D
 Acq On : 13 Jul 2018 10:03
 Operator : MD/SY
 Sample : BFB42
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB42

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
 Title : VOC Analysis
 Last Update : Mon Jul 16 05:07:35 2018

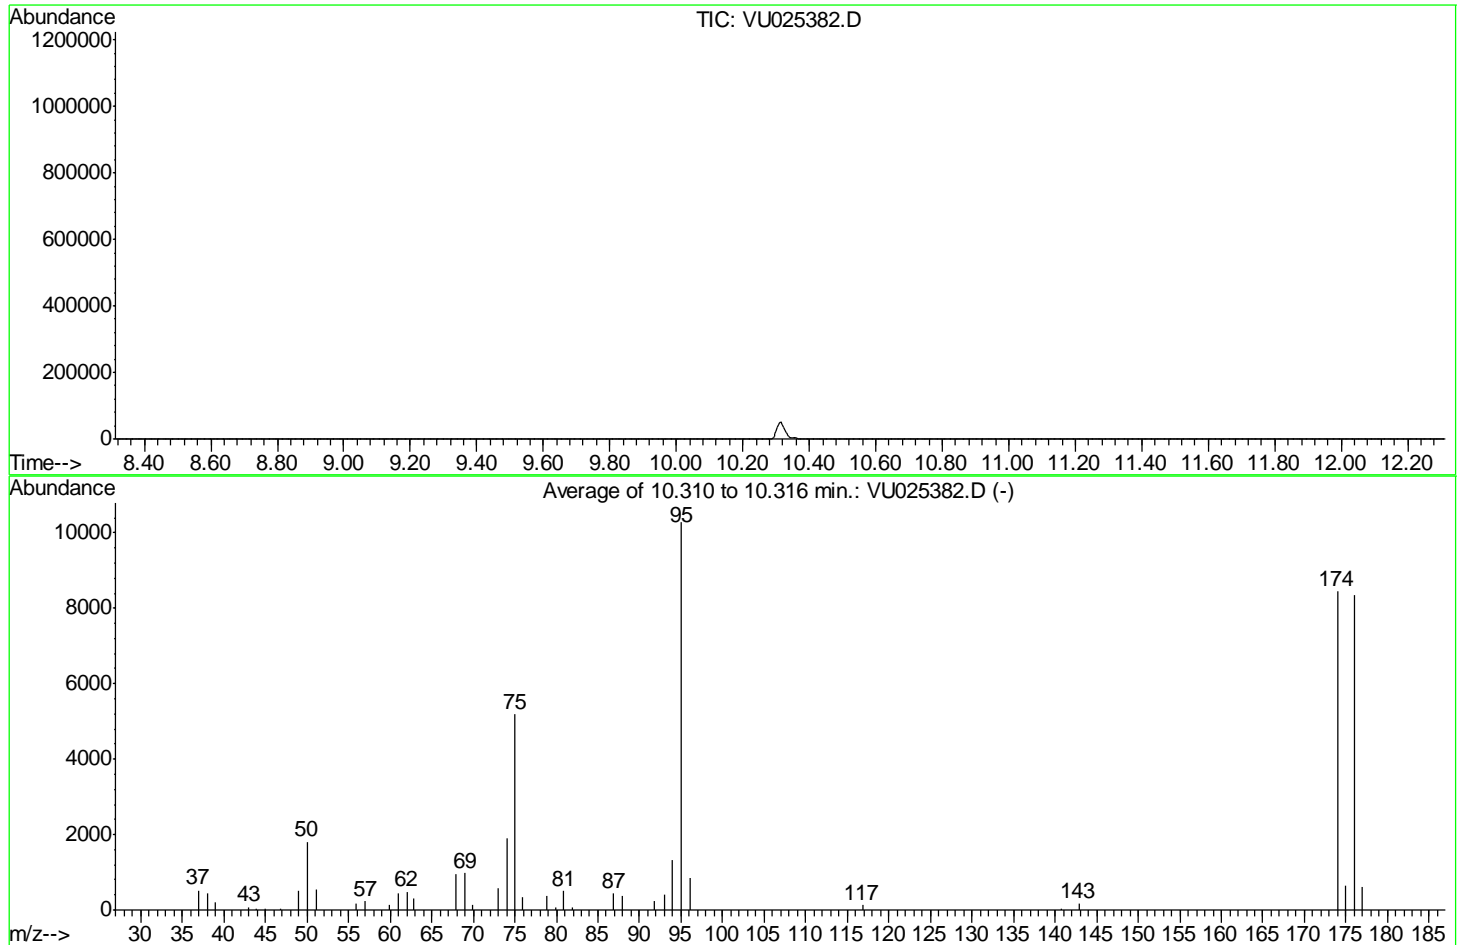

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3013

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	1815	PASS
75	95	30	80	50.5	5191	PASS
95	95	100	100	100.0	10279	PASS
96	95	5	9	8.4	862	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.1	8443	PASS
175	174	5	9	7.5	637	PASS
176	174	95	101	99.1	8364	PASS
177	176	5	9	7.3	609	PASS

m/z	Abundance
43.90	322.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
37.00	553.0
38.00	454.0
38.80	178.0
43.00	138.0
44.00	352.0
45.00	120.0
49.00	461.0
50.00	1736.0
51.10	530.0
55.90	148.0
57.10	249.0
60.00	153.0
61.00	395.0
62.00	460.0
62.90	290.0
68.00	912.0
69.00	960.0
69.90	147.0
73.00	616.0
74.00	1771.0
75.00	5240.0
75.90	387.0
78.80	353.0
80.90	439.0
81.90	107.0
86.90	449.0
87.90	447.0
91.90	192.0
93.00	376.0
94.00	1281.0
95.10	10228.0
96.00	887.0
116.90	109.0
140.80	104.0
142.80	134.0
174.00	8150.0
174.90	616.0
176.00	8173.0
176.90	521.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
37.00	557.0
38.00	458.0
38.90	215.0
43.00	117.0
44.00	363.0
46.80	121.0
49.00	508.0
50.00	1838.0
51.10	561.0
55.90	173.0
57.10	247.0
60.00	144.0
61.00	436.0
62.00	503.0
62.90	288.0
67.90	921.0
69.00	1014.0
70.00	138.0
73.00	574.0
74.00	1939.0
75.00	5310.0
75.90	331.0
78.80	374.0
79.90	104.0
80.90	534.0
81.80	106.0
86.90	452.0
87.90	357.0
91.80	255.0
92.90	425.0
94.00	1397.0
95.10	10711.0
96.10	918.0
116.90	148.0
142.80	179.0
173.90	8635.0
174.90	685.0
176.00	8658.0
176.90	625.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.90	441.0
38.00	402.0
39.00	247.0
44.00	383.0
49.00	527.0
50.00	1873.0
51.10	561.0
55.90	177.0
57.00	209.0
59.90	141.0
61.00	492.0
62.00	473.0
62.90	326.0
67.90	1002.0
69.00	957.0
70.00	126.0
73.00	561.0
74.00	1953.0
75.00	5023.0
75.90	299.0
78.80	361.0
79.90	139.0
80.90	535.0
86.90	423.0
87.80	298.0
91.80	274.0
92.90	400.0
94.00	1344.0
95.00	9899.0
96.10	782.0
116.80	142.0
142.90	196.0
174.00	8544.0
174.90	611.0
176.00	8261.0
177.00	682.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42