


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU071320\
Data File : VU039466.D
Acq On : 13 Jul 2020 11:57
Operator : SY/MD
Sample : BFB30
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB30

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Jul 14 07:08:13 2020

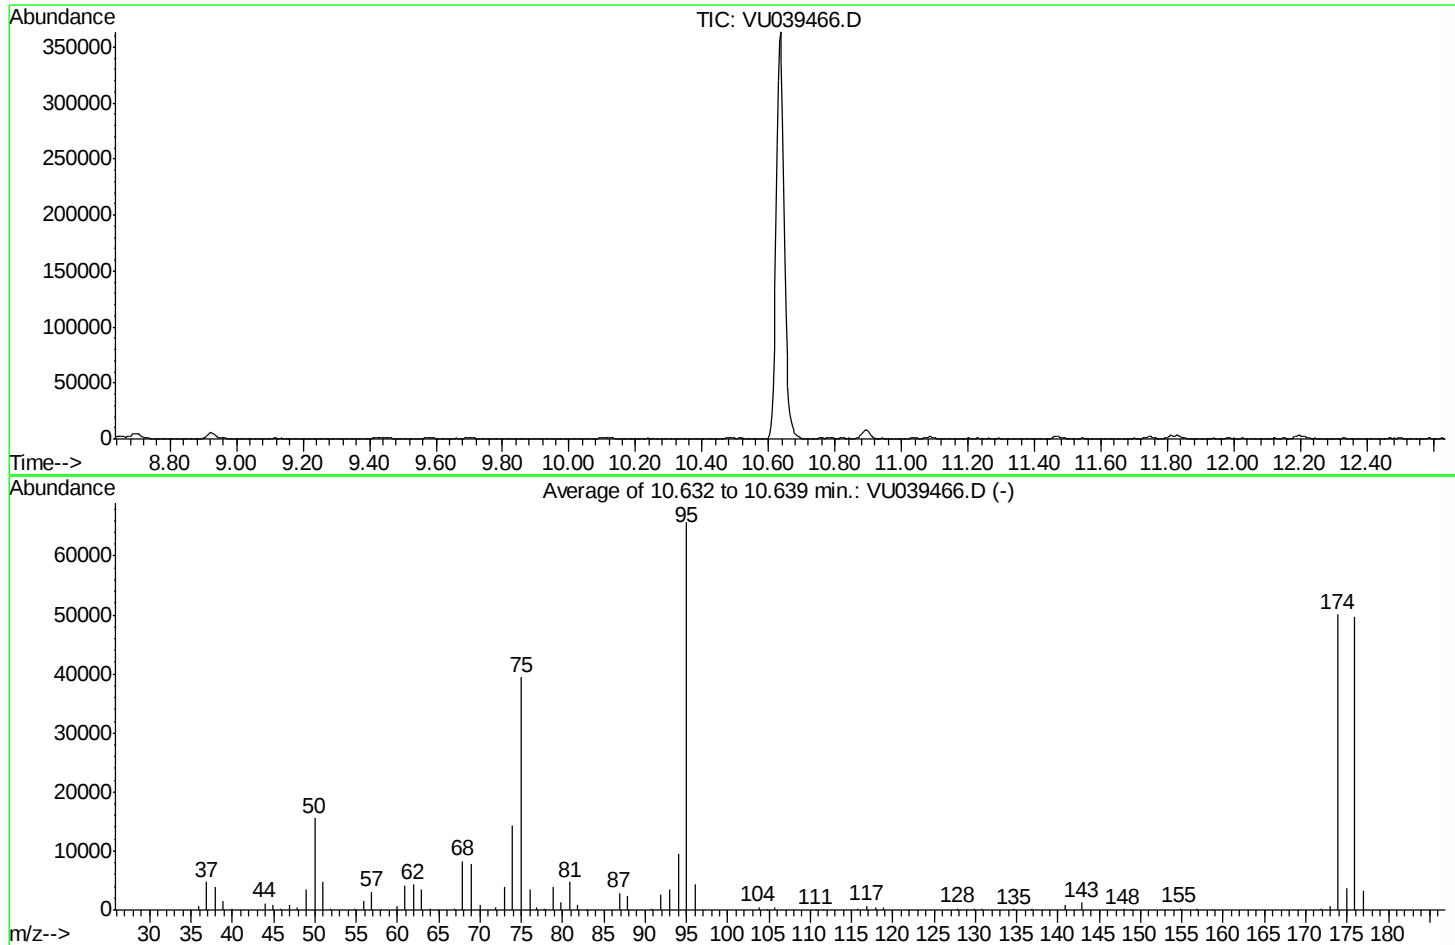

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	15555	PASS
75	95	30	80	60.0	39426	PASS
95	95	100	100	100.0	65704	PASS
96	95	5	9	6.8	4440	PASS
173	174	0.00	2	1.5	732	PASS
174	95	50	120	76.2	50085	PASS
175	174	5	9	7.4	3685	PASS
176	174	95	101	99.2	49682	PASS
177	176	5	9	6.5	3219	PASS

m/z	Abundance
35.90	753.0
36.90	4946.0
37.90	3945.0
38.90	1608.0
39.90	197.0
44.00	1005.0
44.90	1000.0
45.90	142.0
46.90	932.0
47.80	520.0
49.00	3578.0
50.00	15658.0
51.00	4908.0
51.90	206.0
55.00	237.0
56.00	1572.0
56.90	3098.0
60.00	718.0
60.90	4215.0
61.90	4141.0
62.90	3460.0
64.00	323.0
64.90	139.0
66.90	250.0
67.90	8586.0
69.00	8240.0
70.00	824.0
72.00	436.0
73.00	3981.0
73.90	14779.0
75.00	40280.0
76.00	3498.0
76.80	419.0
77.80	243.0
78.90	3956.0
79.90	1294.0
80.90	4940.0
81.90	917.0
86.90	2961.0
87.80	2407.0
90.80	382.0
91.90	2554.0
93.00	3321.0
94.00	9697.0
95.00	67168.0
96.00	4316.0
103.80	500.0
105.70	433.0
115.70	305.0
116.90	725.0
117.80	328.0
118.80	559.0
127.90	355.0
129.90	229.0
130.80	172.0
134.70	122.0
136.80	124.0
140.90	884.0
142.90	1187.0
147.90	205.0
154.80	212.0
156.80	138.0
158.80	102.0
171.90	207.0
173.00	767.0
173.90	50160.0
174.90	3488.0
175.90	49792.0
176.90	3243.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30

m/z	Abundance
35.90	718.0
36.90	4899.0
37.90	4136.0
38.90	1517.0
39.90	203.0
43.90	1207.0
44.90	923.0
45.90	128.0
46.90	883.0
47.80	559.0
49.00	3470.0
49.90	15954.0
51.00	4884.0
51.90	179.0
54.80	285.0
55.90	1508.0
56.90	3175.0
59.90	673.0
60.90	4227.0
61.90	4375.0
62.90	3537.0
64.00	257.0
66.90	235.0
67.90	8498.0
69.00	8011.0
70.00	907.0
72.00	491.0
73.00	3984.0
74.00	14759.0
75.00	40720.0
76.00	3564.0
76.90	403.0
78.00	252.0
78.90	4115.0
79.80	1260.0
80.90	4894.0
81.90	963.0
82.90	112.0
86.90	2940.0
87.80	2576.0
90.80	335.0
91.90	2696.0
92.90	3476.0
94.00	9884.0
95.00	67712.0
96.00	4611.0
103.80	488.0
105.70	475.0
110.70	121.0
111.60	112.0
115.70	312.0
116.90	779.0
117.90	411.0
118.80	551.0
127.90	312.0
128.90	128.0
129.80	290.0
130.80	180.0
134.70	179.0
136.80	127.0
140.90	916.0
142.90	1341.0
148.00	196.0
148.70	102.0
154.80	262.0
156.90	161.0
158.70	110.0
171.90	218.0
173.00	756.0
173.90	51584.0
174.90	3857.0
175.90	51200.0
176.90	3282.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30

m/z	Abundance
35.90	686.0
36.90	4281.0
37.90	3900.0
38.90	1355.0
39.90	170.0
43.90	1178.0
44.90	773.0
45.90	106.0
46.80	709.0
47.80	518.0
49.00	3159.0
49.90	15055.0
51.00	4588.0
51.90	164.0
54.80	308.0
55.90	1424.0
56.90	2911.0
57.90	107.0
59.90	657.0
60.90	3786.0
61.90	4268.0
63.00	3189.0
64.00	206.0
66.90	185.0
67.90	7834.0
68.90	7452.0
70.00	788.0
71.90	454.0
73.00	3639.0
74.00	13647.0
75.00	37280.0
76.00	3243.0
76.90	359.0
77.70	244.0
78.90	3937.0
79.90	1100.0
80.90	4389.0
81.80	949.0
82.90	105.0
86.90	2639.0
87.90	2481.0
90.70	277.0
91.90	2461.0
92.90	3377.0
94.00	9189.0
95.00	62232.0
96.00	4393.0
103.80	461.0
104.80	119.0
105.70	430.0
110.60	151.0
111.60	113.0
115.70	312.0
116.90	664.0
117.90	437.0
118.90	501.0
127.90	234.0
128.80	166.0
129.80	281.0
130.80	155.0
134.70	193.0
136.80	128.0
140.90	889.0
142.90	1247.0
147.90	162.0
154.80	236.0
156.90	163.0
158.70	106.0
171.90	207.0
173.00	673.0
173.90	48512.0
174.90	3711.0
175.90	48056.0
176.90	3134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30

m/z	Abundance
43.70	381.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30