

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
 Data File : VU049698.D
 Acq On : 13 Jul 2022 11:08
 Operator : SY/MD
 Sample : VU0713MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK152

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049698.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.517	52	55	62	rVB3	1790	1546	0.18%	0.024%
2	1.597	72	80	97	rBV	103743	119554	13.88%	1.829%
3	1.903	166	175	188	rBV	80874	105800	12.28%	1.618%
4	2.424	335	337	340	rBV	457	279	0.03%	0.004%
5	2.562	368	380	395	rBV	162046	259214	30.09%	3.965%
6	2.642	403	405	412	rVB2	398	292	0.03%	0.004%
7	2.790	443	451	458	rBV2	791	1075	0.12%	0.016%
8	3.038	523	528	539	rBV5	1257	2035	0.24%	0.031%
9	3.144	554	561	563	rBV2	341	377	0.04%	0.006%
10	3.182	567	573	577	rVV3	395	561	0.07%	0.009%
11	3.533	679	682	685	rVB2	242	181	0.02%	0.003%
12	3.552	685	688	692	rBV	287	249	0.03%	0.004%
13	3.681	723	728	731	rBV	235	222	0.03%	0.003%
14	3.784	757	760	766	rVB	188	181	0.02%	0.003%
15	4.051	840	843	846	rBV2	225	198	0.02%	0.003%
16	4.070	847	849	859	rVB2	276	340	0.04%	0.005%
17	4.208	889	892	899	rVV2	288	369	0.04%	0.006%
18	4.253	903	906	913	rVB2	199	181	0.02%	0.003%
19	4.446	963	966	971	rVV2	213	182	0.02%	0.003%
20	4.491	977	980	984	rVV	273	187	0.02%	0.003%
21	4.620	1007	1020	1047	rBV	106443	255654	29.68%	3.911%
22	4.903	1104	1108	1111	rBV3	250	208	0.02%	0.003%
23	5.060	1142	1157	1183	rVV	161186	348494	40.46%	5.331%
24	5.282	1221	1226	1228	rBV3	856	763	0.09%	0.012%
25	5.321	1236	1238	1241	rVB	493	207	0.02%	0.003%
26	5.478	1281	1287	1291	rBV2	221	306	0.04%	0.005%
27	5.594	1319	1323	1328	rVB	211	183	0.02%	0.003%
28	5.620	1328	1331	1334	rBV	264	214	0.02%	0.003%
29	5.723	1341	1363	1383	rBV2	318842	861322	100.00%	13.176%
30	6.118	1480	1486	1490	rVB3	341	390	0.05%	0.006%
31	6.247	1511	1526	1545	rBV	270067	511467	59.38%	7.824%
32	6.407	1574	1576	1581	rVB2	230	198	0.02%	0.003%
33	6.443	1584	1587	1592	rVB2	366	256	0.03%	0.004%
34	6.485	1592	1600	1601	rBV	183	188	0.02%	0.003%
35	6.523	1607	1612	1622	rBV5	1389	2561	0.30%	0.039%
36	6.690	1646	1664	1687	rBV	207670	404766	46.99%	6.192%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
 Data File : VU049698.D
 Acq On : 13 Jul 2022 11:08
 Operator : SY/MD
 Sample : VU0713MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK152

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.768	1687	1688	1694	rVB2	535	373	0.04%	0.006%
38	6.800	1694	1698	1700	rBV4	364	278	0.03%	0.004%
39	6.858	1713	1716	1718	rBV2	243	170	0.02%	0.003%
40	7.108	1791	1794	1798	rVB	337	264	0.03%	0.004%
41	7.131	1798	1801	1806	rVB2	201	198	0.02%	0.003%
42	7.186	1806	1818	1824	rBV5	700	1506	0.17%	0.023%
43	7.565	1921	1936	1954	rBV2	107330	186857	21.69%	2.858%
44	7.642	1957	1960	1963	rVB2	251	190	0.02%	0.003%
45	7.687	1970	1974	1980	rVB3	875	982	0.11%	0.015%
46	7.800	2001	2009	2013	rBV4	1018	1482	0.17%	0.023%
47	7.896	2026	2039	2056	rBV	367712	628384	72.96%	9.612%
48	7.973	2061	2063	2064	rBV2	437	208	0.02%	0.003%
49	8.179	2115	2127	2140	rBV	70583	118236	13.73%	1.809%
50	8.276	2154	2157	2159	rBV3	290	215	0.02%	0.003%
51	8.411	2195	2199	2204	rBV2	289	269	0.03%	0.004%
52	8.468	2212	2217	2220	rBV2	225	218	0.03%	0.003%
53	8.632	2256	2268	2303	rBV2	284210	539988	62.69%	8.260%
54	8.838	2328	2332	2333	rBV	285	177	0.02%	0.003%
55	8.848	2333	2335	2338	rVB2	322	200	0.02%	0.003%
56	8.915	2351	2356	2358	rBV2	254	237	0.03%	0.004%
57	9.092	2405	2411	2413	rBV2	297	309	0.04%	0.005%
58	9.224	2448	2452	2456	rBV2	220	199	0.02%	0.003%
59	9.417	2499	2512	2533	rBV	368629	615402	71.45%	9.414%
60	9.562	2551	2557	2559	rBV2	328	341	0.04%	0.005%
61	9.578	2559	2562	2565	rVV	302	187	0.02%	0.003%
62	9.642	2578	2582	2586	rBV	331	227	0.03%	0.003%
63	9.710	2600	2603	2611	rVB3	371	426	0.05%	0.007%
64	9.803	2625	2632	2633	rBV	277	311	0.04%	0.005%
65	9.854	2643	2648	2652	rBV	253	268	0.03%	0.004%
66	9.980	2682	2687	2690	rBV2	272	242	0.03%	0.004%
67	10.047	2703	2708	2712	rBV2	314	290	0.03%	0.004%
68	10.102	2722	2725	2728	rBV2	278	215	0.02%	0.003%
69	10.169	2743	2746	2750	rBV2	291	265	0.03%	0.004%
70	10.247	2766	2770	2773	rBV2	218	184	0.02%	0.003%
71	10.356	2798	2804	2809	rVV2	195	298	0.03%	0.005%
72	10.407	2817	2820	2824	rVB	244	194	0.02%	0.003%
73	10.459	2829	2836	2837	rBV2	238	258	0.03%	0.004%
74	10.481	2838	2843	2848	rVV3	431	494	0.06%	0.008%
75	10.565	2866	2869	2875	rVB2	280	271	0.03%	0.004%
76	10.636	2885	2891	2900	rVB2	1869	2637	0.31%	0.040%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
 Data File : VU049698.D
 Acq On : 13 Jul 2022 11:08
 Operator : SY/MD
 Sample : VU0713MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK152

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	10.755	2915	2928	2947	rBV	281416	448377	52.06%	6.859%
78	10.867	2959	2963	2966	rBV2	435	298	0.03%	0.005%
79	11.263	3078	3086	3087	rBV	276	340	0.04%	0.005%
80	11.497	3156	3159	3161	rBV	276	213	0.02%	0.003%
81	11.555	3171	3177	3184	rBV2	601	915	0.11%	0.014%
82	11.722	3226	3229	3231	rBV	238	171	0.02%	0.003%
83	11.745	3232	3236	3243	rVB4	735	811	0.09%	0.012%
84	11.809	3244	3256	3278	rBV	337735	542190	62.95%	8.294%
85	11.957	3299	3302	3305	rBV2	246	194	0.02%	0.003%
86	12.192	3363	3375	3399	rVV	331177	536535	62.29%	8.207%
87	12.340	3419	3421	3427	rVB	298	245	0.03%	0.004%
88	12.410	3440	3443	3446	rBV2	256	175	0.02%	0.003%
89	12.812	3565	3568	3574	rVB	310	253	0.03%	0.004%
90	13.115	3659	3662	3667	rBV	290	242	0.03%	0.004%
91	13.182	3680	3683	3688	rVB2	493	389	0.05%	0.006%
92	13.217	3688	3694	3697	rBV2	959	1164	0.14%	0.018%
93	13.754	3858	3861	3864	rBV	399	280	0.03%	0.004%
94	13.793	3868	3873	3876	rBV2	361	313	0.04%	0.005%
95	13.841	3881	3888	3899	rBV4	2981	4307	0.50%	0.066%
96	14.092	3958	3966	3974	rBV2	6555	9720	1.13%	0.149%
97	14.243	4010	4013	4017	rBV3	280	200	0.02%	0.003%
98	14.333	4033	4041	4051	rVB4	3492	5292	0.61%	0.081%
99	15.172	4300	4302	4305	rBV2	440	293	0.03%	0.004%
100	15.333	4347	4352	4354	rBV2	607	699	0.08%	0.011%




Sum of corrected areas: 6537266

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
Data File : VU049698.D
Acq On : 13 Jul 2022 11:08
Operator : SY/MD
Sample : VU0713MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK152

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

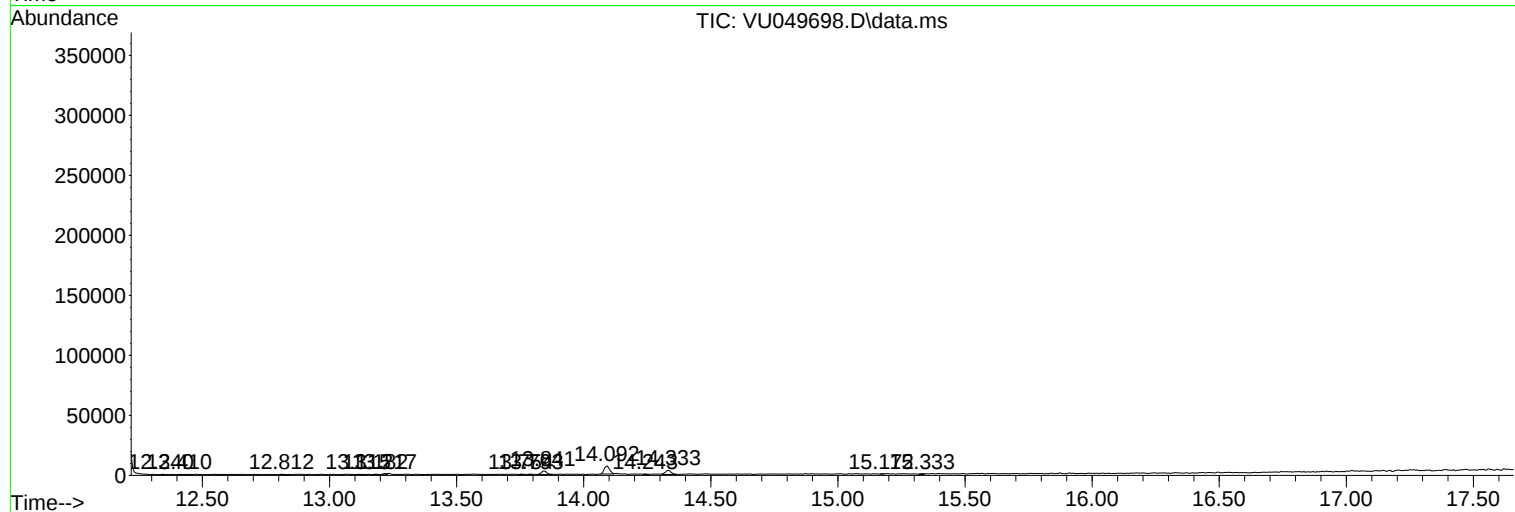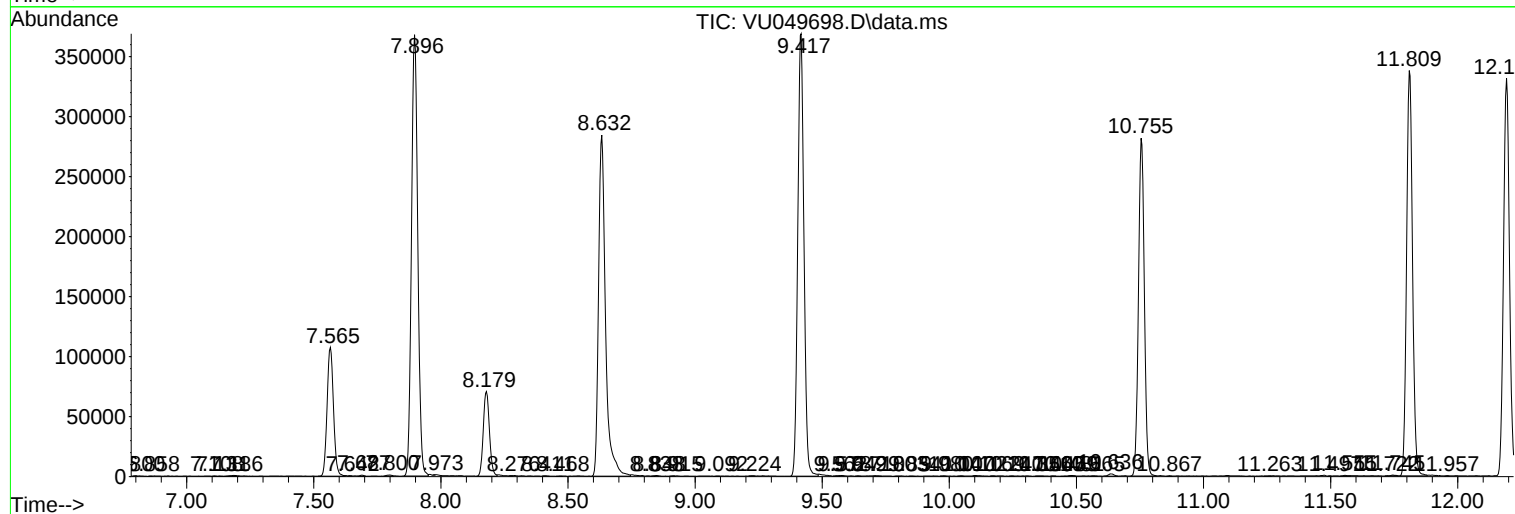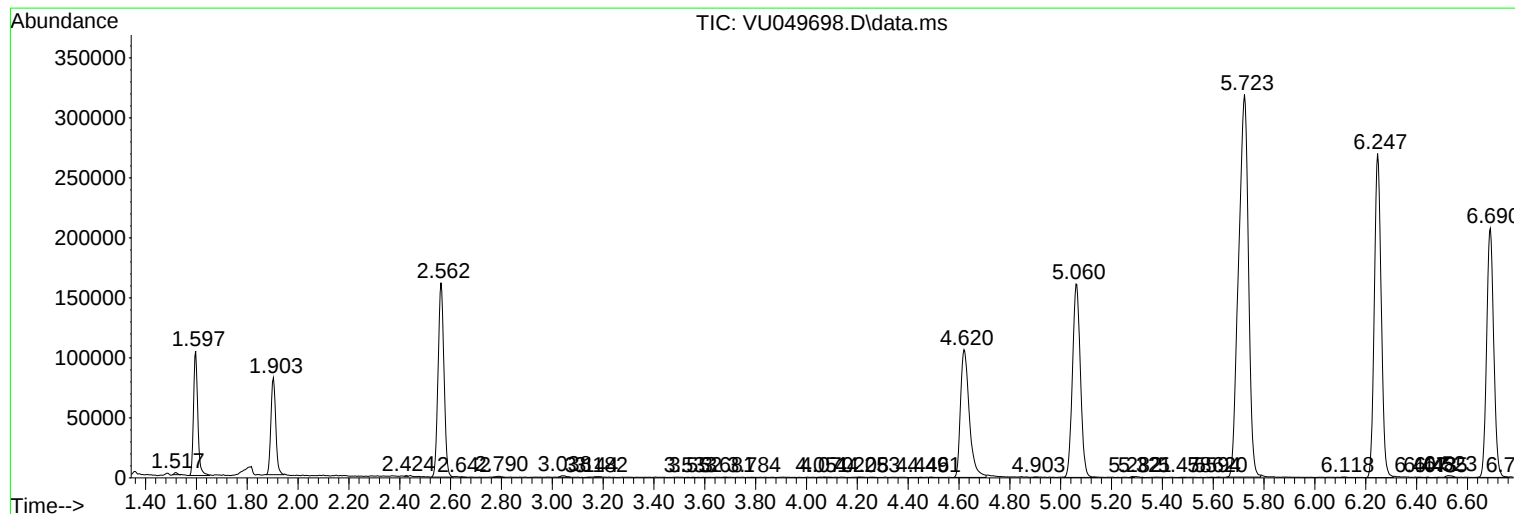

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
Data File : VU049698.D
Acq On : 13 Jul 2022 11:08
Operator : SY/MD
Sample : VU0713MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK152

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
Data File : VU049698.D
Acq On : 13 Jul 2022 11:08
Operator : SY/MD
Sample : VU0713MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK152

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc