

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
 Data File : VU049699.D
 Acq On : 13 Jul 2022 11:32
 Operator : SY/MD
 Sample : VU0713WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK153

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049699.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	10	rVB2	2940	2188	0.25%	0.033%
2	1.517	51	55	67	rBV3	1907	3212	0.36%	0.048%
3	1.597	72	80	97	rBV	106302	120523	13.61%	1.804%
4	1.800	125	143	151	rVB5	8525	16230	1.83%	0.243%
5	1.903	166	175	195	rVB	79915	110079	12.43%	1.648%
6	2.356	313	316	322	rBV3	648	665	0.08%	0.010%
7	2.562	368	380	404	rVB	164462	264503	29.86%	3.959%
8	2.787	445	450	459	rBV2	649	1025	0.12%	0.015%
9	2.861	470	473	475	rBV2	230	145	0.02%	0.002%
10	2.948	495	500	505	rBV2	342	379	0.04%	0.006%
11	3.044	523	530	538	rVB3	1676	2394	0.27%	0.036%
12	3.092	541	545	549	rBV2	212	193	0.02%	0.003%
13	3.141	557	560	564	rBV2	376	401	0.05%	0.006%
14	3.186	564	574	585	rVV	1590	3657	0.41%	0.055%
15	3.250	592	594	600	rVV2	287	276	0.03%	0.004%
16	3.298	605	609	613	rVB2	278	246	0.03%	0.004%
17	3.337	613	621	624	rBV2	266	427	0.05%	0.006%
18	3.456	654	658	662	rBV	406	373	0.04%	0.006%
19	3.475	662	664	672	rVB	421	350	0.04%	0.005%
20	3.636	707	714	718	rBV2	193	240	0.03%	0.004%
21	3.700	731	734	737	rVV	238	147	0.02%	0.002%
22	3.925	800	804	806	rBV	292	237	0.03%	0.004%
23	4.050	837	843	848	rBV	201	230	0.03%	0.003%
24	4.115	859	863	870	rBV2	163	261	0.03%	0.004%
25	4.263	906	909	913	rBV	198	141	0.02%	0.002%
26	4.536	990	994	999	rVB	236	183	0.02%	0.003%
27	4.616	1007	1019	1057	rBV	112062	271260	30.62%	4.060%
28	4.960	1121	1126	1127	rBV2	224	155	0.02%	0.002%
29	5.060	1141	1157	1176	rBV	161763	352313	39.77%	5.273%
30	5.150	1181	1185	1186	rVV2	435	298	0.03%	0.004%
31	5.288	1222	1228	1229	rBV	564	538	0.06%	0.008%
32	5.366	1250	1252	1254	rBV2	362	221	0.02%	0.003%
33	5.443	1270	1276	1280	rVB2	218	252	0.03%	0.004%
34	5.722	1342	1363	1391	rBV2	326863	885870	100.00%	13.260%
35	5.877	1408	1411	1415	rVB2	282	230	0.03%	0.003%
36	5.935	1426	1429	1435	rVB2	337	251	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
 Data File : VU049699.D
 Acq On : 13 Jul 2022 11:32
 Operator : SY/MD
 Sample : VU0713WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK153

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	5.960	1435	1437	1441	rBV2	246	196	0.02%	0.003%
38	5.980	1441	1443	1448	rVV	196	150	0.02%	0.002%
39	6.083	1472	1475	1481	rVB2	181	198	0.02%	0.003%
40	6.118	1482	1486	1489	rBV	239	198	0.02%	0.003%
41	6.247	1512	1526	1544	rBV	274610	514251	58.05%	7.697%
42	6.452	1587	1590	1593	rBV	295	195	0.02%	0.003%
43	6.520	1606	1611	1612	rBV2	1283	820	0.09%	0.012%
44	6.690	1649	1664	1686	rVV	216207	416084	46.97%	6.228%
45	6.771	1686	1689	1692	rVV2	230	175	0.02%	0.003%
46	6.806	1695	1700	1711	rVB4	513	807	0.09%	0.012%
47	7.173	1809	1814	1815	rBV2	389	266	0.03%	0.004%
48	7.185	1815	1818	1822	rVB3	594	479	0.05%	0.007%
49	7.369	1872	1875	1879	rBV	178	160	0.02%	0.002%
50	7.565	1924	1936	1954	rBV	108869	189709	21.41%	2.840%
51	7.693	1971	1976	1979	rBV3	436	470	0.05%	0.007%
52	7.825	2013	2017	2020	rBV	191	173	0.02%	0.003%
53	7.896	2026	2039	2057	rBV	375616	638314	72.06%	9.554%
54	8.025	2074	2079	2084	rVB3	523	589	0.07%	0.009%
55	8.076	2092	2095	2104	rVB3	377	400	0.05%	0.006%
56	8.179	2115	2127	2148	rBV	75945	126072	14.23%	1.887%
57	8.359	2179	2183	2185	rBV2	256	215	0.02%	0.003%
58	8.439	2206	2208	2216	rVB2	172	193	0.02%	0.003%
59	8.475	2216	2219	2223	rBV3	274	188	0.02%	0.003%
60	8.632	2255	2268	2301	rBV2	301106	560489	63.27%	8.389%
61	8.893	2345	2349	2355	rVB2	291	263	0.03%	0.004%
62	9.417	2499	2512	2535	rBV	374578	622513	70.27%	9.318%
63	9.697	2596	2599	2602	rBV	226	155	0.02%	0.002%
64	9.838	2640	2643	2648	rVB	272	226	0.03%	0.003%
65	9.883	2654	2657	2660	rBV2	221	147	0.02%	0.002%
66	10.105	2722	2726	2729	rBV2	466	286	0.03%	0.004%
67	10.131	2732	2734	2737	rBV2	266	144	0.02%	0.002%
68	10.147	2737	2739	2743	rVB	227	148	0.02%	0.002%
69	10.442	2825	2831	2836	rBV2	324	430	0.05%	0.006%
70	10.594	2873	2878	2881	rBV2	317	311	0.04%	0.005%
71	10.635	2886	2891	2901	rVV4	576	943	0.11%	0.014%
72	10.754	2916	2928	2952	rBV	294938	468966	52.94%	7.019%
73	10.918	2976	2979	2986	rBV2	166	189	0.02%	0.003%
74	11.069	3023	3026	3029	rBV	272	205	0.02%	0.003%
75	11.092	3030	3033	3038	rVV	326	293	0.03%	0.004%
76	11.150	3047	3051	3058	rVB	319	418	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
 Data File : VU049699.D
 Acq On : 13 Jul 2022 11:32
 Operator : SY/MD
 Sample : VU0713WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK153

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	11.401	3126	3129	3132	rVB	280	179	0.02%	0.003%
78	11.468	3143	3150	3152	rBV3	429	414	0.05%	0.006%
79	11.510	3160	3163	3170	rVB2	409	514	0.06%	0.008%
80	11.545	3170	3174	3177	rBV2	308	278	0.03%	0.004%
81	11.748	3233	3237	3238	rBV	495	343	0.04%	0.005%
82	11.812	3244	3257	3276	rBV	336892	538086	60.74%	8.054%
83	11.928	3290	3293	3295	rBV2	287	176	0.02%	0.003%
84	11.947	3297	3299	3303	rVB2	459	274	0.03%	0.004%
85	12.057	3330	3333	3338	rVB	339	276	0.03%	0.004%
86	12.089	3338	3343	3344	rBV2	399	288	0.03%	0.004%
87	12.192	3362	3375	3403	rBV	334564	543936	61.40%	8.142%
88	12.388	3432	3436	3439	rBV	281	296	0.03%	0.004%
89	12.635	3507	3513	3518	rBV2	343	509	0.06%	0.008%
90	12.867	3582	3585	3587	rBV	290	178	0.02%	0.003%
91	13.211	3689	3692	3693	rBV	295	162	0.02%	0.002%
92	13.780	3866	3869	3872	rBV	334	299	0.03%	0.004%
93	13.841	3884	3888	3891	rBV2	880	792	0.09%	0.012%
94	14.095	3960	3967	3984	rVB2	2878	5139	0.58%	0.077%
95	14.185	3992	3995	4001	rVB3	481	440	0.05%	0.007%
96	14.240	4009	4012	4015	rBV2	331	261	0.03%	0.004%
97	14.378	4052	4055	4061	rBV3	348	470	0.05%	0.007%
98	14.529	4098	4102	4106	rVB	423	339	0.04%	0.005%
99	14.937	4226	4229	4231	rBV3	481	376	0.04%	0.006%
100	15.770	4485	4488	4492	rBV2	561	436	0.05%	0.007%




Sum of corrected areas: 6680982

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
Data File : VU049699.D
Acq On : 13 Jul 2022 11:32
Operator : SY/MD
Sample : VU0713WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK153

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

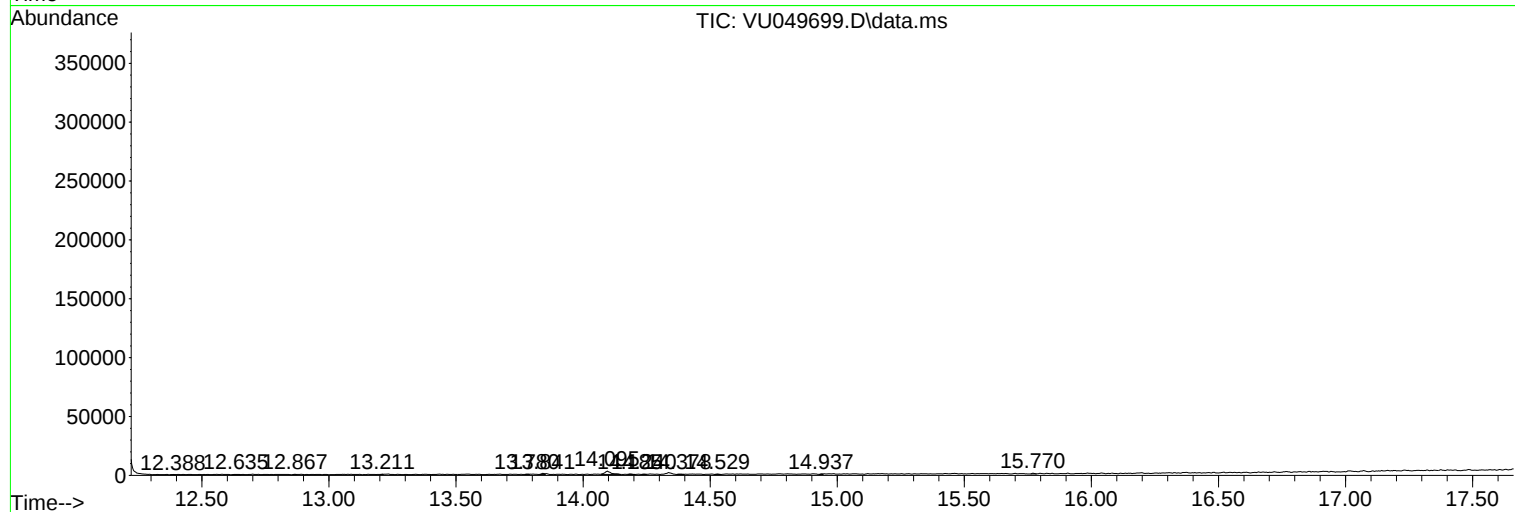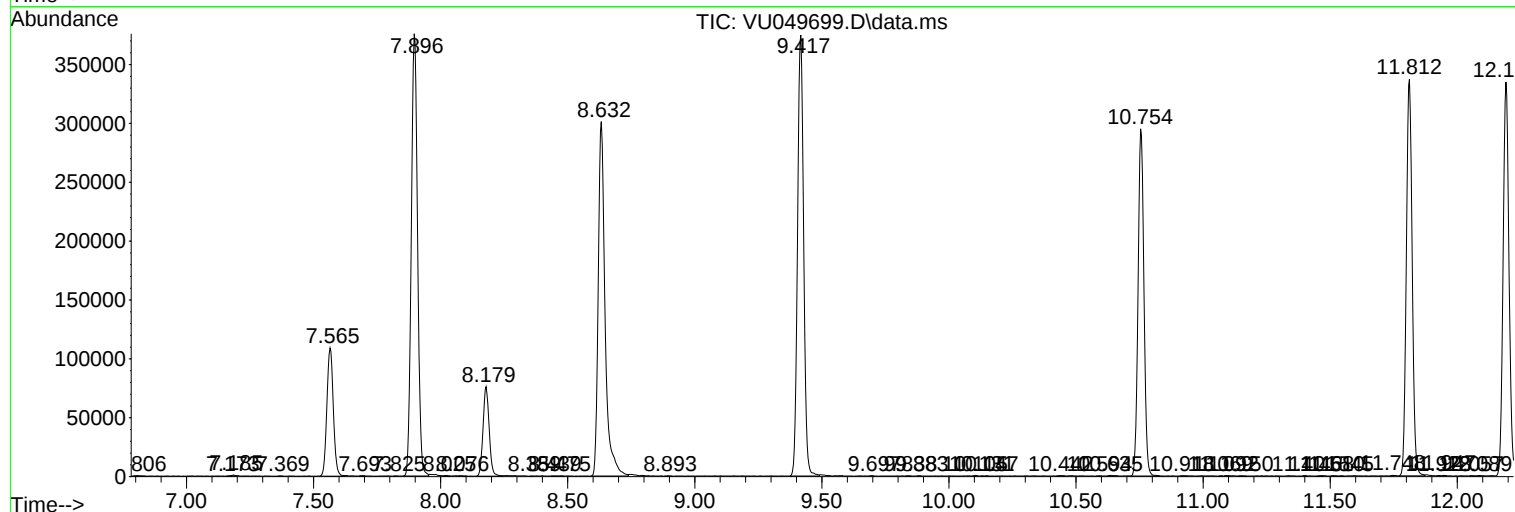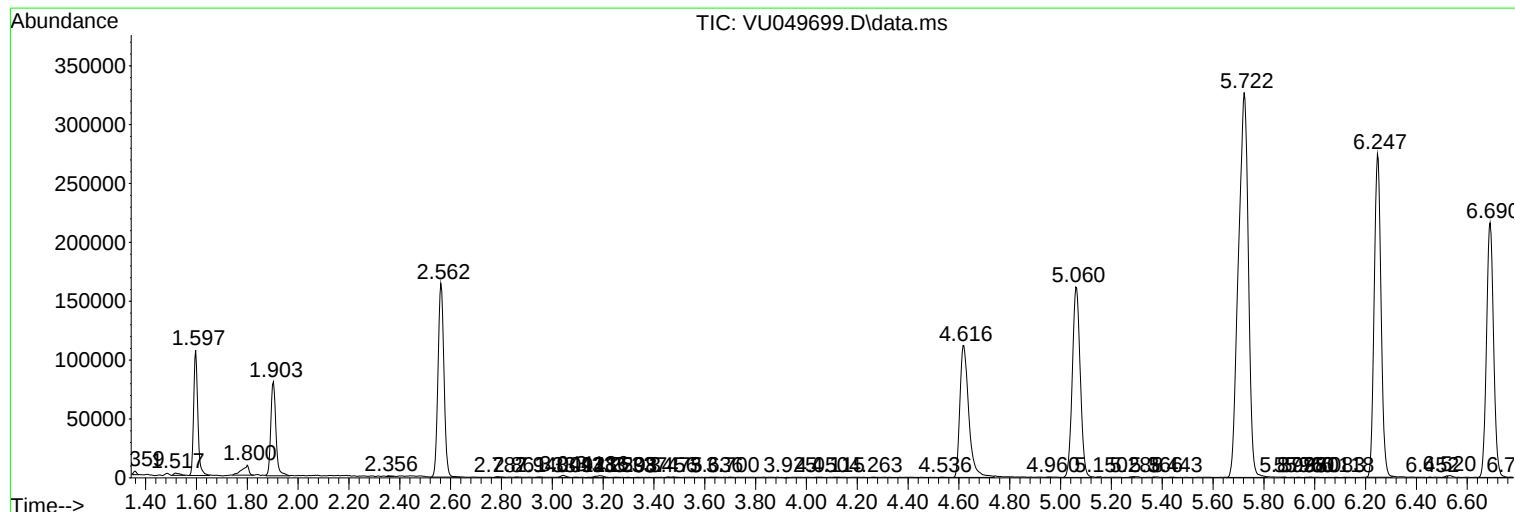

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
Data File : VU049699.D
Acq On : 13 Jul 2022 11:32
Operator : SY/MD
Sample : VU0713WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK153

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
Data File : VU049699.D
Acq On : 13 Jul 2022 11:32
Operator : SY/MD
Sample : VU0713WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK153

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc