

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
 Data File : VU049700.D
 Acq On : 13 Jul 2022 11:58
 Operator : SY/MD
 Sample : N3670-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 MDL-WATER-QT2-2022-04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049700.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.382	9	13	21	rVB	7571	7184	0.82%	0.094%
2	1.520	50	56	72	rBV	7068	11506	1.32%	0.150%
3	1.597	72	80	97	rBV	98462	116498	13.32%	1.524%
4	1.903	167	175	193	rVB	76571	108356	12.39%	1.417%
5	2.134	239	247	256	rVB	11335	15995	1.83%	0.209%
6	2.272	288	290	296	rBV2	538	327	0.04%	0.004%
7	2.433	338	340	341	rBV	449	200	0.02%	0.003%
8	2.562	368	380	394	rBV2	155755	270130	30.88%	3.533%
9	2.633	395	402	418	rVB	6938	12248	1.40%	0.160%
10	2.787	441	450	462	rBV	8782	14342	1.64%	0.188%
11	2.951	491	501	515	rVV2	5079	9755	1.12%	0.128%
12	3.044	519	530	547	rVB2	12616	23374	2.67%	0.306%
13	3.170	566	569	570	rBV	354	207	0.02%	0.003%
14	3.266	596	599	602	rVB	196	135	0.02%	0.002%
15	3.359	615	628	646	rVB4	21342	48471	5.54%	0.634%
16	3.449	653	656	662	rVB2	149	154	0.02%	0.002%
17	3.562	687	691	694	rBV	171	134	0.02%	0.002%
18	3.742	742	747	753	rVB2	236	277	0.03%	0.004%
19	3.774	753	757	763	rBV2	135	158	0.02%	0.002%
20	3.800	763	765	768	rVB	269	171	0.02%	0.002%
21	3.867	768	786	803	rBV2	7233	17371	1.99%	0.227%
22	4.108	857	861	864	rBV	197	171	0.02%	0.002%
23	4.163	876	878	881	rVB	309	175	0.02%	0.002%
24	4.182	881	884	886	rBV	208	145	0.02%	0.002%
25	4.333	927	931	934	rBV2	198	200	0.02%	0.003%
26	4.436	959	963	971	rVB2	184	212	0.02%	0.003%
27	4.478	971	976	978	rBV2	128	133	0.02%	0.002%
28	4.623	1009	1021	1044	rBV	102773	276474	31.61%	3.616%
29	4.977	1116	1131	1142	rBV4	8324	17015	1.95%	0.223%
30	5.063	1142	1158	1181	rVV	160924	367888	42.06%	4.811%
31	5.317	1223	1237	1248	rVV3	9446	20659	2.36%	0.270%
32	5.385	1248	1258	1272	rVB6	12242	26940	3.08%	0.352%
33	5.523	1287	1301	1315	rBV2	8059	17152	1.96%	0.224%
34	5.726	1342	1364	1377	rBV2	318494	874646	100.00%	11.438%
35	5.973	1437	1441	1442	rBV	413	285	0.03%	0.004%
36	6.057	1464	1467	1471	rVB	209	138	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
 Data File : VU049700.D
 Acq On : 13 Jul 2022 11:58
 Operator : SY/MD
 Sample : N3670-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 MDL-WATER-QT2-2022-04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.150	1493	1496	1501	rVB2	207	161	0.02%	0.002%
38	6.247	1512	1526	1551	rBV	271228	518573	59.29%	6.782%
39	6.337	1551	1554	1557	rBV	246	207	0.02%	0.003%
40	6.394	1567	1572	1575	rBV2	440	392	0.04%	0.005%
41	6.430	1580	1583	1588	rVB	302	244	0.03%	0.003%
42	6.542	1606	1618	1630	rBV5	13611	25086	2.87%	0.328%
43	6.603	1634	1637	1642	rVB3	372	294	0.03%	0.004%
44	6.690	1646	1664	1678	rBV	209694	407740	46.62%	5.332%
45	6.761	1679	1686	1688	rBV3	12076	14159	1.62%	0.185%
46	6.848	1709	1713	1716	rBV2	166	176	0.02%	0.002%
47	6.915	1729	1734	1735	rBV	209	174	0.02%	0.002%
48	6.954	1743	1746	1751	rBV	180	144	0.02%	0.002%
49	6.993	1755	1758	1760	rBV2	189	139	0.02%	0.002%
50	7.105	1784	1793	1805	rVB2	9940	16404	1.88%	0.215%
51	7.189	1812	1819	1824	rVV4	950	1162	0.13%	0.015%
52	7.346	1865	1868	1873	rBV	183	168	0.02%	0.002%
53	7.484	1907	1911	1918	rVB2	301	368	0.04%	0.005%
54	7.565	1918	1936	1947	rBV	106376	193925	22.17%	2.536%
55	7.687	1969	1974	1981	rBV3	938	973	0.11%	0.013%
56	7.793	1995	2007	2023	rBV3	24147	42952	4.91%	0.562%
57	7.896	2025	2039	2053	rVV	368004	633063	72.38%	8.279%
58	7.970	2054	2062	2079	rVB	25879	44583	5.10%	0.583%
59	8.089	2095	2099	2102	rVB3	429	359	0.04%	0.005%
60	8.179	2116	2127	2152	rBV2	72877	140603	16.08%	1.839%
61	8.401	2186	2196	2207	rVV3	16044	26112	2.99%	0.341%
62	8.552	2234	2243	2256	rVB4	13426	22239	2.54%	0.291%
63	8.636	2256	2269	2280	rBV2	282778	515309	58.92%	6.739%
64	8.812	2314	2324	2333	rVB2	8719	14056	1.61%	0.184%
65	8.922	2349	2358	2369	rBV	6871	11233	1.28%	0.147%
66	9.063	2396	2402	2405	rBV	198	230	0.03%	0.003%
67	9.121	2415	2420	2425	rVB2	306	310	0.04%	0.004%
68	9.285	2464	2471	2480	rVB2	308	555	0.06%	0.007%
69	9.333	2484	2486	2489	rBV2	234	171	0.02%	0.002%
70	9.417	2499	2512	2539	rBV	388162	674586	77.13%	8.822%
71	9.571	2550	2560	2572	rVB2	25012	40016	4.58%	0.523%
72	9.693	2585	2598	2612	rBV	23059	38227	4.37%	0.500%
73	9.748	2612	2615	2620	rVB2	269	189	0.02%	0.002%
74	9.816	2633	2636	2644	rVB2	207	224	0.03%	0.003%
75	10.105	2713	2726	2742	rBV4	36367	74050	8.47%	0.968%
76	10.291	2772	2784	2796	rBV3	7188	11525	1.32%	0.151%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
 Data File : VU049700.D
 Acq On : 13 Jul 2022 11:58
 Operator : SY/MD
 Sample : N3670-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 MDL-WATER-QT2-2022-04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	10.484	2834	2844	2856	rVB	25294	36637	4.19%	0.479%
78	10.635	2888	2891	2892	rBV	404	231	0.03%	0.003%
79	10.716	2914	2916	2917	rBV	321	160	0.02%	0.002%
80	10.758	2917	2929	2943	rVV	278811	480116	54.89%	6.279%
81	10.822	2943	2949	2963	rVB3	17132	26039	2.98%	0.341%
82	11.089	3022	3032	3042	rBV	21764	32482	3.71%	0.425%
83	11.179	3057	3060	3062	rBV	214	145	0.02%	0.002%
84	11.468	3139	3150	3160	rBV2	21147	30255	3.46%	0.396%
85	11.568	3177	3181	3186	rVB2	232	226	0.03%	0.003%
86	11.745	3227	3236	3245	rBV2	18390	27568	3.15%	0.361%
87	11.812	3245	3257	3276	rVV	355066	596109	68.15%	7.796%
88	12.192	3362	3375	3397	rBV	346991	584091	66.78%	7.639%
89	12.446	3450	3454	3456	rBV	333	243	0.03%	0.003%
90	12.713	3534	3537	3540	rBV2	275	185	0.02%	0.002%
91	12.999	3617	3626	3637	rVB4	5857	8735	1.00%	0.114%
92	13.221	3685	3695	3709	rVB3	15594	23493	2.69%	0.307%
93	13.343	3731	3733	3741	rVB3	416	330	0.04%	0.004%
94	13.684	3836	3839	3841	rBV2	317	214	0.02%	0.003%
95	13.745	3856	3858	3863	rBV	238	172	0.02%	0.002%
96	13.841	3879	3888	3904	rVB3	12400	19684	2.25%	0.257%
97	14.089	3952	3965	3981	rBV2	16318	27802	3.18%	0.364%
98	14.333	4031	4041	4051	rBV4	13996	20854	2.38%	0.273%
99	14.613	4125	4128	4129	rBV2	397	229	0.03%	0.003%
100	15.754	4481	4483	4486	rBV2	495	331	0.04%	0.004%




Sum of corrected areas: 7646638

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
Data File : VU049700.D
Acq On : 13 Jul 2022 11:58
Operator : SY/MD
Sample : N3670-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MDL-WATER-QT2-2022-04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

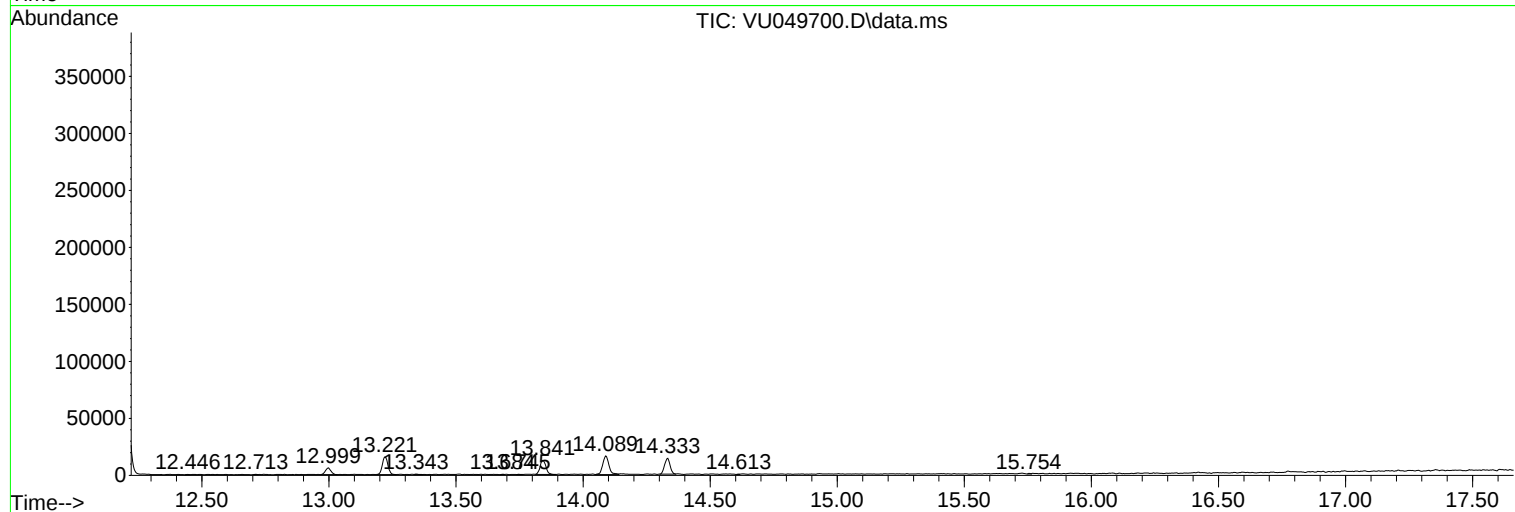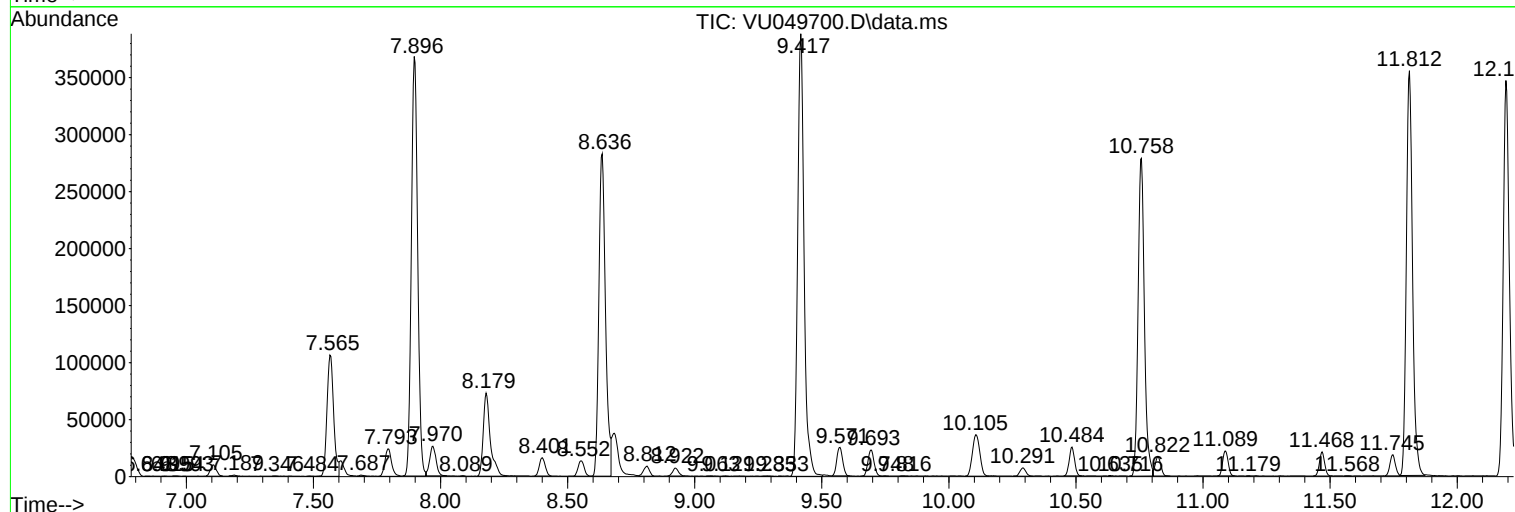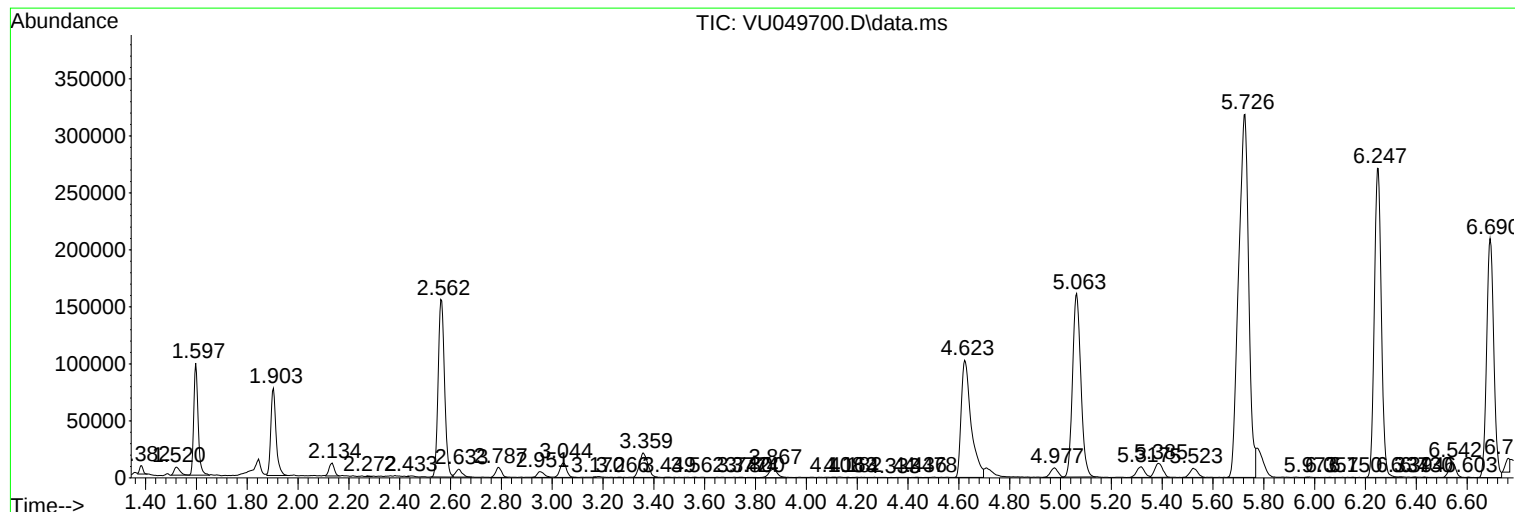

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
Data File : VU049700.D
Acq On : 13 Jul 2022 11:58
Operator : SY/MD
Sample : N3670-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MDL-WATER-QT2-2022-04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
Data File : VU049700.D
Acq On : 13 Jul 2022 11:58
Operator : SY/MD
Sample : N3670-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MDL-WATER-QT2-2022-04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------