

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
 Data File : VU049704.D
 Acq On : 13 Jul 2022 15:49
 Operator : SY/MD
 Sample : N3700-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	98	rBV	100808	115305	12.97%	1.721%
2	1.806	127	145	152	rVB7	8864	19986	2.25%	0.298%
3	1.899	166	174	194	rVB	78751	104127	11.71%	1.554%
4	2.562	368	380	396	rBV	157729	250852	28.22%	3.745%
5	2.784	446	449	451	rBV2	275	198	0.02%	0.003%
6	2.832	460	464	466	rBV	285	208	0.02%	0.003%
7	2.954	497	502	505	rVB3	302	328	0.04%	0.005%
8	2.977	505	509	513	rBV2	283	273	0.03%	0.004%
9	3.044	520	530	539	rBV4	1900	3490	0.39%	0.052%
10	3.176	563	571	572	rBV2	480	481	0.05%	0.007%
11	3.231	582	588	589	rBV	183	186	0.02%	0.003%
12	3.292	601	607	611	rBV2	238	275	0.03%	0.004%
13	3.398	637	640	643	rBV2	270	243	0.03%	0.004%
14	3.485	663	667	669	rBV2	217	152	0.02%	0.002%
15	3.613	704	707	709	rBV2	172	102	0.01%	0.002%
16	3.652	715	719	722	rBV2	161	126	0.01%	0.002%
17	3.671	722	725	729	rBV2	218	155	0.02%	0.002%
18	3.694	729	732	734	rBV2	157	98	0.01%	0.001%
19	3.703	734	735	738	rVB2	319	109	0.01%	0.002%
20	3.732	738	744	745	rBV2	332	278	0.03%	0.004%
21	3.858	779	783	790	rBV	263	309	0.03%	0.005%
22	3.996	823	826	828	rBV2	162	94	0.01%	0.001%
23	4.099	855	858	863	rVB2	216	162	0.02%	0.002%
24	4.147	870	873	878	rBV2	137	118	0.01%	0.002%
25	4.227	895	898	902	rBV2	121	114	0.01%	0.002%
26	4.369	936	942	944	rBV	245	258	0.03%	0.004%
27	4.510	983	986	988	rVB	184	115	0.01%	0.002%
28	4.620	1007	1020	1056	rBV	108051	263107	29.59%	3.928%
29	4.784	1067	1071	1077	rBV3	572	739	0.08%	0.011%
30	4.941	1118	1120	1121	rBV	328	100	0.01%	0.001%
31	4.970	1126	1129	1133	rBV2	335	238	0.03%	0.004%
32	5.063	1141	1158	1183	rBV	164637	355706	40.01%	5.310%
33	5.208	1200	1203	1206	rVB2	283	169	0.02%	0.003%
34	5.288	1219	1228	1231	rBV3	1019	1343	0.15%	0.020%
35	5.366	1239	1252	1253	rBV2	700	803	0.09%	0.012%
36	5.546	1304	1308	1312	rBV2	150	176	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
 Data File : VU049704.D
 Acq On : 13 Jul 2022 15:49
 Operator : SY/MD
 Sample : N3700-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	5.722	1341	1363	1389	rBV2	328197	889049	100.00%	13.272%
38	5.967	1434	1439	1444	rVB3	323	351	0.04%	0.005%
39	5.993	1444	1447	1453	rBV	275	243	0.03%	0.004%
40	6.041	1459	1462	1463	rBV	204	103	0.01%	0.002%
41	6.118	1485	1486	1489	rVB2	221	99	0.01%	0.001%
42	6.144	1491	1494	1497	rVB2	238	185	0.02%	0.003%
43	6.163	1498	1500	1503	rBV2	178	105	0.01%	0.002%
44	6.185	1503	1507	1510	rBV2	237	214	0.02%	0.003%
45	6.250	1513	1527	1551	rBV	261867	495601	55.75%	7.399%
46	6.410	1575	1577	1583	rBV3	414	440	0.05%	0.007%
47	6.439	1583	1586	1589	rBV	346	228	0.03%	0.003%
48	6.523	1607	1612	1613	rBV2	1521	1160	0.13%	0.017%
49	6.690	1649	1664	1686	rBV	217080	421279	47.39%	6.289%
50	6.803	1693	1699	1700	rBV2	467	433	0.05%	0.006%
51	6.893	1725	1727	1731	rVB	306	183	0.02%	0.003%
52	6.970	1748	1751	1755	rBV	213	161	0.02%	0.002%
53	7.005	1759	1762	1764	rBV	214	134	0.02%	0.002%
54	7.179	1812	1816	1817	rBV2	619	427	0.05%	0.006%
55	7.243	1832	1836	1840	rBV	213	155	0.02%	0.002%
56	7.288	1847	1850	1853	rVB	159	109	0.01%	0.002%
57	7.436	1892	1896	1903	rVB2	496	664	0.07%	0.010%
58	7.488	1903	1912	1919	rBV2	369	858	0.10%	0.013%
59	7.565	1924	1936	1956	rBV2	111370	195280	21.97%	2.915%
60	7.690	1973	1975	1983	rVB3	820	823	0.09%	0.012%
61	7.790	2003	2006	2010	rBV2	244	235	0.03%	0.004%
62	7.825	2014	2017	2019	rBV	169	122	0.01%	0.002%
63	7.899	2026	2040	2063	rBV	371927	646314	72.70%	9.649%
64	8.140	2112	2115	2116	rBV	208	122	0.01%	0.002%
65	8.179	2116	2127	2143	rVV	75918	127351	14.32%	1.901%
66	8.333	2173	2175	2177	rVB2	325	114	0.01%	0.002%
67	8.574	2247	2250	2253	rBV2	136	95	0.01%	0.001%
68	8.632	2256	2268	2299	rBV2	289633	549320	61.79%	8.201%
69	8.809	2319	2323	2327	rVB3	326	258	0.03%	0.004%
70	8.870	2339	2342	2344	rBV2	266	177	0.02%	0.003%
71	9.012	2383	2386	2389	rBV2	202	181	0.02%	0.003%
72	9.285	2467	2471	2473	rBV	205	171	0.02%	0.003%
73	9.417	2499	2512	2531	rBV	366351	614141	69.08%	9.168%
74	9.629	2576	2578	2583	rBV	191	117	0.01%	0.002%
75	9.668	2587	2590	2592	rBV	231	149	0.02%	0.002%
76	9.690	2595	2597	2602	rVB2	271	168	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
 Data File : VU049704.D
 Acq On : 13 Jul 2022 15:49
 Operator : SY/MD
 Sample : N3700-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	9.742	2608	2613	2618	rBV2	317	373	0.04%	0.006%
78	9.777	2618	2624	2627	rBV2	298	279	0.03%	0.004%
79	9.851	2644	2647	2650	rBV	188	133	0.01%	0.002%
80	9.967	2679	2683	2684	rBV2	171	135	0.02%	0.002%
81	10.008	2693	2696	2702	rBV2	214	235	0.03%	0.004%
82	10.237	2764	2767	2774	rBV2	260	336	0.04%	0.005%
83	10.449	2829	2833	2838	rBV2	260	311	0.03%	0.005%
84	10.635	2887	2891	2893	rBV	308	247	0.03%	0.004%
85	10.758	2916	2929	2949	rBV	305661	484608	54.51%	7.235%
86	11.073	3025	3027	3034	rVB	289	231	0.03%	0.003%
87	11.108	3035	3038	3040	rBV	247	184	0.02%	0.003%
88	11.417	3131	3134	3141	rBV2	302	389	0.04%	0.006%
89	11.452	3141	3145	3149	rBV2	395	430	0.05%	0.006%
90	11.475	3149	3152	3160	rVB	429	425	0.05%	0.006%
91	11.812	3242	3257	3276	rBV	348265	558519	62.82%	8.338%
92	12.063	3332	3335	3336	rBV2	277	172	0.02%	0.003%
93	12.076	3337	3339	3347	rVB3	707	684	0.08%	0.010%
94	12.195	3363	3376	3393	rBV	361905	581414	65.40%	8.680%
95	12.282	3400	3403	3405	rBV2	324	234	0.03%	0.003%
96	12.851	3577	3580	3583	rBV	360	221	0.02%	0.003%
97	13.876	3897	3899	3903	rBV	279	252	0.03%	0.004%
98	14.066	3956	3958	3963	rBV2	225	176	0.02%	0.003%
99	14.095	3963	3967	3968	rBV	624	439	0.05%	0.007%
100	16.191	4617	4619	4621	rBV2	602	247	0.03%	0.004%




Sum of corrected areas: 6698516

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
Data File : VU049704.D
Acq On : 13 Jul 2022 15:49
Operator : SY/MD
Sample : N3700-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

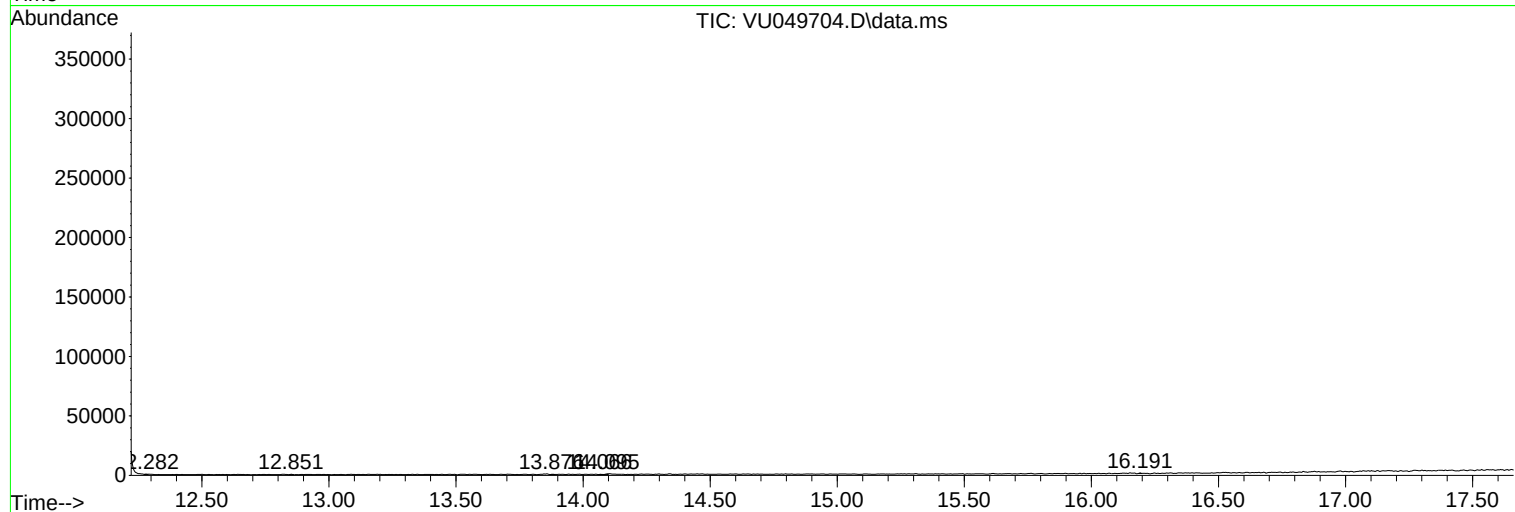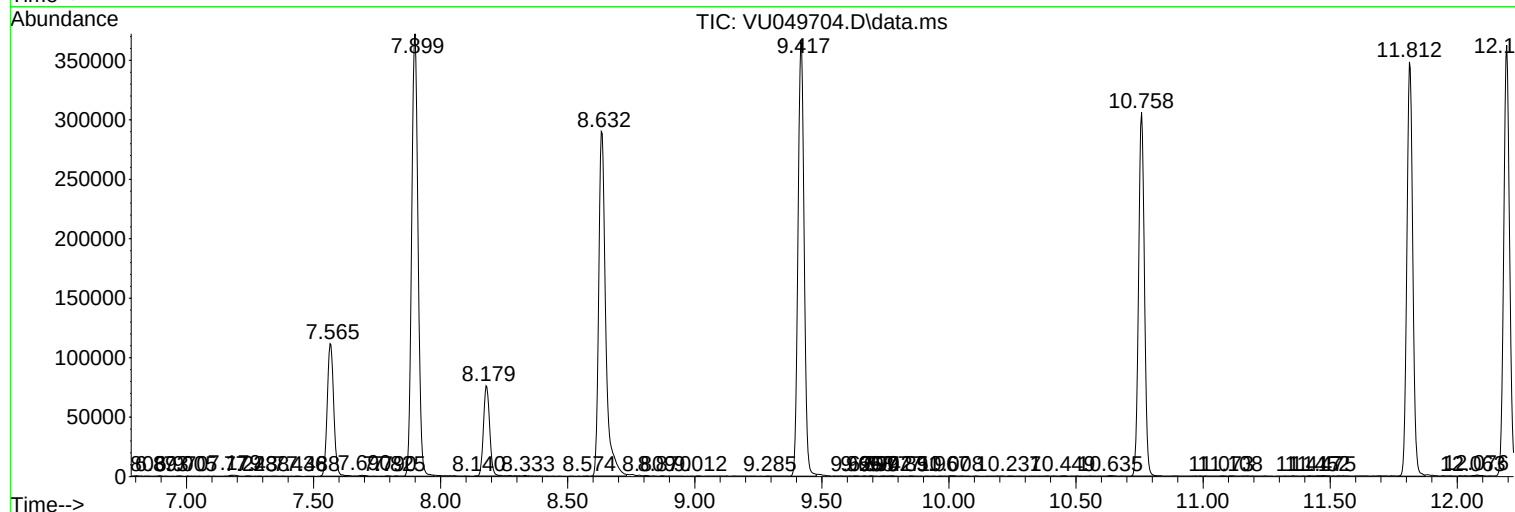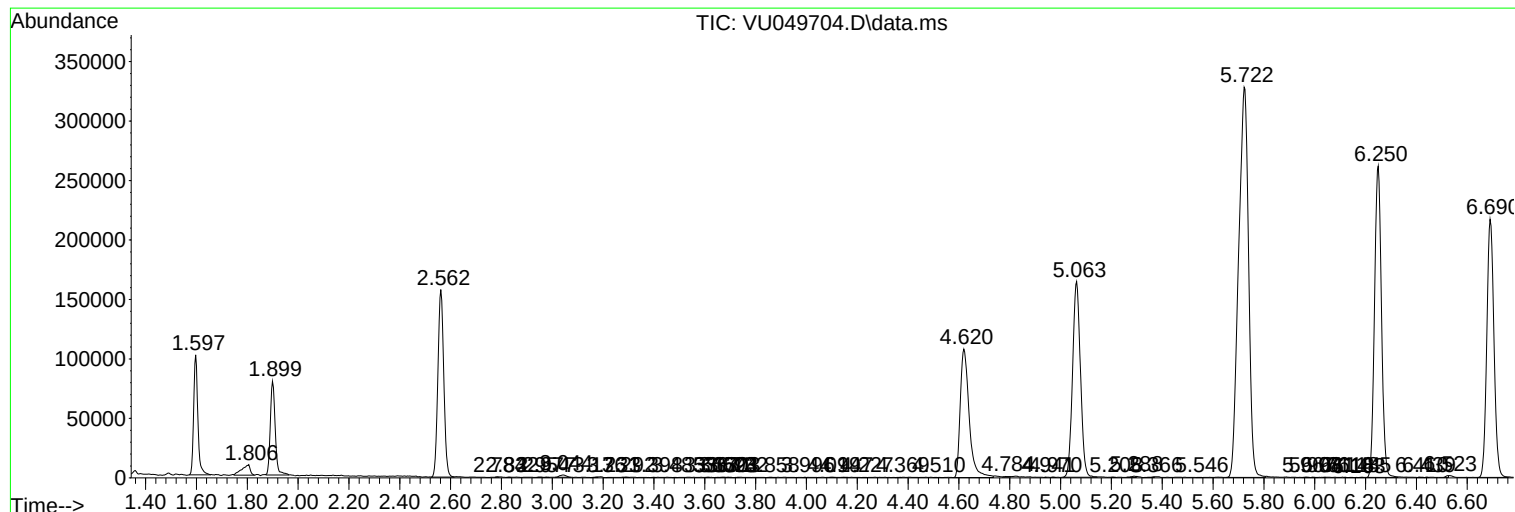

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
Data File : VU049704.D
Acq On : 13 Jul 2022 15:49
Operator : SY/MD
Sample : N3700-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
Data File : VU049704.D
Acq On : 13 Jul 2022 15:49
Operator : SY/MD
Sample : N3700-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------