


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071322\
Data File : VU049696.D
Acq On : 13 Jul 2022 09:52
Operator : SY/MD
Sample : BFB103
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB103

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Title : VOC Analysis
Last Update : Thu Jul 14 05:07:30 2022

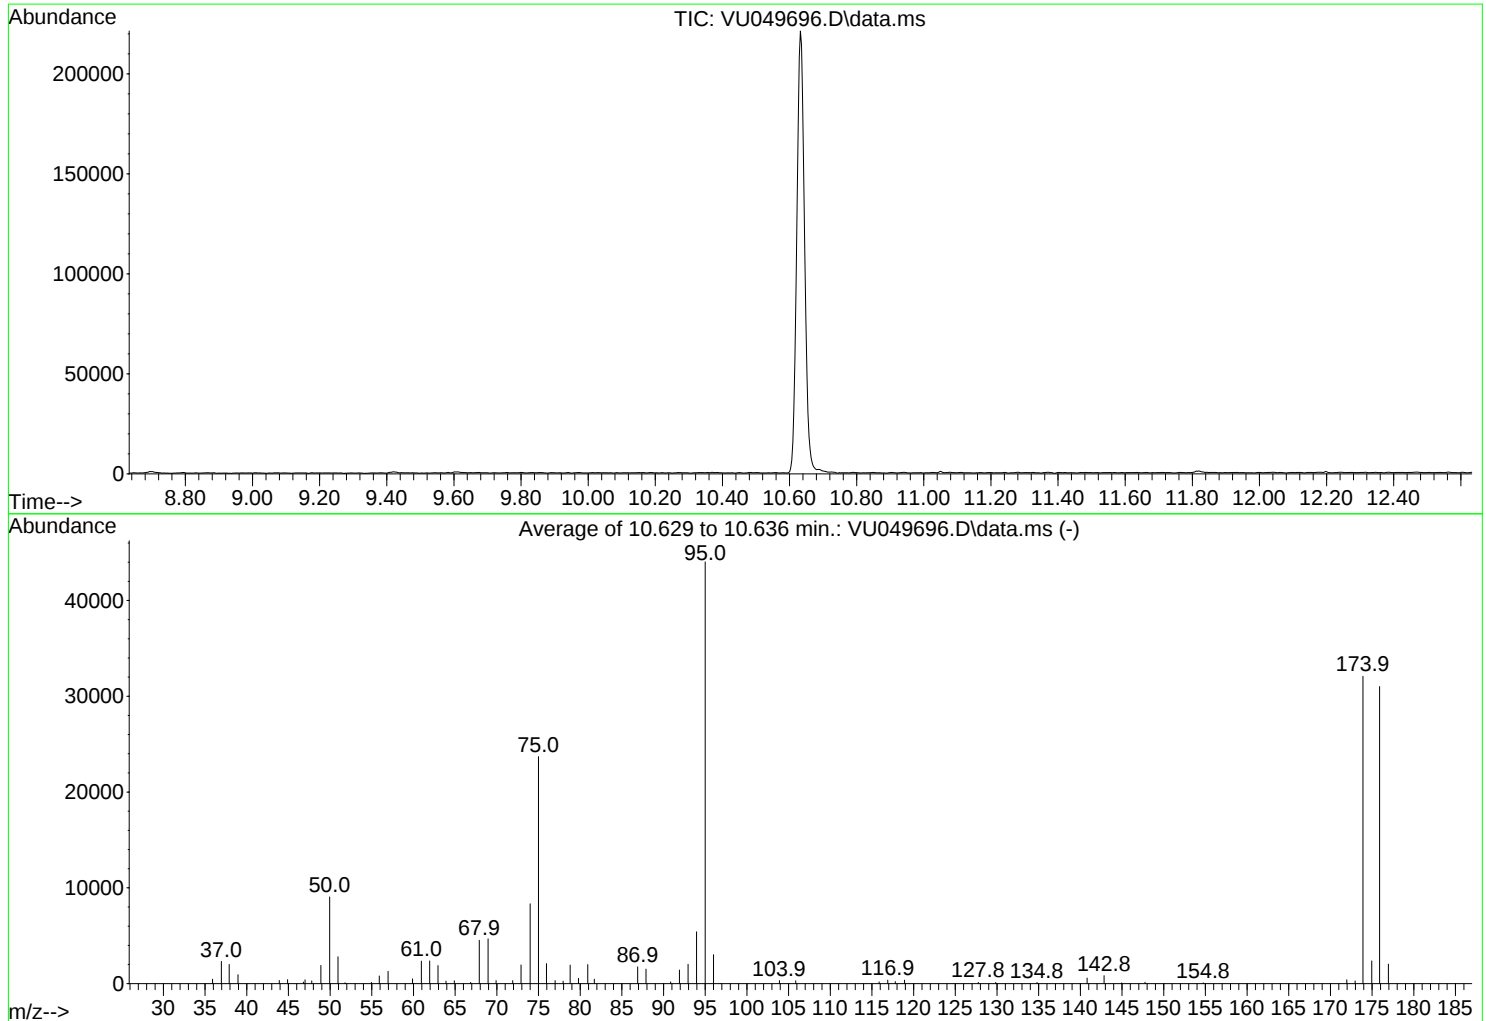

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	9050	PASS
75	95	30	80	53.8	23701	PASS
95	95	100	100	100.0	44035	PASS
96	95	5	9	6.9	3028	PASS
173	174	0.00	2	0.9	285	PASS
174	95	50	120	72.9	32088	PASS
175	174	5	9	7.4	2372	PASS
176	174	95	101	96.7	31021	PASS
177	176	5	9	6.6	2032	PASS

m/z	Abundance
39.90	234.0
43.90	285.0

Instrument :
MSVOA_U
ClientSampleId :
BFB103

m/z	Abundance
35.90	468.0
36.90	2263.0
37.90	1913.0
38.90	1024.0
39.70	135.0
43.90	647.0
44.90	416.0
46.80	507.0
47.90	276.0
48.90	1912.0
49.90	8784.0
50.90	2880.0
51.80	150.0
55.00	110.0
55.90	865.0
56.90	1271.0
59.90	461.0
61.00	2163.0
61.90	2322.0
62.90	1965.0
63.90	219.0
64.90	337.0
66.90	145.0
67.90	4592.0
68.90	4617.0
69.90	338.0
71.90	301.0
72.90	1959.0
74.00	8381.0
75.00	22784.0
75.90	2063.0
77.00	303.0
78.00	299.0
78.80	1886.0
79.80	604.0
80.90	1955.0
81.70	419.0
86.90	1678.0
87.90	1557.0
90.90	139.0
91.90	1492.0
92.90	2019.0
93.90	5321.0
95.00	42608.0
96.00	2861.0
103.90	338.0
105.80	323.0
115.90	159.0
116.90	311.0
117.80	214.0
118.90	298.0
127.80	122.0
129.80	107.0
134.80	135.0
140.80	585.0
142.90	787.0
145.00	128.0
147.70	138.0
172.00	370.0
172.90	398.0
173.90	30608.0
174.90	2395.0
175.90	29464.0
177.00	1967.0

Instrument :
MSVOA_U
ClientSampleId :
BFB103

m/z	Abundance
35.90	494.0
37.00	2397.0
37.90	2031.0
38.90	953.0
39.80	141.0
44.00	617.0
44.90	429.0
47.00	566.0
47.80	284.0
48.90	1969.0
49.90	9320.0
50.90	2889.0
51.80	133.0
55.00	142.0
55.90	797.0
56.90	1290.0
59.90	529.0
61.00	2369.0
62.00	2416.0
62.90	1923.0
63.90	274.0
64.90	324.0
66.90	123.0
67.90	4625.0
69.00	4789.0
69.90	328.0
71.90	353.0
72.90	1988.0
74.00	8569.0
75.00	24456.0
75.90	2172.0
77.00	343.0
78.00	275.0
78.80	1996.0
79.80	572.0
80.90	2043.0
81.70	498.0
86.90	1777.0
87.90	1565.0
90.80	178.0
91.90	1480.0
92.90	2143.0
94.00	5604.0
95.00	45648.0
96.00	3117.0
103.90	334.0
105.80	308.0
115.80	197.0
116.90	371.0
117.80	223.0
118.90	362.0
127.80	135.0
129.90	146.0
134.80	138.0
140.80	604.0
142.80	890.0
144.90	118.0
147.70	148.0
154.70	116.0
172.00	409.0
173.00	456.0
173.90	33024.0
174.90	2469.0
175.90	31880.0
177.00	2102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB103

m/z	Abundance
35.90	464.0
37.00	2300.0
37.90	2087.0
39.00	846.0
39.80	173.0
44.00	577.0
44.90	419.0
47.00	625.0
47.70	316.0
48.90	1850.0
50.00	9045.0
51.00	2643.0
54.90	151.0
55.90	723.0
57.00	1281.0
59.90	499.0
60.90	2528.0
61.90	2398.0
63.00	1760.0
63.90	300.0
64.90	244.0
66.80	123.0
67.90	4366.0
69.00	4603.0
69.90	296.0
71.90	320.0
72.90	1923.0
74.00	8057.0
75.00	23864.0
76.00	2051.0
77.00	315.0
77.90	247.0
78.80	1958.0
79.80	484.0
80.90	1975.0
81.70	506.0
86.90	1788.0
87.90	1435.0
90.80	243.0
91.90	1298.0
93.00	1932.0
94.00	5315.0
95.00	43848.0
96.00	3105.0
96.90	106.0
103.90	295.0
105.90	251.0
115.80	202.0
116.90	413.0
117.80	235.0
118.90	427.0
127.70	163.0
129.90	153.0
134.80	115.0
140.80	579.0
142.80	847.0
147.80	162.0
154.80	130.0
171.90	421.0
173.90	32632.0
175.00	2251.0
175.90	31720.0
176.90	2028.0

Instrument :
MSVOA_U
ClientSampleId :
BFB103