


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071323\
Data File : VU054782.D
Acq On : 13 Jul 2023 08:33
Operator : MD/SY
Sample : BFB033
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB033

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR070723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jul 14 07:53:34 2023

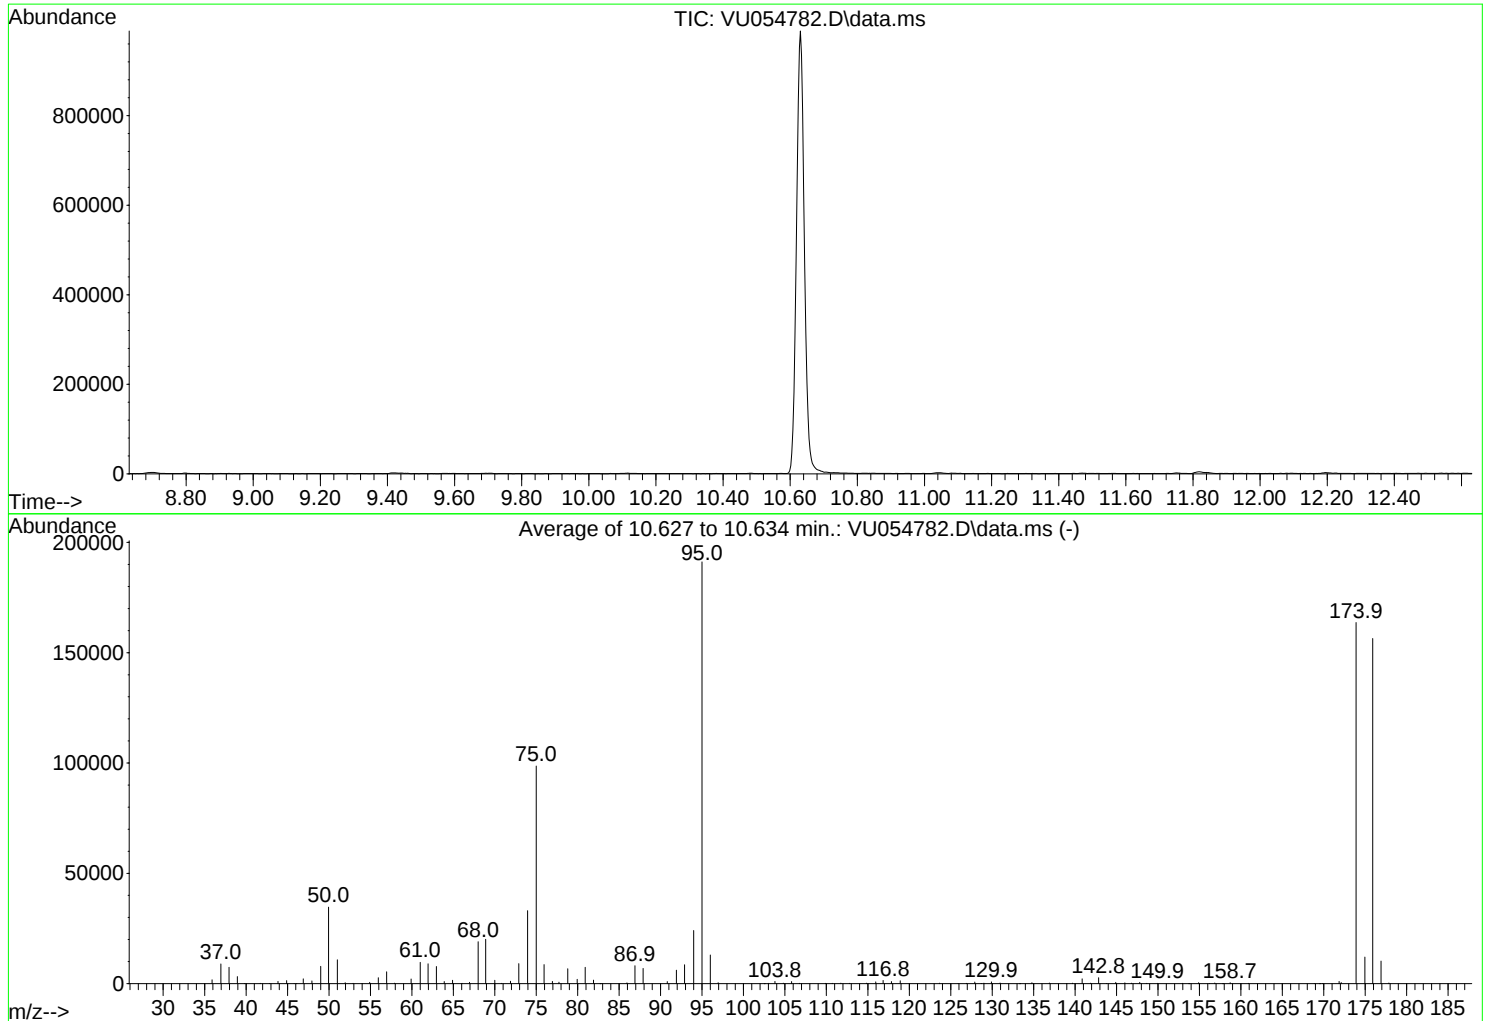

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	34677	PASS
75	95	30	80	51.6	98637	PASS
95	95	100	100	100.0	191189	PASS
96	95	5	9	6.8	12973	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.6	163669	PASS
175	174	5	9	7.4	12074	PASS
176	174	95	101	95.6	156437	PASS
177	176	5	9	6.5	10222	PASS

m/z	Abundance
39.80	233.0
43.70	467.0

Instrument :
MSVOA_U
ClientSampleId :
BFB033

m/z	Abundance
35.90	1828.0
37.00	9147.0
37.90	7777.0
39.00	3073.0
39.80	249.0
40.00	245.0
41.70	122.0
42.90	141.0
43.90	1485.0
44.90	1393.0
45.80	159.0
46.90	2181.0
47.90	1361.0
49.00	7673.0
49.90	35832.0
51.00	10874.0
51.90	472.0
52.90	190.0
54.90	593.0
55.90	2696.0
57.00	5459.0
57.90	210.0
59.90	2045.0
61.00	9412.0
62.00	9428.0
63.00	7826.0
63.90	1031.0
64.90	1443.0
66.00	161.0
67.00	618.0
68.00	19552.0
68.90	20024.0
70.00	1357.0
70.80	195.0
71.90	993.0
72.90	9150.0
74.00	33128.0
75.00	98384.0
75.90	9105.0
76.90	1068.0
77.80	698.0
78.80	6590.0
79.90	1992.0
80.90	7373.0
81.90	1563.0
82.90	159.0
86.00	354.0
86.90	8167.0
87.90	6482.0
90.80	919.0
91.90	6144.0
92.90	8500.0
94.00	23776.0
95.00	190784.0
96.00	12881.0
97.00	515.0
103.10	162.0
103.80	946.0
104.80	293.0
105.80	905.0
106.90	141.0
109.90	139.0
111.70	188.0
112.80	116.0
114.80	234.0
116.00	746.0
116.80	1390.0
117.80	1026.0
118.90	1227.0
123.60	207.0
126.90	103.0
127.90	709.0
128.70	242.0
129.10	220.0
129.90	814.0
130.90	284.0
134.80	351.0
136.90	264.0
139.00	115.0
139.70	198.0
140.80	2145.0
141.80	359.0
142.80	2426.0
144.90	648.0
146.00	342.0
146.80	211.0
147.80	532.0
148.70	140.0
150.00	170.0
153.00	113.0
154.90	489.0
156.20	135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB033

157.00	302.0
157.80	114.0
158.70	460.0
160.90	227.0
168.90	103.0
169.80	101.0
171.90	1495.0
173.90	159552.0
175.00	11890.0
175.90	153600.0
176.90	10203.0
177.80	275.0

Instrument :
MSVOA_U
ClientSampleId :
BFB033

m/z	Abundance
35.90	1829.0
37.00	9270.0
37.90	7586.0
38.90	3260.0
39.80	290.0
41.70	172.0
42.80	110.0
43.90	1519.0
44.90	1500.0
45.80	131.0
46.10	137.0
46.90	2241.0
47.90	1278.0
49.00	8052.0
49.90	35744.0
51.00	11222.0
51.90	454.0
52.90	171.0
54.00	108.0
54.90	607.0
56.00	2721.0
56.90	5496.0
57.90	256.0
59.90	2236.0
61.00	9908.0
61.90	9249.0
62.90	8077.0
63.90	997.0
64.90	1597.0
66.00	200.0
67.00	609.0
68.00	19640.0
68.90	20832.0
70.00	1607.0
70.80	176.0
71.90	1111.0
72.90	9377.0
73.90	33904.0
75.00	101616.0
75.90	8769.0
77.00	1060.0
77.80	708.0
78.80	6925.0
80.00	1996.0
80.90	7725.0
81.90	1655.0
83.00	144.0
86.00	377.0
86.90	8373.0
87.90	7109.0
90.80	972.0
91.90	6373.0
92.90	8776.0
94.00	24888.0
95.00	196928.0
96.00	13506.0
96.90	444.0
102.50	105.0
103.00	181.0
103.80	1024.0
104.80	241.0
105.80	980.0
106.70	177.0
109.90	167.0
110.70	182.0
111.70	194.0
112.80	184.0
114.80	276.0
115.90	800.0
116.90	1441.0
117.90	946.0
118.90	1381.0
123.70	198.0
125.90	140.0
126.90	133.0
127.90	713.0
129.00	255.0
129.90	758.0
130.90	335.0
134.80	433.0
136.90	291.0
139.00	101.0
139.70	202.0
140.90	2208.0
141.90	305.0
142.90	2706.0
144.90	583.0
146.00	383.0
146.80	246.0
147.80	621.0
148.60	110.0
150.00	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB033

152.90	168.0
153.70	104.0
154.90	468.0
156.80	303.0
158.70	511.0
160.90	178.0
168.80	107.0
169.80	117.0
171.80	1459.0
173.90	169280.0
174.90	12484.0
175.90	161664.0
176.90	10582.0
177.90	342.0

Instrument :
MSVOA_U
ClientSampleId :
BFB033

m/z	Abundance
35.90	1590.0
36.90	8326.0
38.00	6918.0
39.00	3149.0
39.80	332.0
41.70	144.0
43.90	1384.0
44.90	1375.0
46.90	2145.0
48.00	1128.0
49.00	7760.0
50.00	32456.0
51.00	10419.0
52.00	433.0
52.90	149.0
54.00	113.0
54.90	575.0
56.00	2615.0
56.90	5071.0
57.90	253.0
59.90	2141.0
61.00	9647.0
61.90	8412.0
62.90	7480.0
63.90	815.0
64.90	1600.0
66.10	183.0
66.90	554.0
68.00	17848.0
68.90	19504.0
70.00	1676.0
71.90	1179.0
72.90	8717.0
73.90	32248.0
75.00	95912.0
76.00	8129.0
76.90	993.0
77.70	672.0
78.80	6653.0
80.00	1801.0
80.90	7187.0
81.90	1522.0
82.70	106.0
85.90	328.0
86.90	7899.0
87.90	7125.0
90.80	886.0
91.90	5887.0
92.90	8501.0
94.00	23528.0
95.00	185856.0
96.00	12532.0
96.90	316.0
102.90	165.0
103.80	1039.0
104.80	205.0
105.80	1005.0
106.70	174.0
109.90	182.0
110.70	266.0
111.80	184.0
112.80	222.0
114.90	280.0
116.00	804.0
116.90	1465.0
117.90	851.0
118.90	1334.0
123.70	221.0
125.90	179.0
126.90	141.0
127.90	743.0
128.90	254.0
129.90	750.0
131.00	343.0
133.30	110.0
134.80	448.0
136.90	244.0
139.70	170.0
140.90	2176.0
142.90	2968.0
143.80	131.0
144.90	504.0
146.00	346.0
146.80	204.0
147.80	641.0
148.60	103.0
149.90	161.0
152.90	224.0
154.90	396.0
156.80	339.0
158.70	430.0
160.90	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB033

169.50	113.0
169.90	107.0
172.10	1450.0
173.90	162176.0
174.90	11849.0
175.90	154048.0
176.90	9882.0
177.90	350.0

Instrument :
MSVOA_U
ClientSampleId :
BFB033