




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071422\
 Data File : VU049718.D
 Acq On : 14 Jul 2022 14:41
 Operator : SY/MD
 Sample : N3678-15ME
 Misc : 5.90g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5B36ME

Manual IntegrationsAPPROVED

Quant Time: Jul 15 04:04:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 15 04:01:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

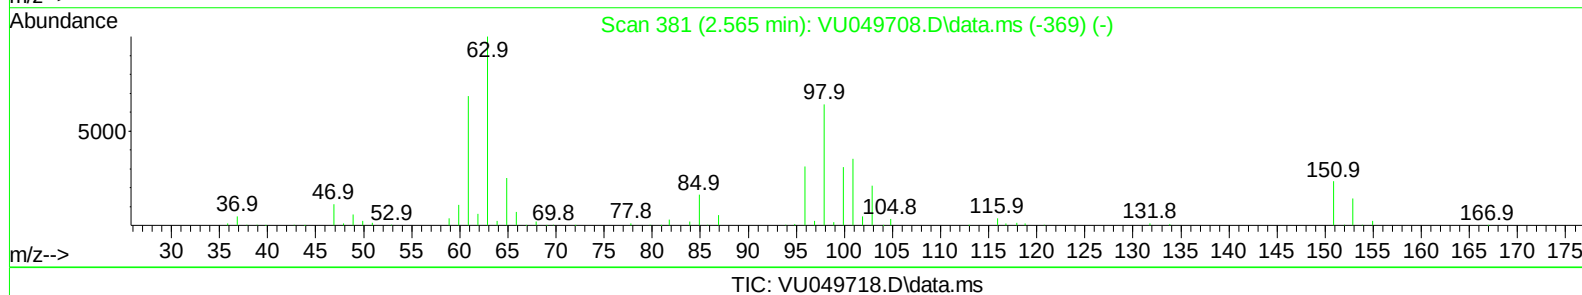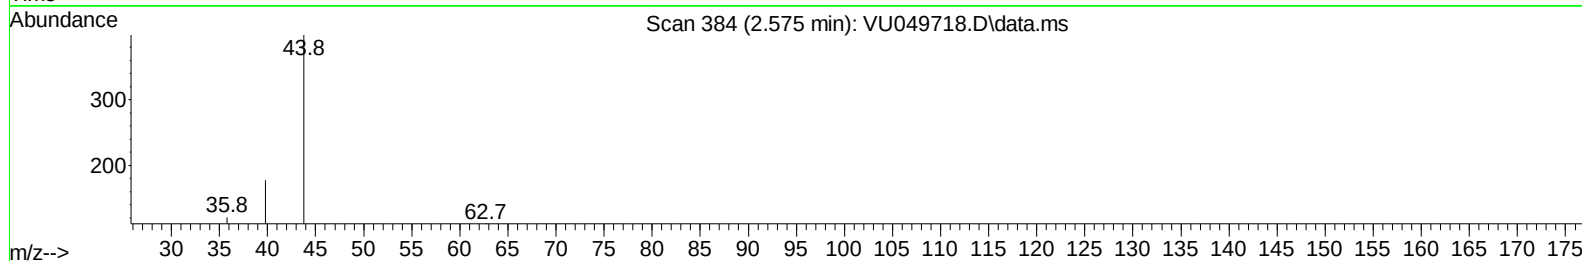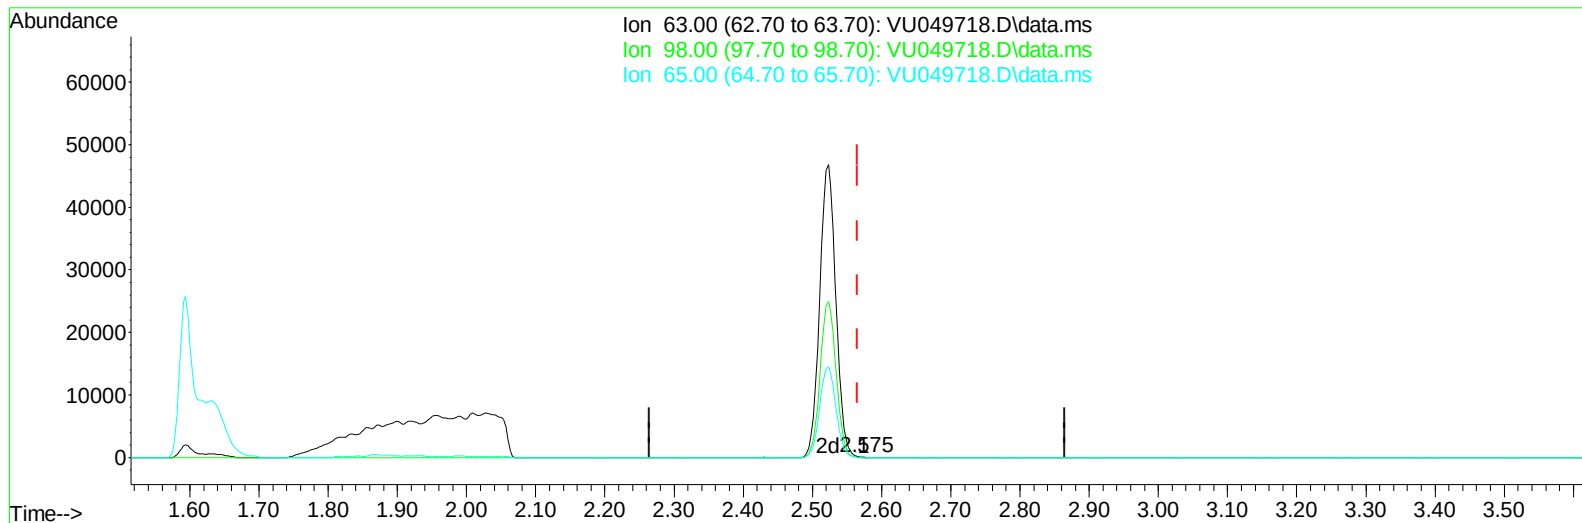

(11) 1,1-Dichloroethene-d2 (S)

2.575min (+ 0.010) 0.01 ug/L

response 21

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	69.30	0.00#
65.00	23.30	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071422\
 Data File : VU049718.D
 Acq On : 14 Jul 2022 14:41
 Operator : SY/MD
 Sample : N3678-15ME
 Misc : 5.90g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5B36ME

Manual IntegrationsAPPROVED

Quant Time: Jul 15 04:04:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 15 04:01:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

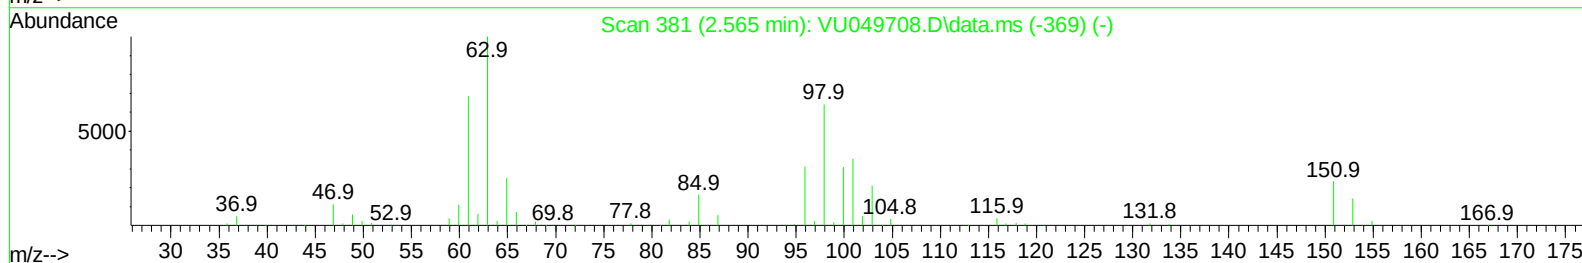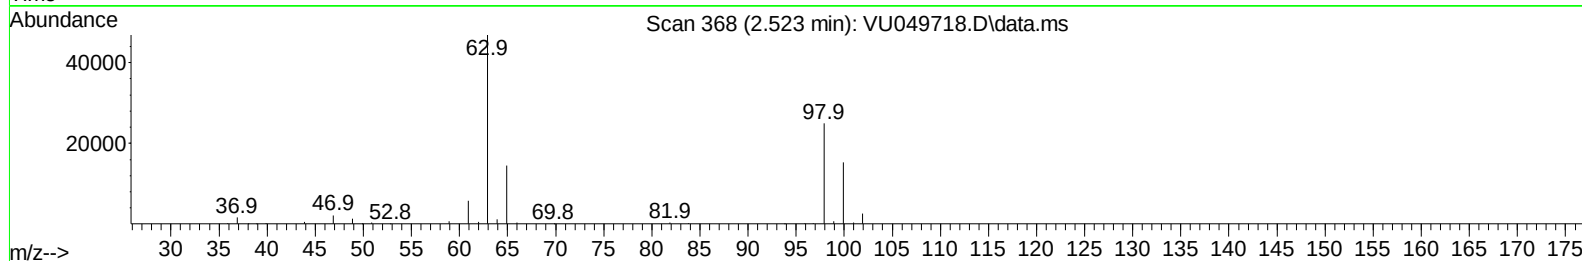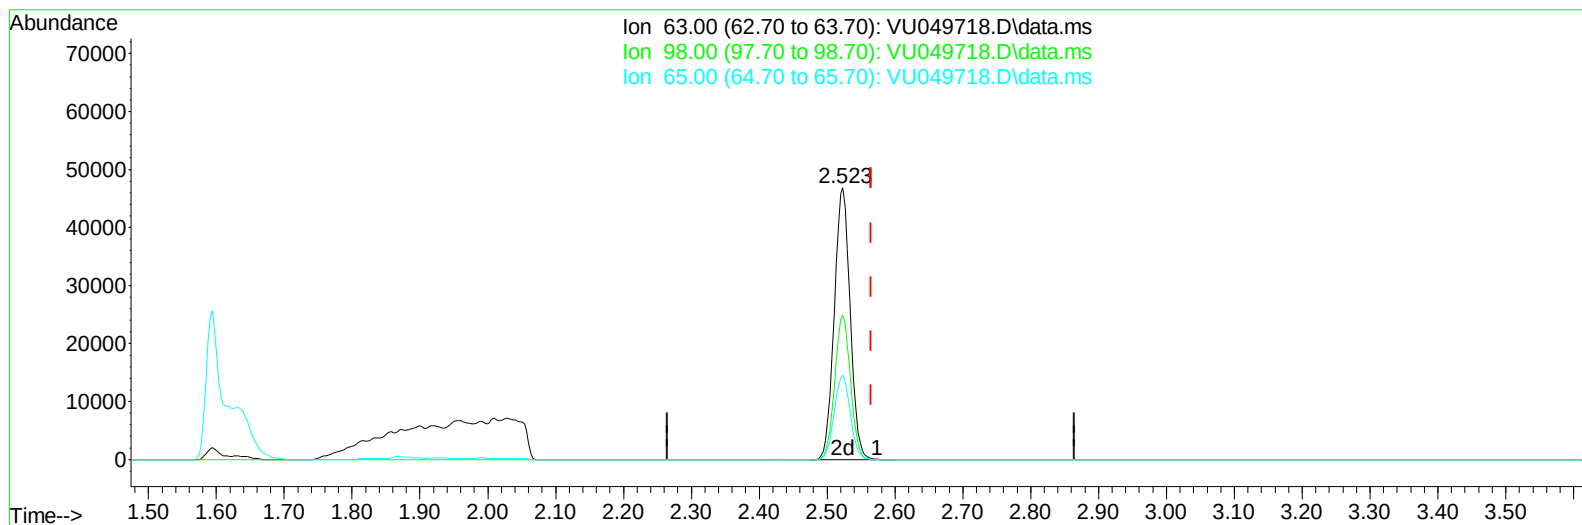

TIC: VU049718.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.523min (-0.042) 25.35 ug/L m

response 75968

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	69.30	0.00#
65.00	23.30	0.00#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071422\
 Data File : VU049718.D
 Acq On : 14 Jul 2022 14:41
 Operator : SY/MD
 Sample : N3678-15ME
 Misc : 5.90g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5B36ME

Manual IntegrationsAPPROVED

Quant Time: Jul 15 04:04:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 15 04:01:16 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	201037	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	198124	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	91672	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	39562	23.323	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	46.640%#	
7) Chloroethane-d5	1.871	69	23019	18.774	ug/L	-0.03
Spiked Amount 50.000	Range 70	- 130	Recovery	=	37.540%#	
11) 1,1-Dichloroethene-d2	2.523	63	75968m	25.355	ug/L	-0.04
Spiked Amount 50.000	Range 60	- 125	Recovery	=	50.700%#	
21) 2-Butanone-d5	4.636	46	163114	112.646	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	112.650%	
24) Chloroform-d	5.060	84	134537	44.781	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	89.560%	
26) 1,2-Dichloroethane-d4	5.697	65	98457	48.422	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	96.840%	
32) Benzene-d6	5.719	84	245856	40.847	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	81.700%	
36) 1,2-Dichloropropane-d6	6.687	67	93408	46.138	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	92.280%	
41) Toluene-d8	7.896	98	209442	39.958	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	79.920%#	
43) trans-1,3-Dichloroprop...	8.179	79	35178	41.241	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	82.480%	
47) 2-Hexanone-d5	8.648	63	105092	115.399	ug/L	0.02
Spiked Amount 100.000	Range 45	- 130	Recovery	=	115.400%	
56) 1,1,2,2-Tetrachloroeth...	10.761	84	148979	52.592	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	105.180%	
66) 1,2-Dichlorobenzene-d4	12.195	152	84916	49.129	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	98.260%	
Target Compounds						
13) Acetone	2.645	43	3409	2.477	ug/L	Qvalue 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071422\
Data File : VU049718.D
Acq On : 14 Jul 2022 14:41
Operator : SY/MD
Sample : N3678-15ME
Misc : 5.90g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5B36ME

Manual IntegrationsAPPROVED

Quant Time: Jul 15 04:04:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 15 04:01:16 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/15/2022
Supervised By :Mahesh Dadoda 07/15/2022

