

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071422\
 Data File : VU049717.D
 Acq On : 14 Jul 2022 14:18
 Operator : SY/MD
 Sample : N3678-11ME
 Misc : 6.41g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5B30ME

Quant Time: Jul 15 04:03:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 15 04:01:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	223369	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	209606	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	93843	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	36744	19.496	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	39.000%#	
7) Chloroethane-d5	1.883	69	24962	18.323	ug/L	-0.02
Spiked Amount	50.000	Range 70 - 130	Recovery	=	36.640%#	
11) 1,1-Dichloroethene-d2	2.526	63	89012	26.738	ug/L	-0.04
Spiked Amount	50.000	Range 60 - 125	Recovery	=	53.480%#	
21) 2-Butanone-d5	4.639	46	167072	103.844	ug/L	0.02
Spiked Amount	100.000	Range 40 - 130	Recovery	=	103.840%	
24) Chloroform-d	5.060	84	144045	43.153	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	86.300%	
26) 1,2-Dichloroethane-d4	5.700	65	103619	45.866	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	91.740%	
32) Benzene-d6	5.719	84	263058	41.311	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	82.620%	
36) 1,2-Dichloropropane-d6	6.690	67	98867	46.160	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	92.320%	
41) Toluene-d8	7.896	98	226778	40.895	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	81.800%	
43) trans-1,3-Dichloroprop...	8.182	79	36408	40.345	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	80.700%	
47) 2-Hexanone-d5	8.658	63	103984	107.928	ug/L	0.03
Spiked Amount	100.000	Range 45 - 130	Recovery	=	107.930%	
56) 1,1,2,2-Tetrachloroeth...	10.764	84	146896	49.016	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	98.040%	
66) 1,2-Dichlorobenzene-d4	12.195	152	88687	50.124	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	100.240%	
Target Compounds						
20) cis-1,2-Dichloroethene	4.658	96	3418	1.741	ug/L	Qvalue 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071422\
Data File : VU049717.D
Acq On : 14 Jul 2022 14:18
Operator : SY/MD
Sample : N3678-11ME
Misc : 6.41g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5B30ME

Quant Time: Jul 15 04:03:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 15 04:01:16 2022
Response via : Initial Calibration

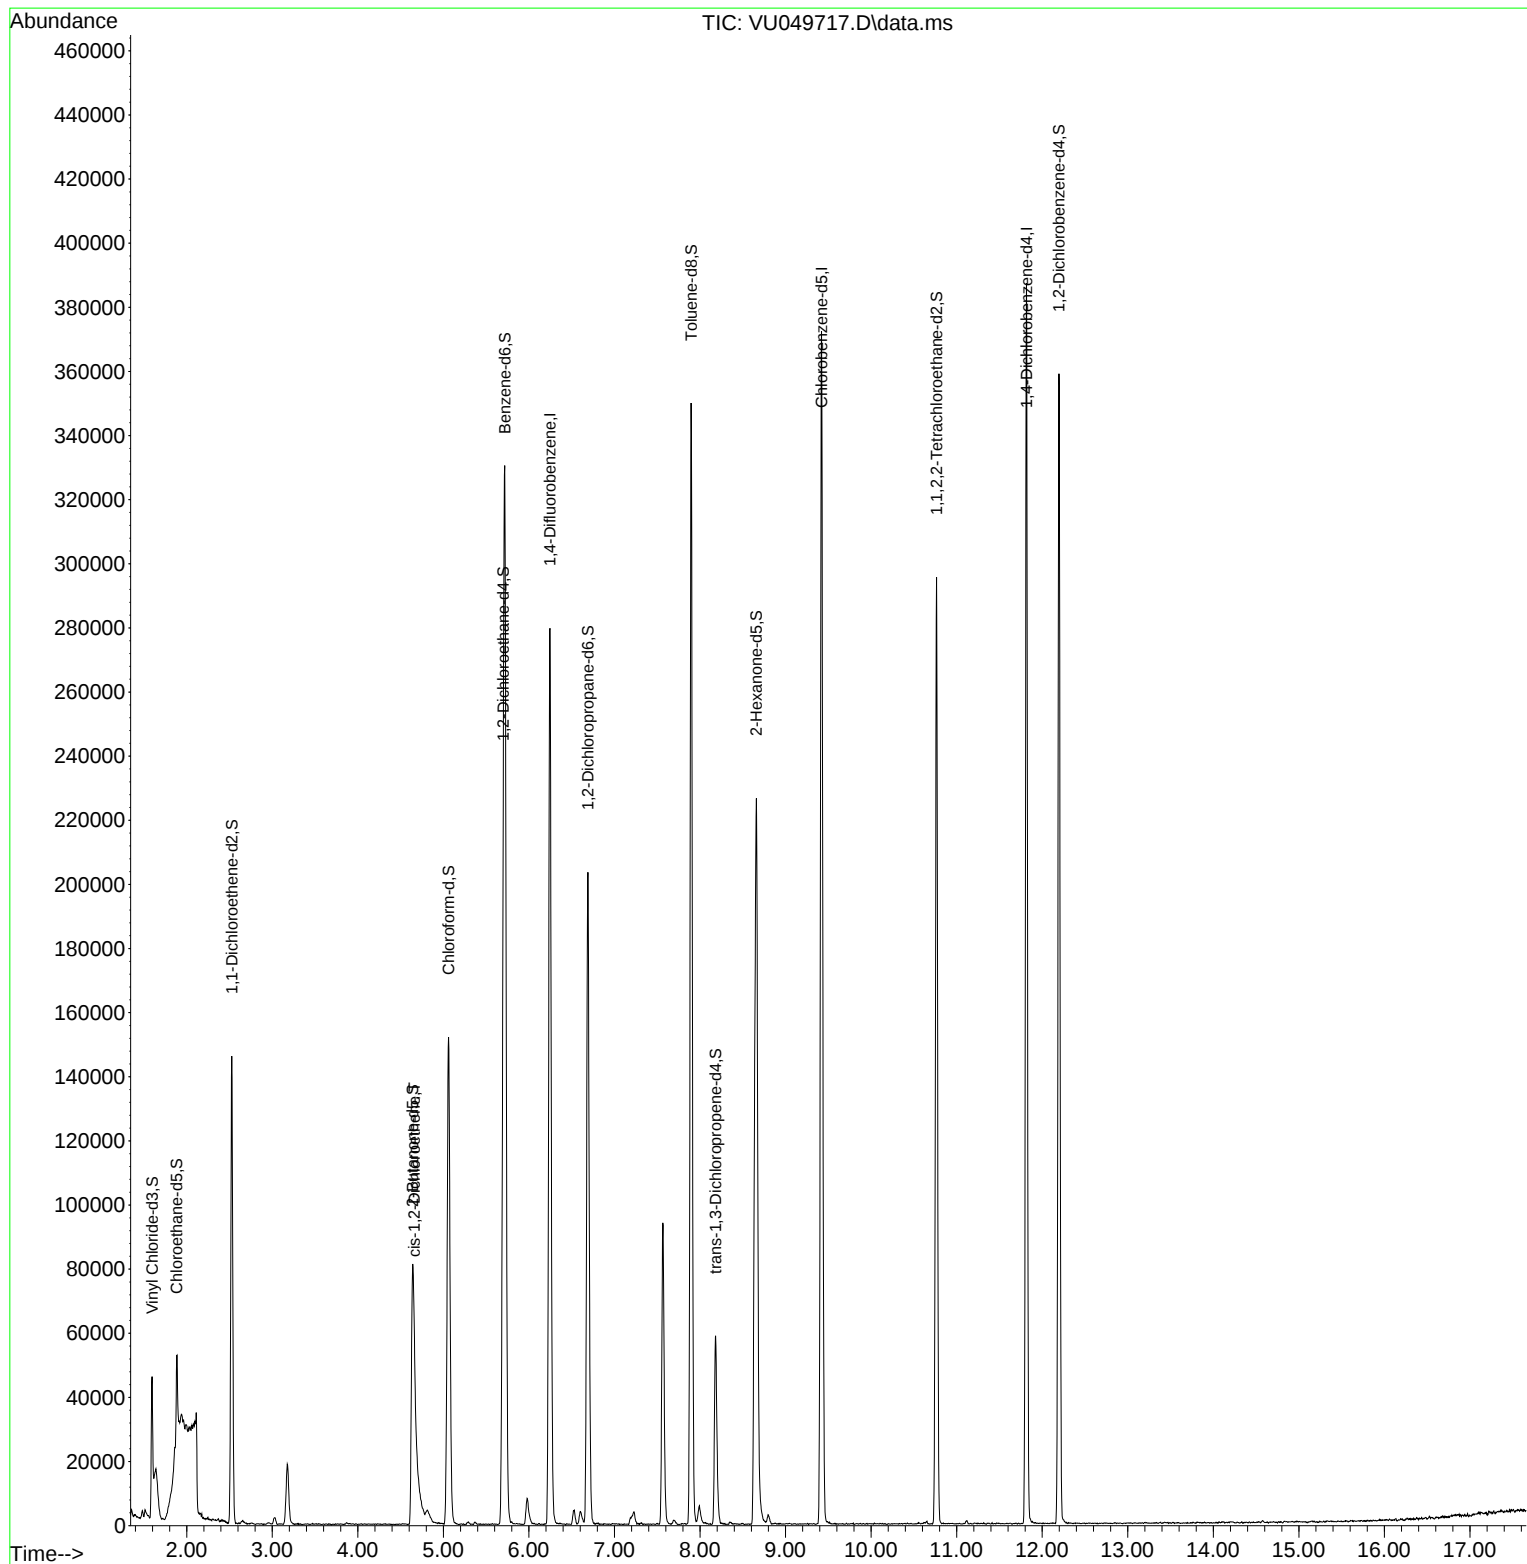

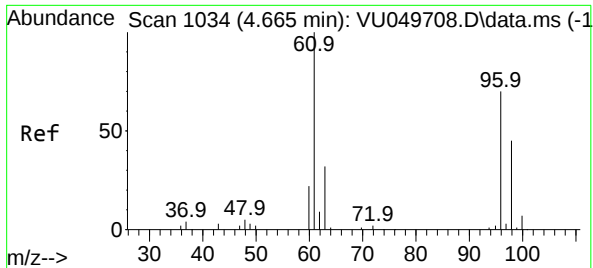

#20
 cis-1,2-Dichloroethene
 Concen: 1.741 ug/L
 RT: 4.658 min Scan# 10
 Delta R.T. -0.006 min
 Lab File: VU049717.D
 Acq: 14 Jul 2022 14:18

Instrument :
 MSVOA_U
 ClientSampleId :
 F5B30ME

Tgt Ion: 96 Resp: 3418
 Ion Ratio Lower Upper
 96 100
 61 121.0 101.1 187.7
 68 0.0 0.0 0.0

