

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071422\
 Data File : VU049718.D
 Acq On : 14 Jul 2022 14:41
 Operator : SY/MD
 Sample : N3678-15ME
 Misc : 5.90g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5B36ME

Quant Time: Jul 15 04:04:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 15 04:01:16 2022
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Krupa Patel 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	201037	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	198124	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	91672	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	39562	23.323	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	46.640%#		
7) Chloroethane-d5	1.871	69	23019	18.774	ug/L	-0.03
Spiked Amount 50.000	Range 70 - 130		Recovery =	37.540%#		
11) 1,1-Dichloroethene-d2	2.523	63	75968m	25.355	ug/L	-0.04
Spiked Amount 50.000	Range 60 - 125		Recovery =	50.700%#		
21) 2-Butanone-d5	4.636	46	163114	112.646	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	112.650%		
24) Chloroform-d	5.060	84	134537	44.781	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.560%		
26) 1,2-Dichloroethane-d4	5.697	65	98457	48.422	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.840%		
32) Benzene-d6	5.719	84	245856	40.847	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.700%		
36) 1,2-Dichloropropane-d6	6.687	67	93408	46.138	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.280%		
41) Toluene-d8	7.896	98	209442	39.958	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	79.920%#		
43) trans-1,3-Dichloroprop...	8.179	79	35178	41.241	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.480%		
47) 2-Hexanone-d5	8.648	63	105092	115.399	ug/L	0.02
Spiked Amount 100.000	Range 45 - 130		Recovery =	115.400%		
56) 1,1,2,2-Tetrachloroeth...	10.761	84	148979	52.592	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	105.180%		
66) 1,2-Dichlorobenzene-d4	12.195	152	84916	49.129	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.260%		
Target Compounds					Qvalue	
13) Acetone	2.645	43	3409	2.477	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071422\
Data File : VU049718.D
Acq On : 14 Jul 2022 14:41
Operator : SY/MD
Sample : N3678-15ME
Misc : 5.90g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 13 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
F5B36ME

Quant Time: Jul 15 04:04:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 15 04:01:16 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Krupa Patel 07/15/2022
Supervised By :Mahesh Dadoda 07/15/2022

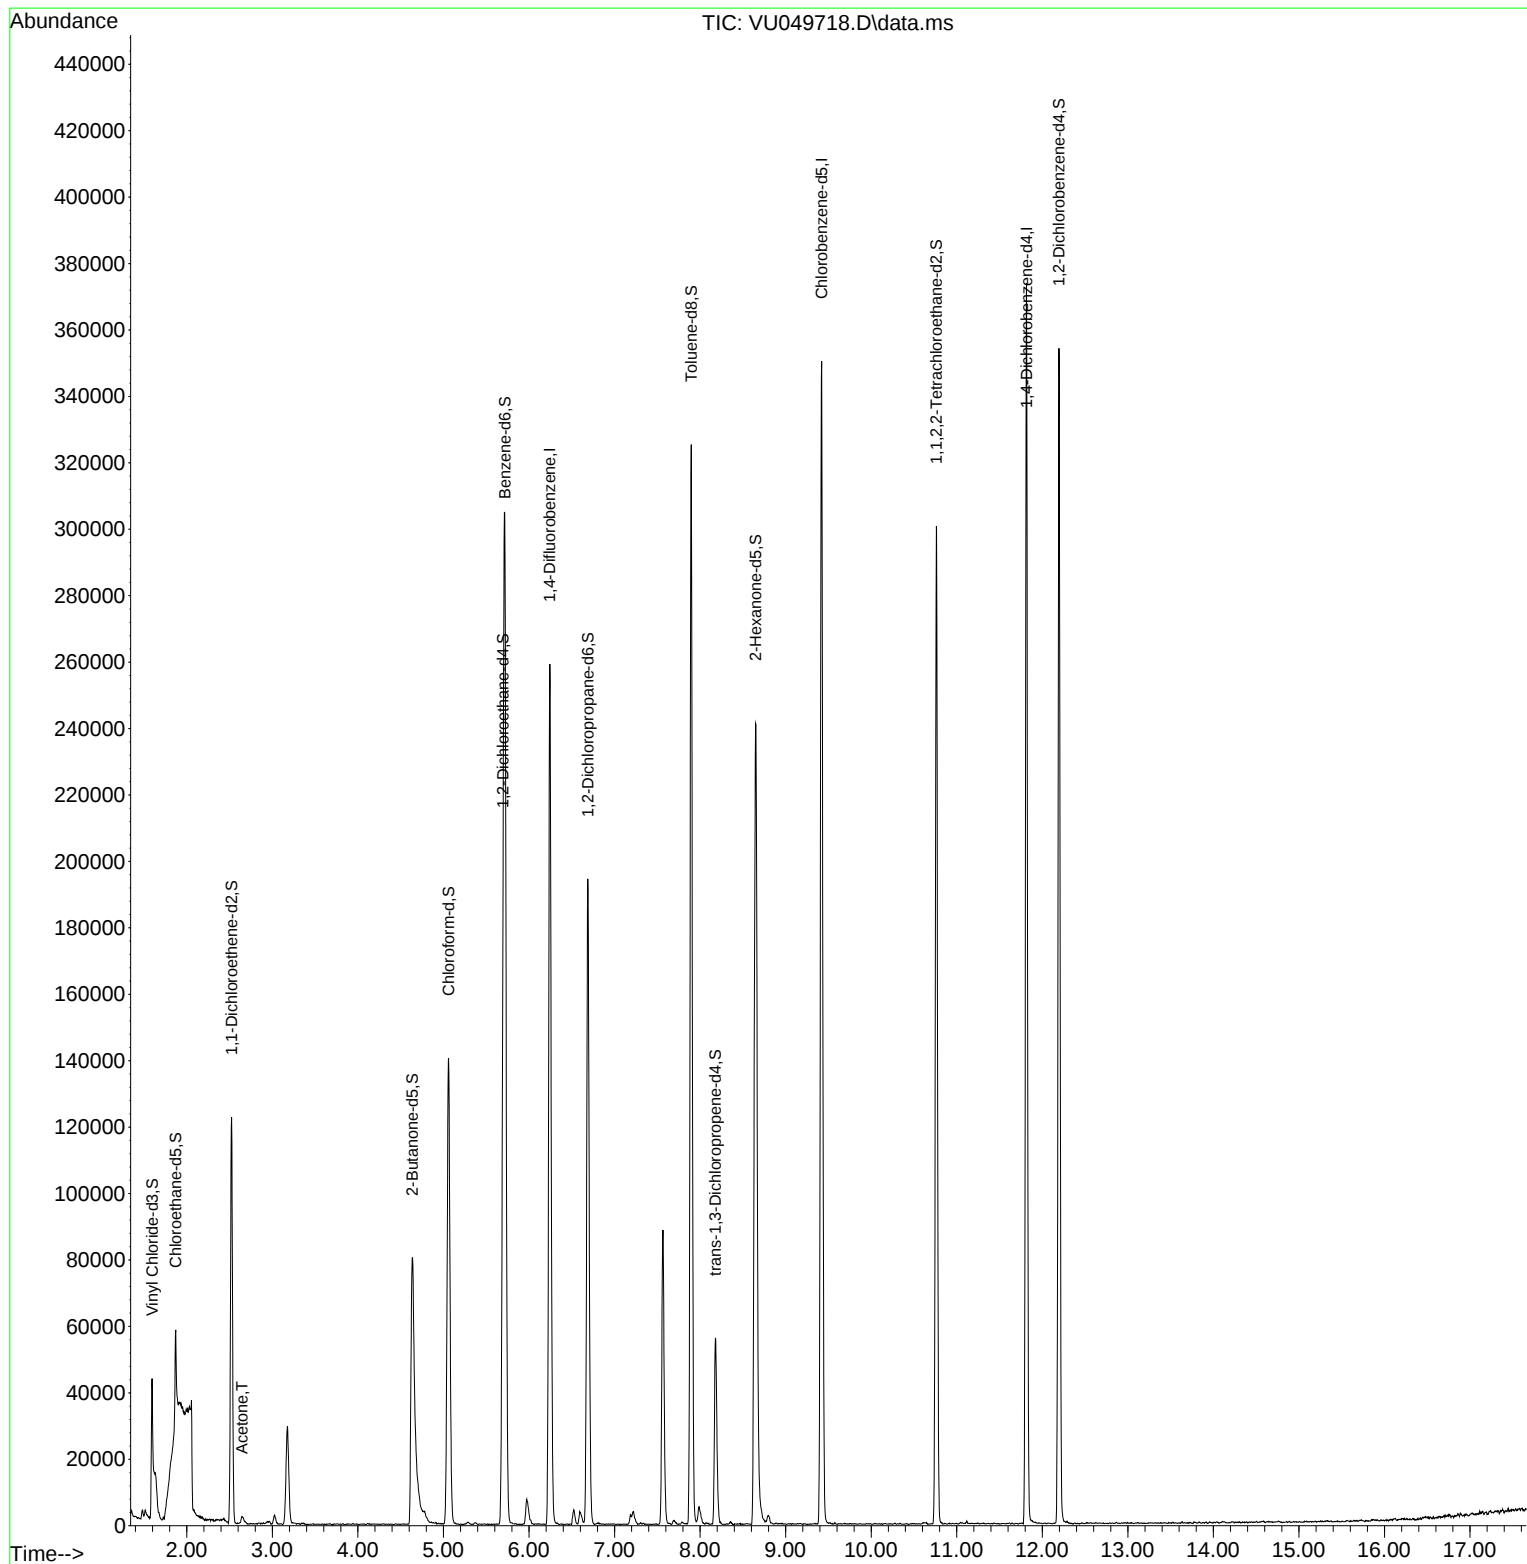

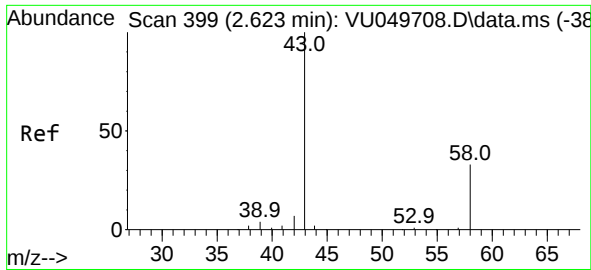

#13
 Acetone
 Concen: 2.477 ug/L
 RT: 2.645 min Scan# 406
 Delta R.T. 0.023 min
 Lab File: VU049718.D
 Acq: 14 Jul 2022 14:41

Instrument :
 MSVOA_U
 ClientSampleId :
 F5B36ME

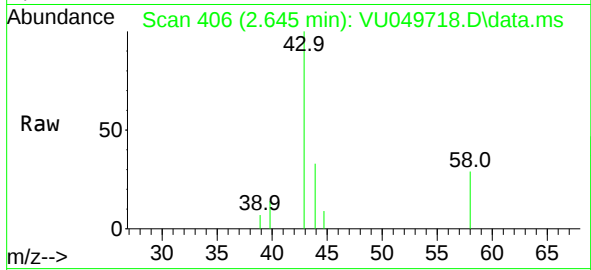

Tgt Ion: 43 Resp: 3409
 Ion Ratio Lower Upper
 43 100
 58 24.7 0.0 61.4

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 07/15/2022
 Supervised By :Mahesh Dadoda 07/15/2022

