
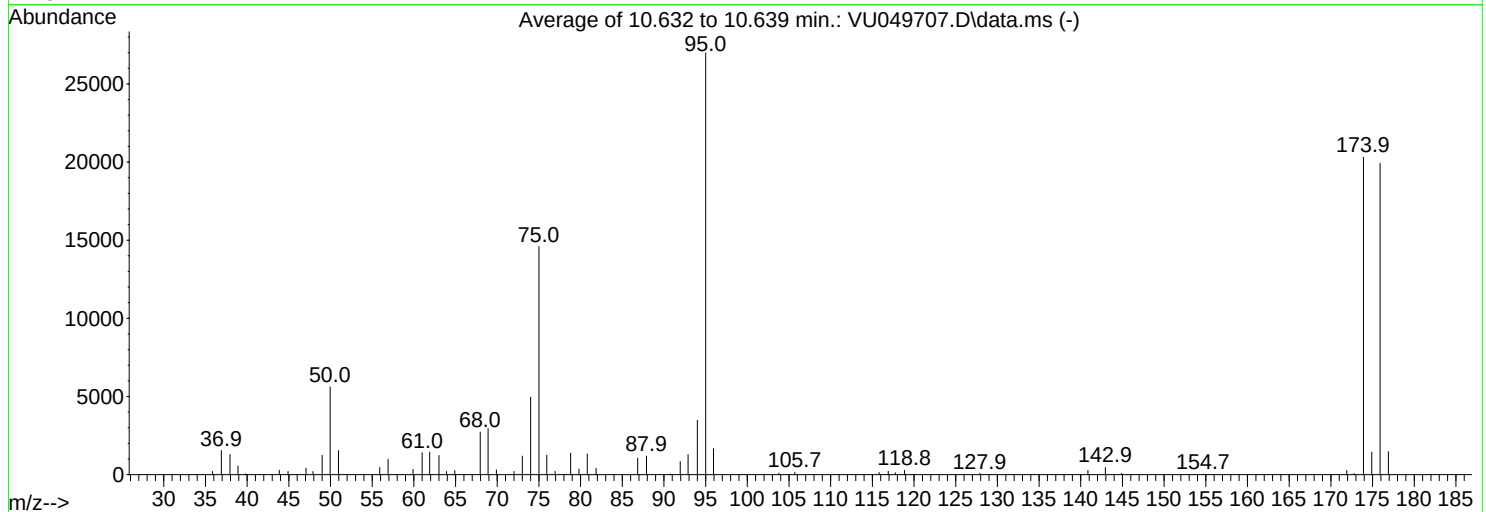


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071422\
 Data File : VU049707.D
 Acq On : 14 Jul 2022 08:46
 Operator : SY/MD
 Sample : BFB104
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB104

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis
 Last Update : Fri Jul 15 04:01:16 2022

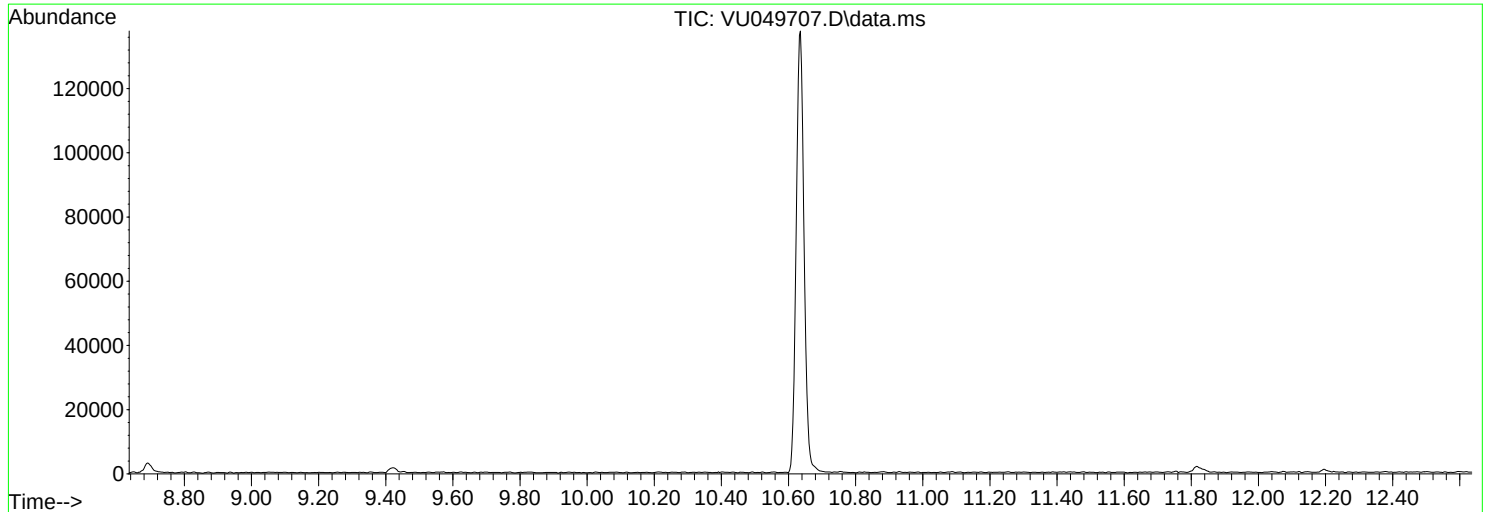

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	5620	PASS
75	95	30	80	54.1	14599	PASS
95	95	100	100	100.0	26987	PASS
96	95	5	9	6.2	1662	PASS
173	174	0.00	2	0.3	68	PASS
174	95	50	120	75.2	20304	PASS
175	174	5	9	7.1	1442	PASS
176	174	95	101	98.1	19920	PASS
177	176	5	9	7.4	1466	PASS

m/z	Abundance
39.70	174.0
44.00	259.0

Instrument :
MSVOA_U
ClientSampleId :
BFB104

m/z	Abundance
35.90	229.0
36.90	1457.0
38.00	1297.0
38.90	522.0
39.90	229.0
43.90	628.0
44.90	234.0
47.00	398.0
47.80	171.0
49.00	1409.0
50.00	5987.0
50.90	1619.0
55.90	492.0
56.90	1027.0
59.80	335.0
61.00	1449.0
61.90	1582.0
63.00	1293.0
63.90	162.0
64.90	260.0
68.00	2794.0
68.90	3193.0
69.90	321.0
72.00	210.0
73.00	1246.0
74.00	5064.0
75.00	15128.0
75.90	1400.0
77.00	229.0
78.10	105.0
78.80	1412.0
79.80	323.0
80.80	1292.0
81.90	412.0
86.80	1016.0
87.90	1167.0
90.80	124.0
92.00	851.0
92.90	1381.0
94.00	3765.0
95.00	27352.0
95.90	1685.0
103.80	171.0
105.80	150.0
115.80	120.0
116.90	213.0
117.80	123.0
118.90	227.0
127.90	129.0
140.90	260.0
143.00	480.0
144.90	122.0
154.70	109.0
171.90	298.0
173.90	20160.0
174.90	1493.0
175.90	19800.0
176.90	1453.0

Instrument :
MSVOA_U
ClientSampleId :
BFB104

m/z	Abundance
35.90	210.0
36.90	1617.0
37.90	1315.0
38.90	584.0
39.90	248.0
43.80	560.0
44.90	221.0
47.10	453.0
47.90	215.0
49.00	1277.0
50.00	5801.0
51.00	1621.0
55.90	466.0
56.90	1055.0
59.90	331.0
61.00	1473.0
61.90	1474.0
63.00	1267.0
63.90	216.0
64.90	270.0
67.90	2806.0
68.90	2949.0
69.90	321.0
72.00	206.0
73.00	1239.0
74.00	5069.0
75.00	14967.0
75.90	1286.0
77.00	224.0
78.80	1426.0
79.80	369.0
80.80	1367.0
81.80	418.0
86.80	1062.0
87.90	1249.0
91.90	860.0
92.90	1353.0
94.00	3555.0
95.00	27824.0
96.00	1735.0
103.80	123.0
105.70	157.0
115.80	157.0
116.90	228.0
117.70	130.0
118.90	304.0
127.90	115.0
140.90	265.0
143.00	469.0
144.90	118.0
171.90	273.0
172.80	203.0
173.90	20968.0
174.90	1475.0
175.90	20432.0
176.90	1526.0

Instrument :
MSVOA_U
ClientSampleId :
BFB104

m/z	Abundance
35.80	189.0
36.90	1558.0
37.90	1271.0
38.90	564.0
39.90	210.0
43.90	435.0
44.90	161.0
47.00	406.0
48.00	240.0
49.00	1021.0
49.90	5072.0
51.00	1378.0
55.90	428.0
56.90	876.0
60.00	348.0
61.00	1285.0
61.90	1261.0
63.00	1139.0
63.90	249.0
64.90	261.0
67.90	2558.0
68.90	2711.0
69.90	276.0
72.00	193.0
73.00	1070.0
74.00	4722.0
75.00	13703.0
76.00	1076.0
76.90	187.0
78.80	1293.0
79.80	389.0
80.80	1289.0
81.80	400.0
86.90	1088.0
87.90	1136.0
91.90	806.0
92.90	1116.0
94.00	3103.0
95.00	25784.0
96.00	1567.0
105.60	175.0
115.80	139.0
116.90	202.0
117.70	110.0
118.80	306.0
140.80	291.0
142.90	437.0
171.90	234.0
173.90	19784.0
174.90	1359.0
175.90	19528.0
176.90	1419.0

Instrument :
MSVOA_U
ClientSampleId :
BFB104