


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU071519\
 Data File : VU033243.D
 Acq On : 15 Jul 2019 08:54
 Operator : JC/SP
 Sample : BFB35
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB35

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071219WMA.M
 Title : VOC Analysis
 Last Update : Tue Jul 16 01:46:18 2019

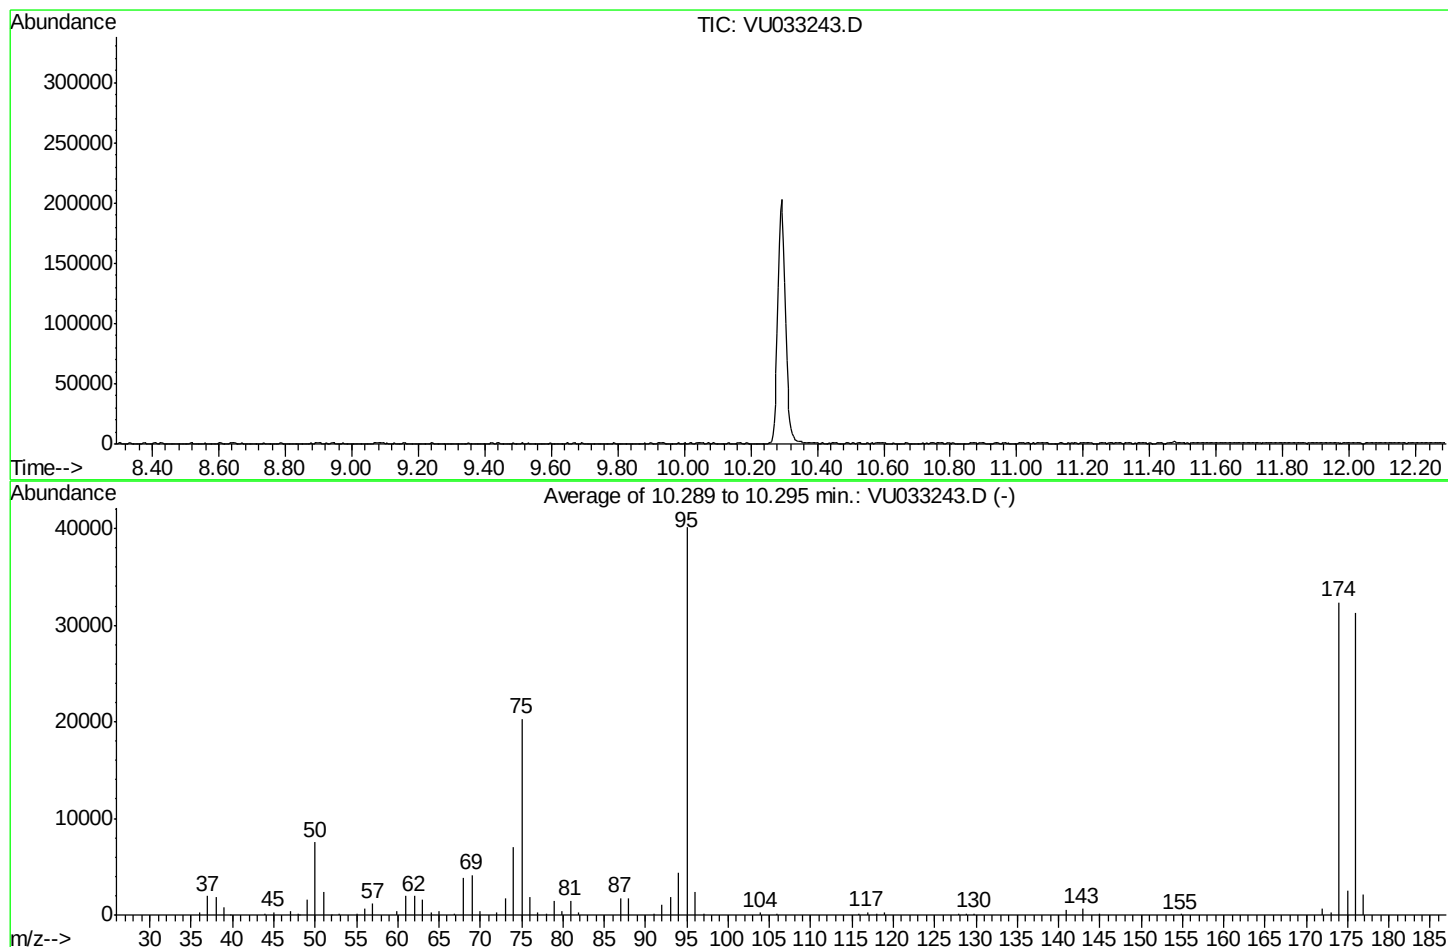

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	7543	PASS
75	95	30	80	50.6	20325	PASS
95	95	100	100	100.0	40136	PASS
96	95	5	9	5.9	2351	PASS
173	174	0.00	2	0.6	204	PASS
174	95	50	120	80.6	32360	PASS
175	174	5	9	7.6	2461	PASS
176	174	95	101	96.6	31250	PASS
177	176	5	9	6.9	2154	PASS

Scan 2850 (10.254 min): VU033243.D
BFB35

m/z	Abundance
39.90	206.0
43.90	423.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35

m/z	Abundance
36.00	336.0
37.00	1918.0
38.00	1948.0
39.00	739.0
39.80	216.0
44.00	591.0
45.00	347.0
47.10	429.0
47.90	237.0
49.00	1638.0
50.00	7657.0
51.00	2249.0
56.00	639.0
57.00	1087.0
59.80	378.0
61.00	2041.0
62.10	1965.0
63.00	1611.0
64.00	286.0
65.10	387.0
66.90	114.0
68.00	3842.0
69.00	4123.0
70.00	418.0
72.00	276.0
73.00	1743.0
74.00	7032.0
75.00	20576.0
76.00	1885.0
76.90	245.0
78.00	129.0
78.90	1379.0
79.90	414.0
80.90	1472.0
82.00	272.0
87.00	1746.0
88.00	1669.0
91.00	164.0
92.00	1101.0
93.00	1723.0
94.00	4454.0
95.00	39448.0
96.00	2288.0
97.00	122.0
103.90	240.0
105.90	183.0
115.80	159.0
116.90	313.0
117.90	137.0
118.90	214.0
127.90	152.0
128.80	135.0
129.80	175.0
140.90	473.0
142.90	627.0
144.90	117.0
154.90	104.0
171.90	646.0
174.00	31464.0
175.00	2370.0
176.00	30288.0
177.00	2123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35

m/z	Abundance
35.90	335.0
37.00	2030.0
38.00	1973.0
39.00	831.0
39.80	218.0
44.00	629.0
45.00	308.0
47.00	400.0
47.90	215.0
49.00	1713.0
50.00	7819.0
51.00	2399.0
52.00	104.0
52.90	106.0
55.00	108.0
56.00	673.0
57.00	1185.0
59.90	397.0
61.00	1990.0
62.00	2032.0
63.00	1640.0
64.10	283.0
65.00	392.0
66.90	105.0
68.00	4018.0
69.00	4256.0
70.00	436.0
72.00	307.0
73.00	1774.0
74.00	7194.0
75.00	20920.0
76.00	1913.0
77.00	285.0
78.00	160.0
78.90	1469.0
79.90	424.0
80.90	1486.0
81.90	286.0
87.00	1839.0
88.00	1782.0
90.90	168.0
92.00	1163.0
93.00	1862.0
94.00	4536.0
95.00	41472.0
96.00	2400.0
97.00	114.0
103.90	269.0
105.80	158.0
115.80	138.0
116.90	325.0
117.90	139.0
118.90	211.0
127.90	171.0
128.80	118.0
129.80	201.0
140.90	491.0
142.90	685.0
144.90	114.0
154.80	109.0
171.90	707.0
174.00	33424.0
175.00	2532.0
176.00	32232.0
177.00	2219.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35

m/z	Abundance
35.90	284.0
37.00	1872.0
38.00	1808.0
38.90	840.0
39.80	229.0
44.00	604.0
45.00	305.0
46.90	324.0
48.10	175.0
49.00	1603.0
50.00	7155.0
51.00	2369.0
52.00	103.0
53.00	115.0
55.00	129.0
56.00	601.0
57.00	1135.0
59.90	349.0
60.90	1825.0
62.00	1883.0
63.00	1605.0
64.10	273.0
65.00	409.0
68.00	3745.0
69.00	3957.0
70.00	397.0
72.00	302.0
73.00	1692.0
74.00	6764.0
75.00	19480.0
76.00	1706.0
76.90	276.0
78.00	170.0
78.90	1450.0
79.90	442.0
80.90	1435.0
81.90	278.0
87.00	1777.0
88.00	1723.0
90.90	143.0
92.00	1074.0
93.00	1805.0
94.00	4283.0
95.00	39488.0
96.00	2365.0
103.90	240.0
105.80	125.0
115.80	109.0
116.90	296.0
118.00	181.0
119.00	222.0
127.90	165.0
129.80	182.0
140.90	496.0
142.90	601.0
154.80	101.0
172.00	671.0
173.00	612.0
174.00	32192.0
175.00	2481.0
176.00	31232.0
176.90	2121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB35