

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071520\
 Data File : VU039497.D
 Acq On : 15 Jul 2020 14:12
 Operator : SY/MD
 Sample : L3292-01DL 50X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFT88DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.607	75	83	93	rVB	31653	35727	8.06%	1.022%
2	1.925	173	182	196	rBV	37952	51330	11.58%	1.469%
3	2.581	374	386	403	rBV2	62471	108169	24.41%	3.095%
4	3.060	523	535	552	rVB4	22527	43037	9.71%	1.231%
5	4.652	1015	1030	1068	rBV	62605	195401	44.09%	5.591%
6	5.083	1148	1164	1189	rVB	58039	137581	31.05%	3.937%
7	5.739	1342	1368	1392	rBV2	120839	319620	72.13%	9.146%
8	6.263	1515	1531	1549	rBV	126933	239773	54.11%	6.861%
9	6.555	1610	1622	1636	rBV2	38633	72679	16.40%	2.080%
10	6.703	1651	1668	1686	rVB2	79720	154406	34.84%	4.418%
11	7.575	1927	1939	1953	rBV2	42356	72661	16.40%	2.079%
12	7.906	2029	2042	2059	rBV	142966	240596	54.29%	6.885%
13	8.189	2118	2130	2147	rBV2	26022	45316	10.23%	1.297%
14	8.559	2233	2245	2258	rBV2	221669	371449	83.82%	10.629%
15	8.642	2259	2271	2307	rVB	229613	443147	100.00%	12.680%
16	9.420	2500	2513	2538	rBV	185733	309043	69.74%	8.843%
17	10.758	2917	2929	2942	rBV	68072	110759	24.99%	3.169%
18	10.893	2961	2971	2983	rVB2	6367	10529	2.38%	0.301%
19	11.809	3245	3256	3273	rVB	177653	295163	66.61%	8.446%
20	12.189	3362	3374	3389	rBV	150062	238355	53.79%	6.820%


Sum of corrected areas: 3494741

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU071520\
Data File : VU039497.D
Acq On : 15 Jul 2020 14:12
Operator : SY/MD
Sample : L3292-01DL 50X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFT88DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

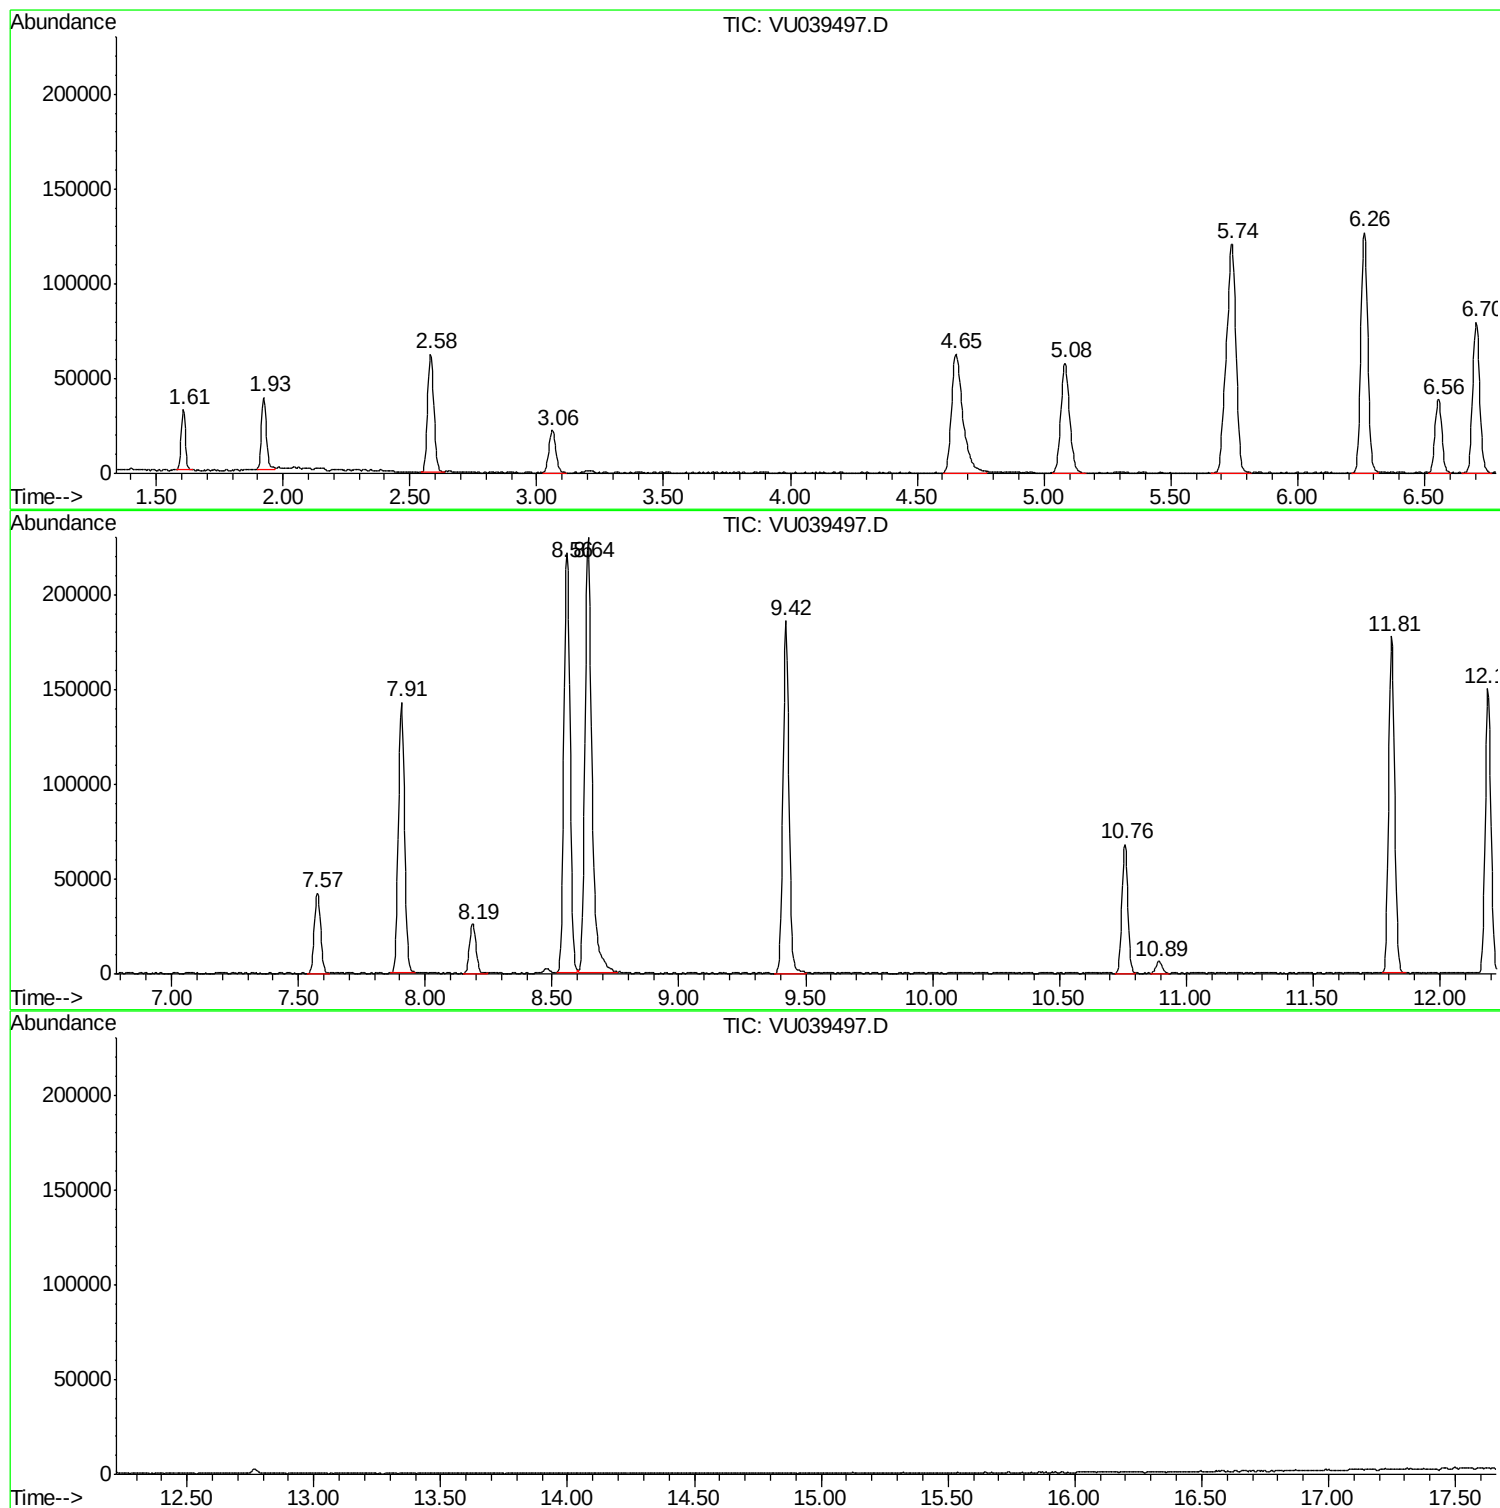

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071520\
Data File : VU039497.D
Acq On : 15 Jul 2020 14:12
Operator : SY/MD
Sample : L3292-01DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFT88DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071520\
Data File : VU039497.D
Acq On : 15 Jul 2020 14:12
Operator : SY/MD
Sample : L3292-01DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFT88DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc