


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU071520\
 Data File : VU039494.D
 Acq On : 15 Jul 2020 08:25
 Operator : SY/MD
 Sample : BFB02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB02

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Jul 16 04:09:55 2020

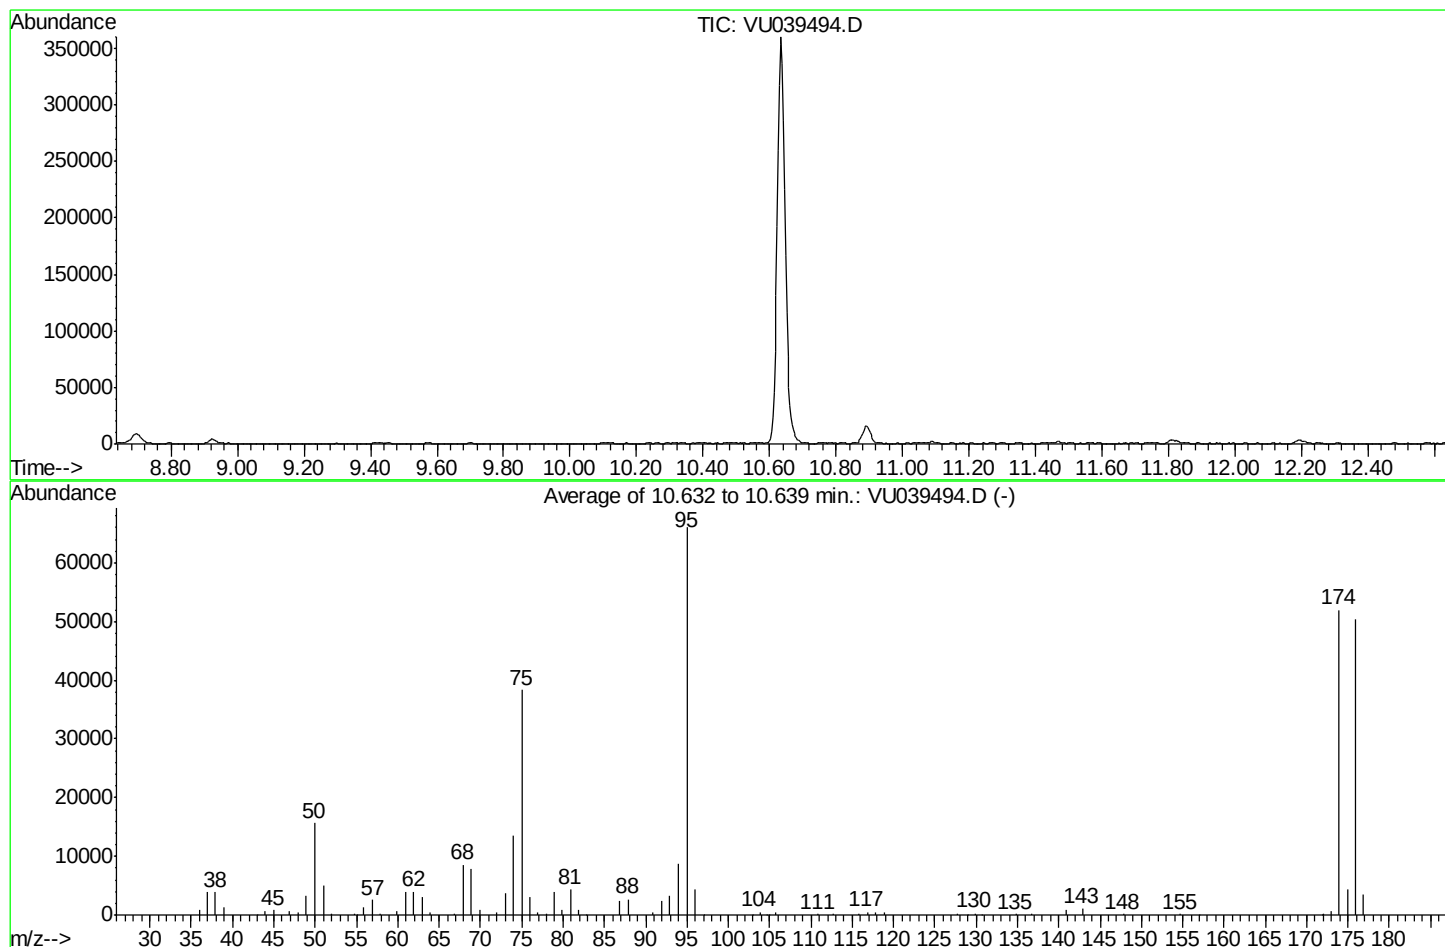

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.8	15705	PASS
75	95	30	80	58.1	38370	PASS
95	95	100	100	100.0	66064	PASS
96	95	5	9	6.6	4343	PASS
173	174	0.00	2	1.1	590	PASS
174	95	50	120	78.8	52026	PASS
175	174	5	9	8.4	4349	PASS
176	174	95	101	96.9	50405	PASS
177	176	5	9	6.9	3453	PASS

m/z	Abundance
36.00	1000.0
37.00	3978.0
38.00	3962.0
38.90	1349.0
39.80	187.0
43.00	105.0
44.00	877.0
45.00	899.0
46.80	608.0
47.90	597.0
48.90	3372.0
49.90	16154.0
51.00	5260.0
51.90	181.0
54.70	246.0
55.90	1452.0
57.00	2742.0
57.90	184.0
59.90	601.0
60.90	4136.0
62.00	4196.0
62.90	3201.0
64.00	454.0
66.90	219.0
67.90	8694.0
68.90	7865.0
69.90	892.0
71.90	467.0
73.00	3670.0
74.00	13497.0
75.00	39216.0
75.90	3320.0
76.90	432.0
78.00	250.0
78.90	4217.0
79.90	852.0
80.90	4367.0
81.80	930.0
82.90	101.0
86.90	2398.0
87.90	2586.0
90.80	422.0
92.00	2570.0
92.90	3373.0
94.00	8679.0
95.00	67736.0
95.90	4523.0
97.10	109.0
103.80	512.0
104.70	128.0
105.80	428.0
110.80	136.0
112.80	102.0
115.90	247.0
116.80	608.0
117.70	360.0
118.90	444.0
127.80	282.0
128.90	122.0
129.90	338.0
134.80	161.0
136.70	130.0
140.90	1040.0
142.90	1096.0
147.80	291.0
154.70	107.0
171.80	263.0
173.00	589.0
173.90	51440.0
174.90	4365.0
175.90	49520.0
176.90	3577.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

m/z	Abundance
36.00	1083.0
37.00	3924.0
38.00	3967.0
39.00	1408.0
39.90	141.0
43.00	112.0
44.00	922.0
44.90	889.0
46.80	806.0
47.90	544.0
48.90	3433.0
49.90	16102.0
51.00	5161.0
51.90	211.0
54.80	245.0
55.90	1470.0
56.90	2678.0
57.90	199.0
59.80	643.0
60.90	4121.0
61.90	4117.0
62.90	3258.0
64.00	486.0
66.90	239.0
67.90	8883.0
68.90	8014.0
70.00	817.0
71.90	471.0
73.00	3864.0
74.00	13902.0
75.00	39344.0
76.00	3208.0
76.90	497.0
78.00	243.0
78.90	4106.0
79.80	920.0
80.90	4379.0
81.80	1018.0
82.90	111.0
86.90	2526.0
87.90	2793.0
90.80	418.0
92.00	2551.0
92.90	3223.0
94.00	8867.0
95.00	68016.0
95.90	4485.0
97.10	112.0
103.80	524.0
105.00	103.0
105.80	473.0
110.80	126.0
112.80	134.0
115.80	275.0
116.80	540.0
117.80	359.0
118.90	476.0
127.80	290.0
129.90	320.0
134.80	164.0
136.70	147.0
140.90	986.0
142.90	1095.0
147.80	240.0
154.70	143.0
172.00	258.0
172.90	604.0
173.90	53536.0
174.90	4527.0
175.90	52160.0
176.90	3611.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

m/z	Abundance
36.00	984.0
37.00	3724.0
37.90	3800.0
39.00	1370.0
39.90	110.0
43.00	103.0
44.00	874.0
44.90	787.0
46.80	847.0
47.90	466.0
48.90	3220.0
50.00	14860.0
51.00	4604.0
51.90	191.0
55.00	259.0
55.90	1358.0
56.90	2393.0
57.90	171.0
59.80	707.0
61.00	3699.0
61.90	3748.0
62.90	2990.0
63.90	480.0
66.90	217.0
67.90	7954.0
68.90	7538.0
70.00	660.0
71.90	476.0
73.00	3641.0
74.00	13419.0
75.00	36552.0
76.00	2965.0
76.90	522.0
78.00	234.0
78.80	3740.0
79.90	885.0
80.90	4095.0
81.80	968.0
82.80	107.0
86.90	2381.0
87.90	2671.0
90.80	339.0
91.90	2307.0
92.90	2944.0
94.00	8569.0
95.00	62440.0
95.90	4021.0
103.00	104.0
103.80	463.0
105.80	471.0
110.90	122.0
112.70	126.0
115.80	304.0
116.80	466.0
117.90	293.0
118.80	429.0
127.70	275.0
129.80	236.0
130.70	104.0
134.80	158.0
136.70	162.0
140.90	844.0
142.80	1007.0
147.80	128.0
154.80	141.0
157.00	115.0
172.10	239.0
172.90	578.0
173.90	51104.0
174.90	4155.0
175.90	49536.0
176.90	3171.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

Scan 2876 (10.587 min): VU039494.D
BFB02

m/z	Abundance
35.80	202.0
39.90	159.0
43.90	299.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02