




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
 Data File : VU049743.D
 Acq On : 15 Jul 2022 17:46
 Operator : SY/MD
 Sample : N3698-04ME
 Misc : 5.23g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5B69ME

Manual IntegrationsAPPROVED

Quant Time: Jul 15 23:08:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 15 23:03:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

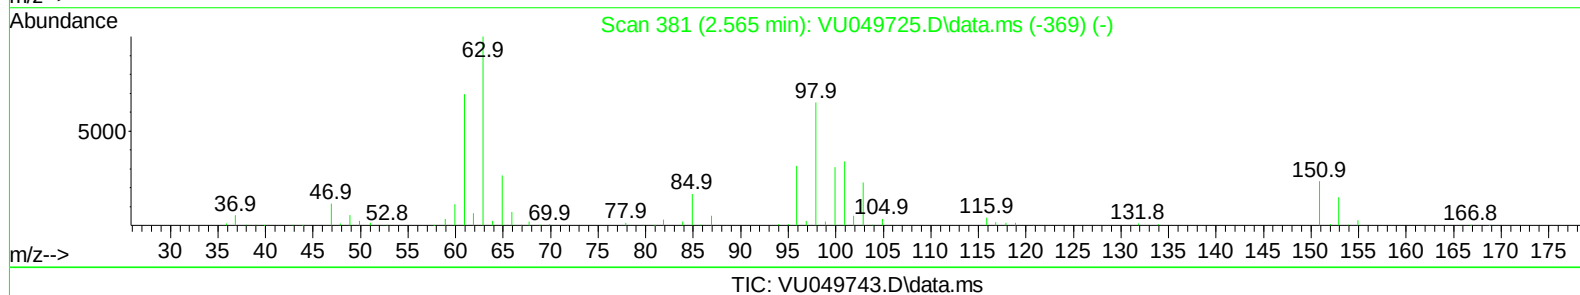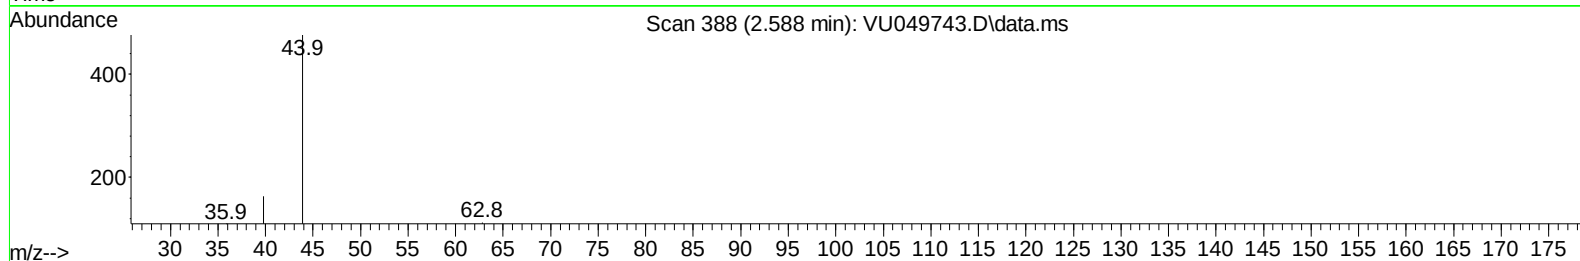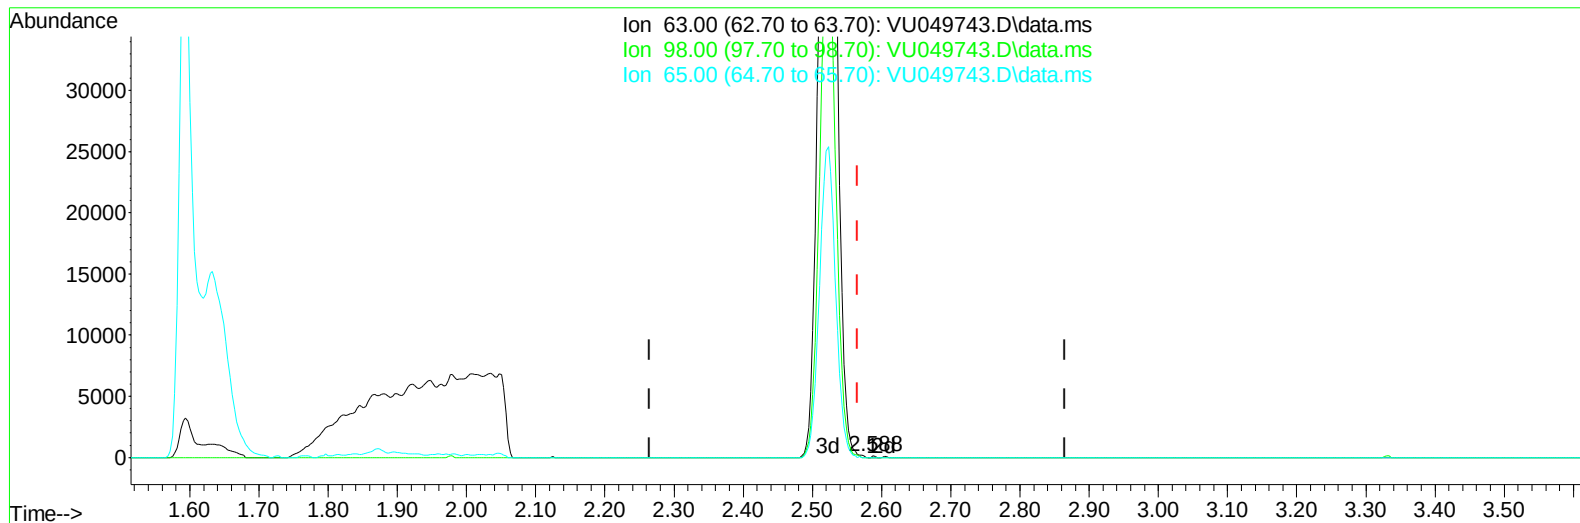

(11) 1,1-Dichloroethene-d2 (S)

2.588min (+ 0.023) 0.02 ug/L

response 42

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	69.30	0.00#
65.00	23.30	47.62#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
 Data File : VU049743.D
 Acq On : 15 Jul 2022 17:46
 Operator : SY/MD
 Sample : N3698-04ME
 Misc : 5.23g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5B69ME

Manual IntegrationsAPPROVED

Quant Time: Jul 15 23:08:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 15 23:03:46 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

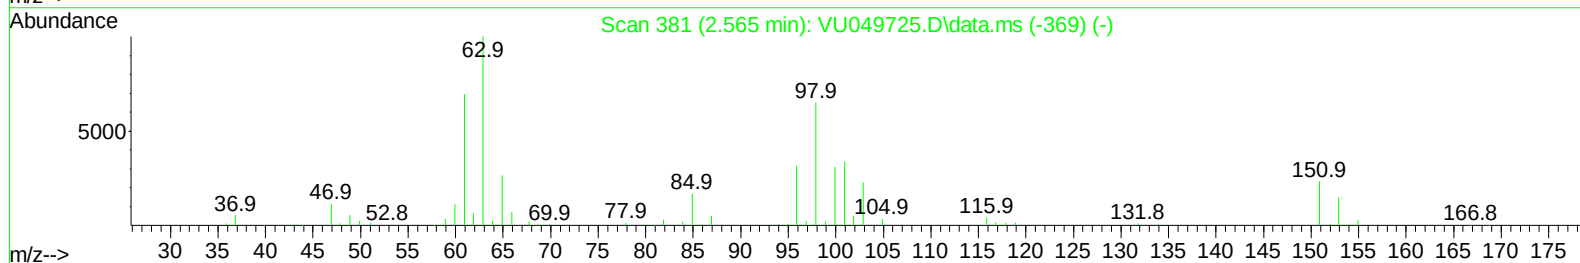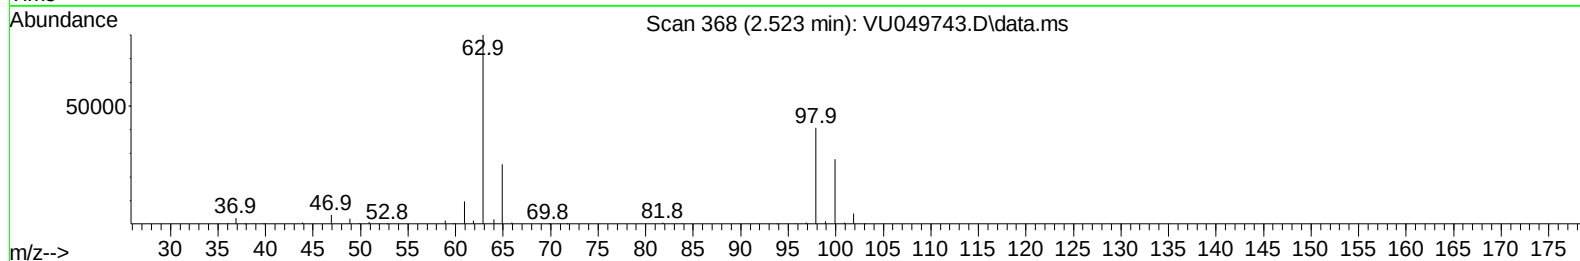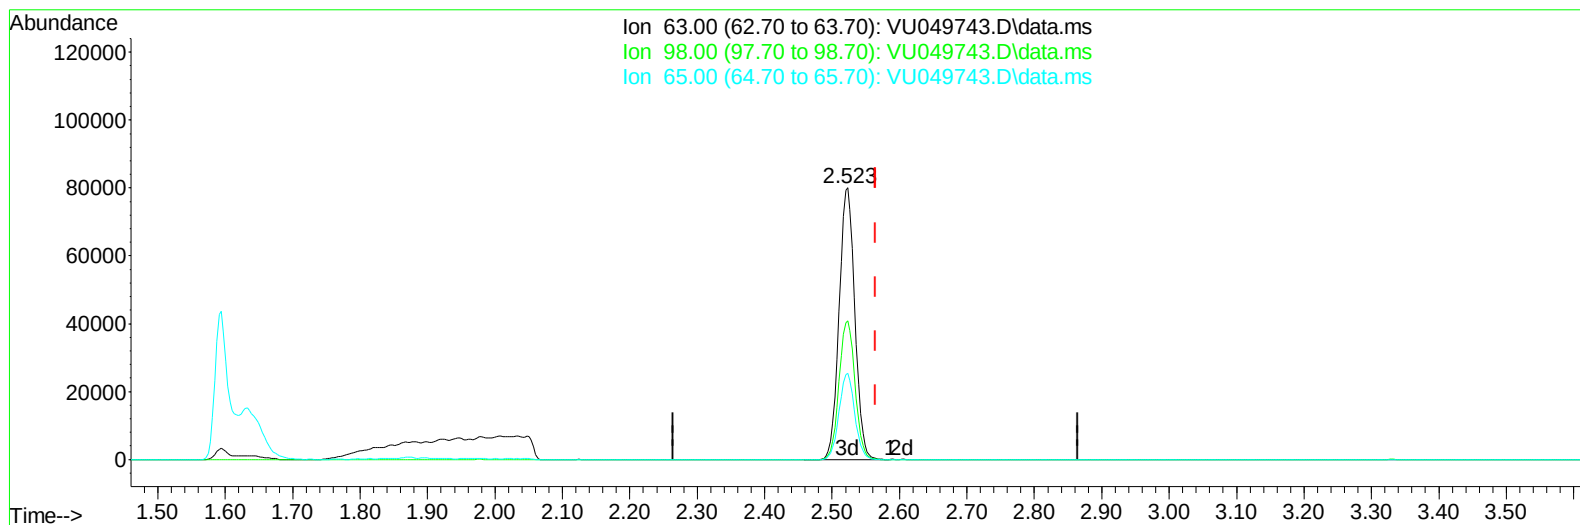

TIC: VU049743.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.523min (-0.042) 47.48 ug/L m

response 129386

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	69.30	0.00#
65.00	23.30	0.02#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
 Data File : VU049743.D
 Acq On : 15 Jul 2022 17:46
 Operator : SY/MD
 Sample : N3698-04ME
 Misc : 5.23g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5B69ME

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 07/18/2022
 Supervised By :Mahesh Dadoda 07/18/2022

Quant Time: Jul 15 23:08:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 15 23:03:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	182847	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	178294	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	83402	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	62464	40.488	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	80.980%		
7) Chloroethane-d5	1.871	69	40638	36.441	ug/L	-0.03
Spiked Amount 50.000	Range 70 - 130		Recovery =	72.880%		
11) 1,1-Dichloroethene-d2	2.523	63	129386m	47.479	ug/L	-0.04
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.960%		
21) 2-Butanone-d5	4.632	46	332184	252.227	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery =	252.230%#		
24) Chloroform-d	5.057	84	254641	93.190	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	186.380%#		
26) 1,2-Dichloroethane-d4	5.697	65	181182	97.971	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	195.940%#		
32) Benzene-d6	5.719	84	435476	80.398	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	160.800%#		
36) 1,2-Dichloropropane-d6	6.687	67	170494	93.581	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	187.160%#		
41) Toluene-d8	7.896	98	362365	76.822	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	153.640%#		
43) trans-1,3-Dichloroprop...	8.182	79	67276	87.644	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	175.280%#		
47) 2-Hexanone-d5	8.648	63	217087	264.891	ug/L	0.02
Spiked Amount 100.000	Range 45 - 130		Recovery =	264.890%#		
56) 1,1,2,2-Tetrachloroeth...	10.761	84	305528	119.852	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	239.700%#		
66) 1,2-Dichlorobenzene-d4	12.195	152	168304	107.030	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	214.060%#		
Target Compounds						
					Qvalue	
5) vinyl chloride	1.597	62	2730	1.256	ug/L #	65
16) Methylene chloride	3.028	84	2479	1.506	ug/L	94
20) cis-1,2-Dichloroethene	4.655	96	5816	3.619	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
Data File : VU049743.D
Acq On : 15 Jul 2022 17:46
Operator : SY/MD
Sample : N3698-04ME
Misc : 5.23g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5B69ME

Manual IntegrationsAPPROVED

Quant Time: Jul 15 23:08:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 15 23:03:46 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 07/18/2022
Supervised By :Mahesh Dadoda 07/18/2022

