

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
 Data File : VU049727.D
 Acq On : 15 Jul 2022 10:35
 Operator : SY/MD
 Sample : VU0715WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK157

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049727.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.514	51	54	63	rBV2	918	1114	0.14%	0.018%
2	1.597	71	80	97	rBV	86120	99516	12.68%	1.633%
3	1.806	131	145	153	rVB8	6675	14282	1.82%	0.234%
4	1.900	166	174	191	rBV	67735	90494	11.53%	1.485%
5	2.285	291	294	297	rVB	540	322	0.04%	0.005%
6	2.327	305	307	317	rVB4	505	559	0.07%	0.009%
7	2.369	318	320	322	rBV2	449	253	0.03%	0.004%
8	2.562	368	380	395	rBV	136056	219423	27.96%	3.601%
9	2.777	444	447	448	rVV	413	256	0.03%	0.004%
10	2.787	448	450	456	rVV2	584	485	0.06%	0.008%
11	2.996	511	515	521	rBV2	265	265	0.03%	0.004%
12	3.038	523	528	537	rVB4	802	1207	0.15%	0.020%
13	3.179	559	572	585	rBV2	2007	4001	0.51%	0.066%
14	3.488	660	668	671	rBV2	267	389	0.05%	0.006%
15	3.568	689	693	698	rVB2	172	180	0.02%	0.003%
16	3.597	699	702	708	rVB2	177	175	0.02%	0.003%
17	3.723	734	741	744	rBV	335	401	0.05%	0.007%
18	3.867	781	786	792	rBV2	182	218	0.03%	0.004%
19	4.086	849	854	856	rBV	192	170	0.02%	0.003%
20	4.150	871	874	878	rVB2	206	172	0.02%	0.003%
21	4.176	878	882	889	rBV2	220	283	0.04%	0.005%
22	4.330	928	930	936	rVB2	207	181	0.02%	0.003%
23	4.469	970	973	981	rBV2	145	172	0.02%	0.003%
24	4.536	988	994	999	rBV2	294	391	0.05%	0.006%
25	4.620	1007	1020	1061	rBV	103905	254901	32.48%	4.183%
26	4.832	1082	1086	1087	rBV3	269	172	0.02%	0.003%
27	4.871	1096	1098	1103	rVB3	270	262	0.03%	0.004%
28	4.896	1103	1106	1110	rVB2	258	203	0.03%	0.003%
29	4.919	1110	1113	1115	rBV	222	167	0.02%	0.003%
30	4.938	1116	1119	1126	rVB2	304	299	0.04%	0.005%
31	4.977	1127	1131	1135	rVB2	276	218	0.03%	0.004%
32	5.060	1141	1157	1182	rBV	144255	318791	40.61%	5.231%
33	5.189	1195	1197	1203	rVB2	218	165	0.02%	0.003%
34	5.282	1218	1226	1228	rBV4	556	568	0.07%	0.009%
35	5.298	1228	1231	1235	rVB2	678	502	0.06%	0.008%
36	5.546	1306	1308	1315	rVB	207	179	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
 Data File : VU049727.D
 Acq On : 15 Jul 2022 10:35
 Operator : SY/MD
 Sample : VU0715WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK157

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	5.723	1342	1363	1385	rBV2	287774	784910	100.00%	12.880%
38	5.854	1401	1404	1408	rVB	321	229	0.03%	0.004%
39	5.893	1413	1416	1419	rVV2	276	200	0.03%	0.003%
40	5.977	1439	1442	1446	rVB	336	205	0.03%	0.003%
41	6.041	1460	1462	1466	rBV2	240	206	0.03%	0.003%
42	6.247	1508	1526	1546	rBV	241269	457495	58.29%	7.507%
43	6.408	1572	1576	1580	rVB3	232	166	0.02%	0.003%
44	6.485	1596	1600	1606	rBV2	195	285	0.04%	0.005%
45	6.530	1606	1614	1622	rBV4	2242	3873	0.49%	0.064%
46	6.690	1650	1664	1683	rBV	193036	374675	47.73%	6.148%
47	6.877	1719	1722	1728	rVB2	193	193	0.02%	0.003%
48	7.186	1808	1818	1826	rVV4	969	1747	0.22%	0.029%
49	7.465	1901	1905	1909	rBV	238	204	0.03%	0.003%
50	7.565	1922	1936	1954	rBV	98260	171132	21.80%	2.808%
51	7.687	1967	1974	1976	rBV	659	748	0.10%	0.012%
52	7.793	1996	2007	2016	rBV4	635	1192	0.15%	0.020%
53	7.896	2021	2039	2056	rBV	329162	568057	72.37%	9.321%
54	8.179	2106	2127	2145	rBV2	67087	113112	14.41%	1.856%
55	8.546	2237	2241	2245	rVB2	419	361	0.05%	0.006%
56	8.578	2245	2251	2253	rBV	331	404	0.05%	0.007%
57	8.633	2256	2268	2305	rVV2	261524	529343	67.44%	8.686%
58	8.890	2343	2348	2353	rBV2	285	245	0.03%	0.004%
59	8.915	2353	2356	2363	rVV2	187	181	0.02%	0.003%
60	8.977	2370	2375	2378	rBV	262	232	0.03%	0.004%
61	9.295	2468	2474	2480	rBV2	341	516	0.07%	0.008%
62	9.417	2498	2512	2531	rBV	333786	561648	71.56%	9.216%
63	9.552	2551	2554	2564	rBV4	235	381	0.05%	0.006%
64	9.671	2586	2591	2594	rBV2	259	278	0.04%	0.005%
65	9.700	2594	2600	2606	rVB4	541	512	0.07%	0.008%
66	9.922	2665	2669	2672	rBV2	182	174	0.02%	0.003%
67	10.099	2720	2724	2727	rBV	375	314	0.04%	0.005%
68	10.128	2730	2733	2735	rBV3	276	167	0.02%	0.003%
69	10.234	2764	2766	2770	rVB2	263	181	0.02%	0.003%
70	10.272	2770	2778	2781	rBV	706	897	0.11%	0.015%
71	10.539	2858	2861	2863	rBV	261	165	0.02%	0.003%
72	10.636	2885	2891	2898	rVV5	661	880	0.11%	0.014%
73	10.665	2898	2900	2907	rVB	307	235	0.03%	0.004%
74	10.700	2907	2911	2915	rBV	212	221	0.03%	0.004%
75	10.755	2915	2928	2946	rBV	271830	445417	56.75%	7.309%
76	10.944	2984	2987	2991	rVB2	310	244	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
 Data File : VU049727.D
 Acq On : 15 Jul 2022 10:35
 Operator : SY/MD
 Sample : VU0715WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK157

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	10.986	2997	3000	3007	rBV	231	231	0.03%	0.004%
78	11.060	3020	3023	3028	rVV2	243	242	0.03%	0.004%
79	11.089	3029	3032	3038	rVV2	333	332	0.04%	0.005%
80	11.131	3042	3045	3048	rVB2	261	164	0.02%	0.003%
81	11.247	3074	3081	3084	rBV	370	492	0.06%	0.008%
82	11.417	3131	3134	3140	rBV2	162	193	0.02%	0.003%
83	11.755	3233	3239	3242	rVB2	437	469	0.06%	0.008%
84	11.812	3244	3257	3279	rVV	322750	514823	65.59%	8.448%
85	12.057	3330	3333	3336	rBV2	273	209	0.03%	0.003%
86	12.192	3363	3375	3394	rBV	328221	535003	68.16%	8.779%
87	12.304	3407	3410	3414	rBV3	302	262	0.03%	0.004%
88	12.369	3427	3430	3433	rBV2	240	176	0.02%	0.003%
89	12.915	3596	3600	3606	rBV2	398	294	0.04%	0.005%
90	12.957	3611	3613	3618	rVB2	309	191	0.02%	0.003%
91	13.227	3692	3697	3701	rBV2	418	460	0.06%	0.008%
92	13.404	3748	3752	3756	rVB3	255	208	0.03%	0.003%
93	13.427	3756	3759	3761	rBV3	425	285	0.04%	0.005%
94	13.767	3861	3865	3869	rBV3	378	297	0.04%	0.005%
95	13.845	3882	3889	3891	rBV3	872	965	0.12%	0.016%
96	13.960	3922	3925	3929	rBV2	282	248	0.03%	0.004%
97	14.092	3957	3966	3974	rBV	2992	4431	0.56%	0.073%
98	14.224	4002	4007	4008	rBV	322	295	0.04%	0.005%
99	14.687	4148	4151	4155	rBV2	360	259	0.03%	0.004%
100	14.732	4158	4165	4168	rBV3	461	645	0.08%	0.011%




Sum of corrected areas: 6094135

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
Data File : VU049727.D
Acq On : 15 Jul 2022 10:35
Operator : SY/MD
Sample : VU0715WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK157

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

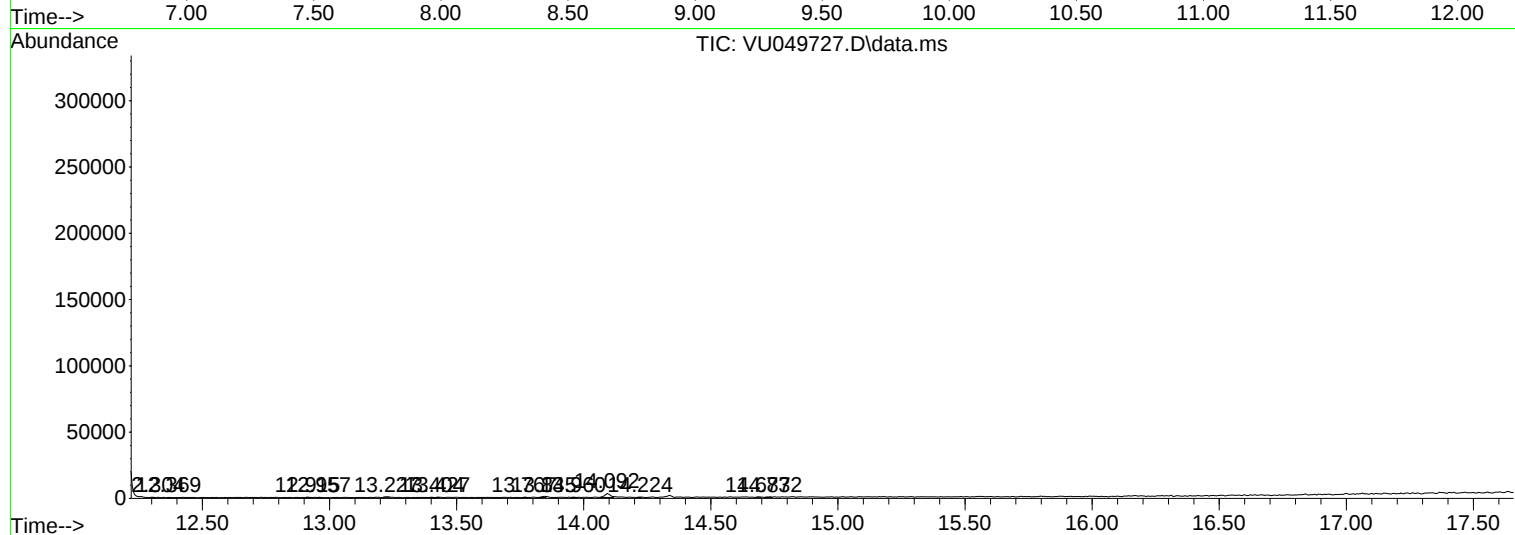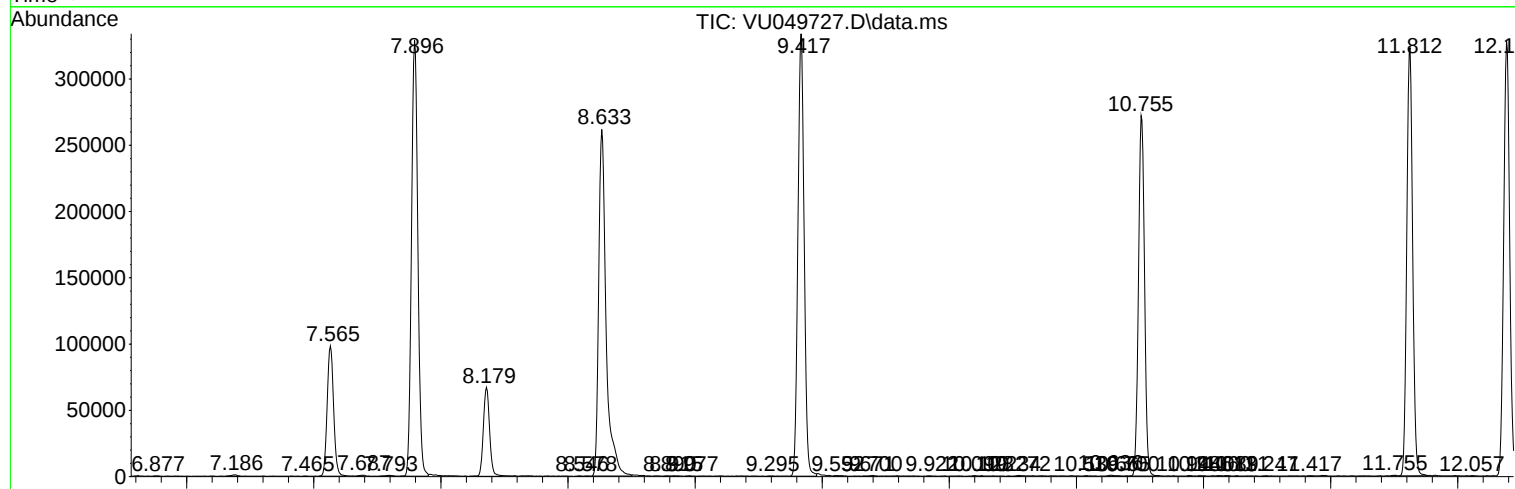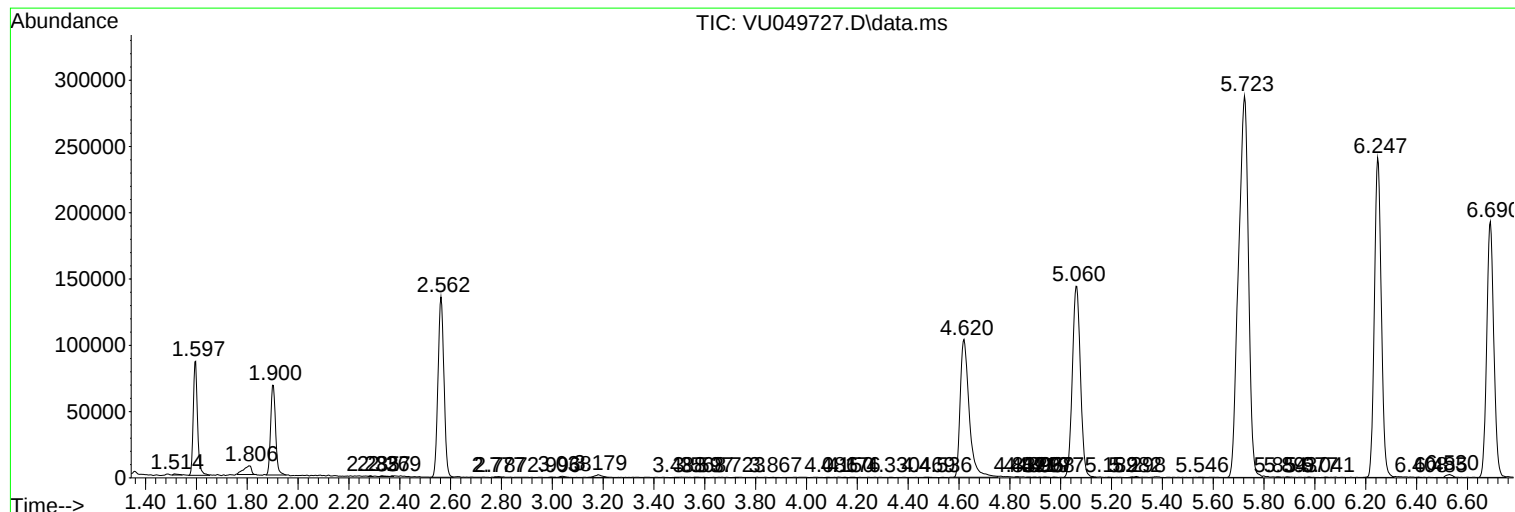

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
Data File : VU049727.D
Acq On : 15 Jul 2022 10:35
Operator : SY/MD
Sample : VU0715WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK157

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
Data File : VU049727.D
Acq On : 15 Jul 2022 10:35
Operator : SY/MD
Sample : VU0715WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK157

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------