

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
 Data File : VU049729.D
 Acq On : 15 Jul 2022 12:08
 Operator : SY/MD
 Sample : N3721-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049729.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	10	rVB3	1840	1373	0.16%	0.021%
2	1.597	72	80	101	rVB	93737	108263	12.37%	1.641%
3	1.903	166	175	188	rBV	74093	100127	11.44%	1.517%
4	2.565	369	381	396	rBV	151326	243448	27.81%	3.689%
5	2.748	435	438	441	rVB2	269	154	0.02%	0.002%
6	2.787	446	450	455	rBV2	438	433	0.05%	0.007%
7	3.041	519	529	540	rBV3	3533	6608	0.75%	0.100%
8	3.182	567	573	575	rBV2	554	552	0.06%	0.008%
9	3.404	639	642	646	rBV	178	151	0.02%	0.002%
10	3.562	689	691	697	rVB2	253	216	0.02%	0.003%
11	3.674	720	726	728	rBV2	203	218	0.02%	0.003%
12	3.694	728	732	739	rVB2	274	362	0.04%	0.005%
13	3.793	758	763	766	rBV2	175	193	0.02%	0.003%
14	3.935	804	807	813	rBV2	264	339	0.04%	0.005%
15	4.015	827	832	836	rVB2	285	296	0.03%	0.004%
16	4.041	836	840	842	rBV	262	247	0.03%	0.004%
17	4.163	875	878	884	rVB2	242	287	0.03%	0.004%
18	4.192	884	887	891	rBV	224	203	0.02%	0.003%
19	4.623	1009	1021	1049	rBV	100370	254532	29.07%	3.857%
20	4.809	1076	1079	1081	rBV3	277	184	0.02%	0.003%
21	4.832	1083	1086	1091	rVB2	624	461	0.05%	0.007%
22	4.948	1120	1122	1129	rVB3	286	208	0.02%	0.003%
23	4.980	1129	1132	1136	rBV2	195	182	0.02%	0.003%
24	4.996	1136	1137	1141	rVB2	276	169	0.02%	0.003%
25	5.063	1141	1158	1180	rBV	165385	359921	41.11%	5.455%
26	5.285	1222	1227	1232	rBV3	765	1057	0.12%	0.016%
27	5.330	1237	1241	1244	rBV2	326	271	0.03%	0.004%
28	5.382	1251	1257	1262	rBV2	487	713	0.08%	0.011%
29	5.610	1325	1328	1334	rBV2	178	159	0.02%	0.002%
30	5.726	1342	1364	1387	rBV2	318535	875515	100.00%	13.268%
31	5.925	1423	1426	1428	rBV2	233	149	0.02%	0.002%
32	6.044	1456	1463	1465	rBV2	417	269	0.03%	0.004%
33	6.115	1481	1485	1488	rVB3	182	156	0.02%	0.002%
34	6.250	1510	1527	1544	rBV	265896	502144	57.35%	7.610%
35	6.414	1574	1578	1582	rVB2	270	216	0.02%	0.003%
36	6.536	1606	1616	1627	rBV5	2272	4224	0.48%	0.064%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
 Data File : VU049729.D
 Acq On : 15 Jul 2022 12:08
 Operator : SY/MD
 Sample : N3721-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.578	1627	1629	1634	rVB	248	176	0.02%	0.003%
38	6.616	1635	1641	1648	rBV2	256	353	0.04%	0.005%
39	6.690	1648	1664	1685	rBV	215394	422467	48.25%	6.403%
40	6.812	1699	1702	1707	rVB3	558	473	0.05%	0.007%
41	6.922	1733	1736	1738	rBV	240	153	0.02%	0.002%
42	7.182	1811	1817	1829	rBV5	1136	1702	0.19%	0.026%
43	7.333	1862	1864	1870	rVB2	203	184	0.02%	0.003%
44	7.398	1881	1884	1887	rBV	212	167	0.02%	0.003%
45	7.565	1922	1936	1954	rBV	110197	192924	22.04%	2.924%
46	7.629	1954	1956	1960	rVB2	395	223	0.03%	0.003%
47	7.648	1960	1962	1967	rVB2	270	192	0.02%	0.003%
48	7.693	1970	1976	1978	rBV2	780	834	0.10%	0.013%
49	7.841	2018	2022	2025	rBV2	224	193	0.02%	0.003%
50	7.899	2025	2040	2064	rBV	368616	638390	72.92%	9.675%
51	8.179	2116	2127	2145	rBV	73669	124407	14.21%	1.885%
52	8.404	2193	2197	2203	rBV	385	411	0.05%	0.006%
53	8.430	2203	2205	2207	rVV	231	154	0.02%	0.002%
54	8.452	2210	2212	2217	rVV2	236	200	0.02%	0.003%
55	8.478	2217	2220	2224	rVB2	381	293	0.03%	0.004%
56	8.504	2224	2228	2232	rBV	326	348	0.04%	0.005%
57	8.636	2256	2269	2305	rBV3	272121	551744	63.02%	8.362%
58	8.790	2316	2317	2323	rVB2	429	353	0.04%	0.005%
59	8.867	2338	2341	2344	rVB	285	183	0.02%	0.003%
60	8.902	2347	2352	2355	rBV	226	232	0.03%	0.004%
61	9.308	2476	2478	2484	rBV	217	197	0.02%	0.003%
62	9.417	2499	2512	2533	rBV	368959	608716	69.53%	9.225%
63	9.626	2574	2577	2581	rVV2	239	197	0.02%	0.003%
64	9.652	2582	2585	2587	rVV	266	162	0.02%	0.002%
65	9.771	2619	2622	2626	rBV	261	223	0.03%	0.003%
66	10.002	2691	2694	2698	rVB	271	227	0.03%	0.003%
67	10.192	2748	2753	2756	rBV2	193	177	0.02%	0.003%
68	10.250	2767	2771	2774	rBV2	204	207	0.02%	0.003%
69	10.488	2843	2845	2850	rVB2	454	289	0.03%	0.004%
70	10.523	2850	2856	2860	rBV2	323	457	0.05%	0.007%
71	10.652	2891	2896	2899	rVB	412	370	0.04%	0.006%
72	10.668	2899	2901	2904	rBV2	227	191	0.02%	0.003%
73	10.758	2916	2929	2951	rBV	294827	475392	54.30%	7.205%
74	11.070	3020	3026	3029	rBV2	197	250	0.03%	0.004%
75	11.188	3060	3063	3067	rVB	252	150	0.02%	0.002%
76	11.246	3078	3081	3086	rVB2	265	234	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
 Data File : VU049729.D
 Acq On : 15 Jul 2022 12:08
 Operator : SY/MD
 Sample : N3721-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	11.275	3086	3090	3093	rBV	356	296	0.03%	0.004%
78	11.327	3101	3106	3109	rBV2	578	617	0.07%	0.009%
79	11.751	3234	3238	3244	rBV2	306	299	0.03%	0.005%
80	11.812	3244	3257	3279	rBV	337503	535867	61.21%	8.121%
81	11.925	3290	3292	3295	rBV	263	152	0.02%	0.002%
82	12.076	3335	3339	3344	rBV2	374	371	0.04%	0.006%
83	12.192	3363	3375	3390	rBV	343576	568156	64.89%	8.610%
84	12.275	3399	3401	3409	rVB4	656	415	0.05%	0.006%
85	12.529	3477	3480	3484	rBV2	239	232	0.03%	0.004%
86	12.696	3530	3532	3536	rBV	261	153	0.02%	0.002%
87	12.815	3567	3569	3572	rBV	291	169	0.02%	0.003%
88	12.963	3613	3615	3621	rVB	269	194	0.02%	0.003%
89	12.992	3621	3624	3626	rBV2	248	170	0.02%	0.003%
90	13.658	3828	3831	3833	rBV	284	156	0.02%	0.002%
91	13.690	3839	3841	3844	rVB	356	167	0.02%	0.003%
92	13.706	3844	3846	3849	rBV2	233	165	0.02%	0.003%
93	13.774	3865	3867	3870	rBV	266	151	0.02%	0.002%
94	13.970	3926	3928	3930	rBV2	321	163	0.02%	0.002%
95	14.098	3960	3968	3972	rBV3	619	1005	0.11%	0.015%
96	14.404	4060	4063	4066	rBV2	441	313	0.04%	0.005%
97	14.545	4104	4107	4109	rBV3	316	218	0.02%	0.003%
98	14.655	4138	4141	4146	rBV2	272	295	0.03%	0.004%
99	15.442	4384	4386	4393	rBV2	420	324	0.04%	0.005%
100	16.095	4587	4589	4591	rBV2	650	218	0.02%	0.003%




Sum of corrected areas: 6598461

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
Data File : VU049729.D
Acq On : 15 Jul 2022 12:08
Operator : SY/MD
Sample : N3721-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

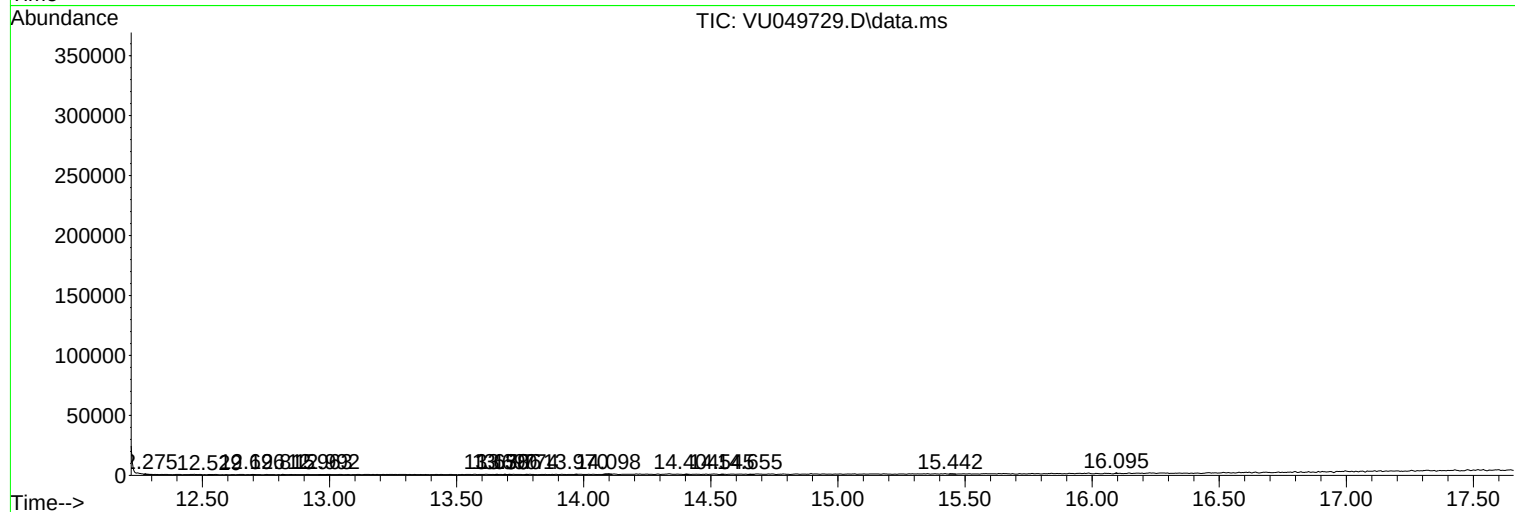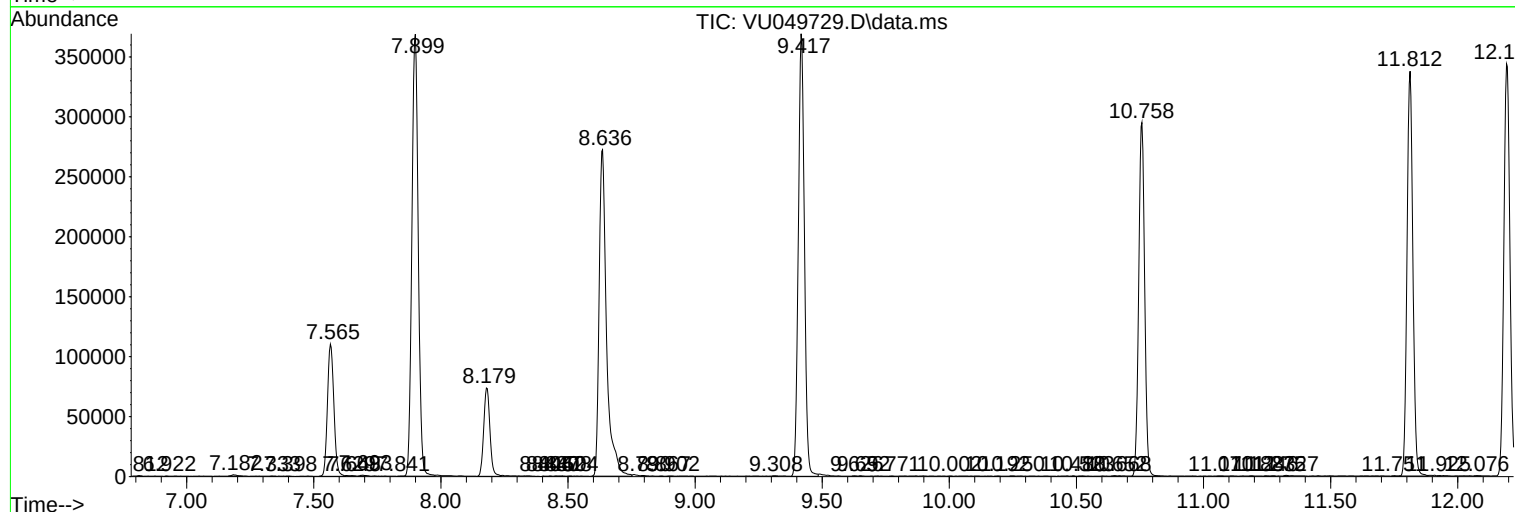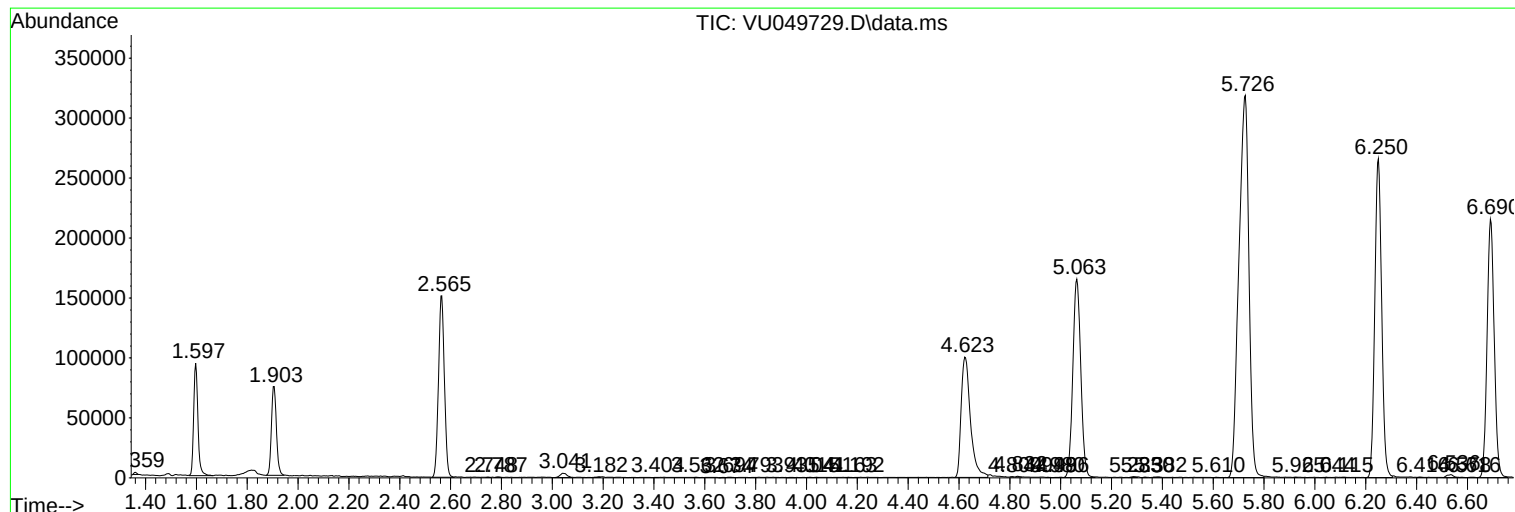

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
Data File : VU049729.D
Acq On : 15 Jul 2022 12:08
Operator : SY/MD
Sample : N3721-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
Data File : VU049729.D
Acq On : 15 Jul 2022 12:08
Operator : SY/MD
Sample : N3721-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------