

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
 Data File : VU049738.D
 Acq On : 15 Jul 2022 15:48
 Operator : SY/MD
 Sample : N3748-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH0E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

Signal : TIC: VU049738.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.523	51	57	62	rBV2	2649	3450	0.45%	0.059%
2	1.597	73	80	97	rVB	75749	85908	11.29%	1.457%
3	1.797	129	142	149	rVB7	7665	15604	2.05%	0.265%
4	1.903	166	175	188	rBV	64684	84921	11.17%	1.440%
5	2.353	313	315	319	rBV4	426	247	0.03%	0.004%
6	2.462	346	349	354	rBV2	226	167	0.02%	0.003%
7	2.562	368	380	395	rBV	121140	193341	25.42%	3.279%
8	2.626	396	400	410	rVB3	1296	1916	0.25%	0.032%
9	2.671	410	414	415	rBV	302	239	0.03%	0.004%
10	2.697	418	422	427	rBV2	148	186	0.02%	0.003%
11	2.793	449	452	455	rBV2	337	246	0.03%	0.004%
12	2.858	466	472	475	rBV2	247	271	0.04%	0.005%
13	2.919	487	491	494	rBV3	203	198	0.03%	0.003%
14	3.041	523	529	536	rBV3	748	1015	0.13%	0.017%
15	3.076	536	540	543	rVV2	197	184	0.02%	0.003%
16	3.099	543	547	551	rVV	134	168	0.02%	0.003%
17	3.121	551	554	559	rVV2	224	272	0.04%	0.005%
18	3.182	560	573	588	rVB	6214	13067	1.72%	0.222%
19	3.292	605	607	613	rVB	228	178	0.02%	0.003%
20	3.530	675	681	690	rVV2	294	414	0.05%	0.007%
21	3.854	777	782	786	rBV2	194	177	0.02%	0.003%
22	4.034	835	838	843	rBV2	204	248	0.03%	0.004%
23	4.125	861	866	872	rBV2	245	265	0.03%	0.004%
24	4.215	892	894	901	rVB2	139	158	0.02%	0.003%
25	4.324	925	928	931	rBV2	212	165	0.02%	0.003%
26	4.359	936	939	947	rBV2	212	339	0.04%	0.006%
27	4.620	1007	1020	1045	rBV	108391	261528	34.38%	4.435%
28	4.986	1128	1134	1140	rVB3	222	269	0.04%	0.005%
29	5.063	1140	1158	1177	rBV	142996	310319	40.80%	5.262%
30	5.295	1220	1230	1240	rVB	648	1298	0.17%	0.022%
31	5.362	1248	1251	1252	rBV	431	213	0.03%	0.004%
32	5.568	1310	1315	1319	rVB2	270	269	0.04%	0.005%
33	5.620	1327	1331	1336	rVB2	206	227	0.03%	0.004%
34	5.723	1336	1363	1383	rBV2	277200	760595	100.00%	12.898%
35	5.996	1446	1448	1454	rVB2	212	169	0.02%	0.003%
36	6.176	1500	1504	1509	rBV2	179	169	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
 Data File : VU049738.D
 Acq On : 15 Jul 2022 15:48
 Operator : SY/MD
 Sample : N3748-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH0E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

37	6.247	1512	1526	1550	rBV	246548	468133	61.55%	7.938%
38	6.414	1575	1578	1581	rVB2	286	211	0.03%	0.004%
39	6.433	1581	1584	1586	rBV2	287	201	0.03%	0.003%
40	6.526	1607	1613	1614	rBV3	1854	1868	0.25%	0.032%
41	6.690	1649	1664	1686	rBV	190442	369576	48.59%	6.267%
42	6.944	1736	1743	1745	rVV2	218	220	0.03%	0.004%
43	6.960	1745	1748	1751	rVB2	231	166	0.02%	0.003%
44	7.005	1760	1762	1767	rVB	366	218	0.03%	0.004%
45	7.041	1767	1773	1779	rVB2	372	541	0.07%	0.009%
46	7.067	1779	1781	1784	rBV2	208	171	0.02%	0.003%
47	7.160	1806	1810	1812	rBV2	272	218	0.03%	0.004%
48	7.182	1812	1817	1824	rVB3	1118	1252	0.16%	0.021%
49	7.317	1854	1859	1862	rBV2	294	328	0.04%	0.006%
50	7.462	1901	1904	1908	rVB	272	197	0.03%	0.003%
51	7.497	1909	1915	1917	rBV	156	165	0.02%	0.003%
52	7.565	1924	1936	1952	rBV	91051	160181	21.06%	2.716%
53	7.694	1968	1976	1982	rBV5	971	1412	0.19%	0.024%
54	7.896	2025	2039	2060	rBV	308560	526059	69.16%	8.921%
55	8.076	2092	2095	2102	rVB3	380	475	0.06%	0.008%
56	8.179	2115	2127	2146	rBV	63706	105746	13.90%	1.793%
57	8.266	2152	2154	2156	rVB2	385	181	0.02%	0.003%
58	8.308	2165	2167	2173	rVB2	278	155	0.02%	0.003%
59	8.346	2176	2179	2181	rBV2	198	166	0.02%	0.003%
60	8.378	2188	2189	2194	rVB	292	180	0.02%	0.003%
61	8.411	2194	2199	2202	rBV	321	353	0.05%	0.006%
62	8.462	2212	2215	2218	rBV	268	200	0.03%	0.003%
63	8.552	2237	2243	2253	rVB3	2181	3152	0.41%	0.053%
64	8.632	2253	2268	2299	rBV2	279002	543612	71.47%	9.218%
65	8.819	2323	2326	2329	rBV3	373	326	0.04%	0.006%
66	8.883	2342	2346	2349	rBB2	300	198	0.03%	0.003%
67	8.989	2376	2379	2384	rBV	240	192	0.03%	0.003%
68	9.140	2420	2426	2429	rBV	170	162	0.02%	0.003%
69	9.292	2469	2473	2478	rVB2	235	221	0.03%	0.004%
70	9.417	2499	2512	2538	rVV	340564	563005	74.02%	9.547%
71	9.600	2563	2569	2573	rBV2	670	837	0.11%	0.014%
72	9.645	2580	2583	2586	rBV	289	168	0.02%	0.003%
73	9.845	2641	2645	2649	rBV2	208	187	0.02%	0.003%
74	9.915	2664	2667	2674	rBV2	238	309	0.04%	0.005%
75	10.324	2791	2794	2799	rBV	213	170	0.02%	0.003%
76	10.410	2814	2821	2822	rBV2	329	382	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
 Data File : VU049738.D
 Acq On : 15 Jul 2022 15:48
 Operator : SY/MD
 Sample : N3748-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH0E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
 Title : VOC Analysis

77	10.488	2842	2845	2848	rVB	291	184	0.02%	0.003%
78	10.754	2916	2928	2945	rBV	275841	441364	58.03%	7.485%
79	11.115	3036	3040	3042	rBV2	227	185	0.02%	0.003%
80	11.343	3106	3111	3116	rVB2	204	256	0.03%	0.004%
81	11.369	3116	3119	3121	rBV	283	169	0.02%	0.003%
82	11.523	3161	3167	3169	rBV2	213	270	0.04%	0.005%
83	11.623	3193	3198	3200	rBV2	213	212	0.03%	0.004%
84	11.709	3217	3225	3227	rBV2	254	363	0.05%	0.006%
85	11.812	3243	3257	3273	rBV	301002	484232	63.66%	8.211%
86	12.102	3344	3347	3351	rBV2	353	323	0.04%	0.005%
87	12.192	3362	3375	3397	rBV	294848	475713	62.54%	8.067%
88	12.304	3405	3410	3414	rVB4	487	481	0.06%	0.008%
89	12.327	3414	3417	3420	rVB2	327	167	0.02%	0.003%
90	12.346	3420	3423	3427	rBV	284	191	0.03%	0.003%
91	13.217	3687	3694	3698	rBV2	326	434	0.06%	0.007%
92	13.362	3736	3739	3742	rVB	388	212	0.03%	0.004%
93	13.536	3788	3793	3796	rBV	305	314	0.04%	0.005%
94	13.680	3835	3838	3839	rBV2	300	164	0.02%	0.003%
95	14.008	3937	3940	3942	rBV	351	226	0.03%	0.004%
96	14.349	4042	4046	4050	rVB	414	374	0.05%	0.006%
97	14.372	4050	4053	4057	rBV2	295	273	0.04%	0.005%
98	14.484	4085	4088	4090	rBV2	380	235	0.03%	0.004%
99	14.504	4090	4094	4099	rVB2	328	344	0.05%	0.006%
100	14.729	4159	4164	4166	rBV3	412	460	0.06%	0.008%




Sum of corrected areas: 5897040

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
Data File : VU049738.D
Acq On : 15 Jul 2022 15:48
Operator : SY/MD
Sample : N3748-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH0E3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

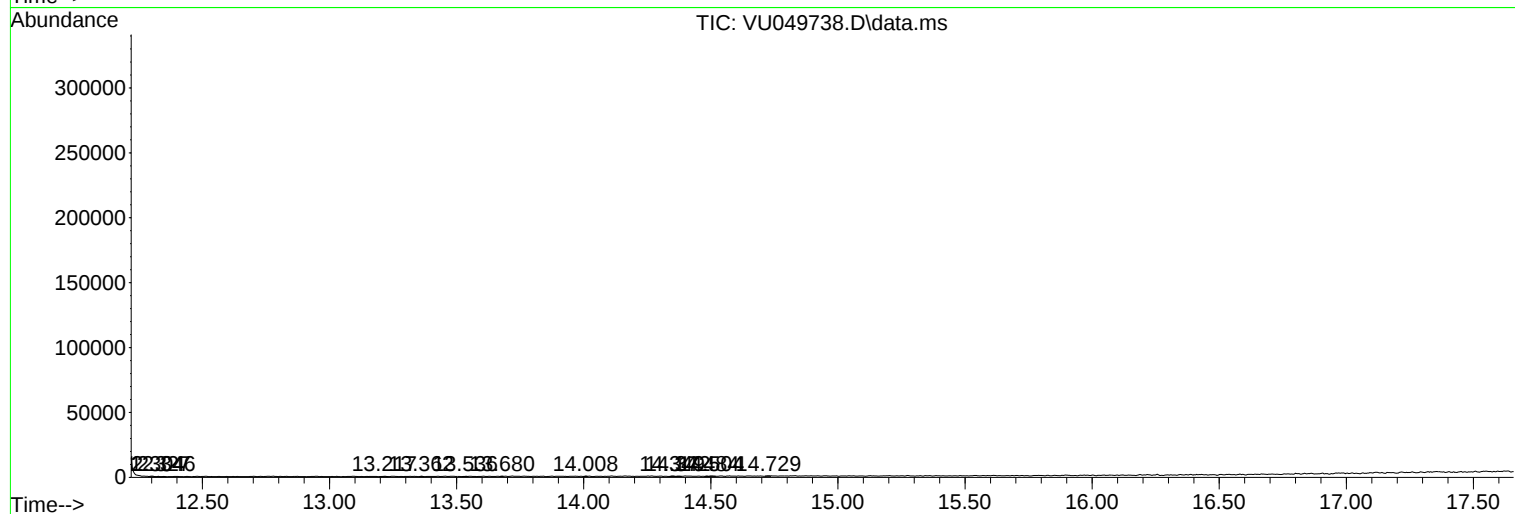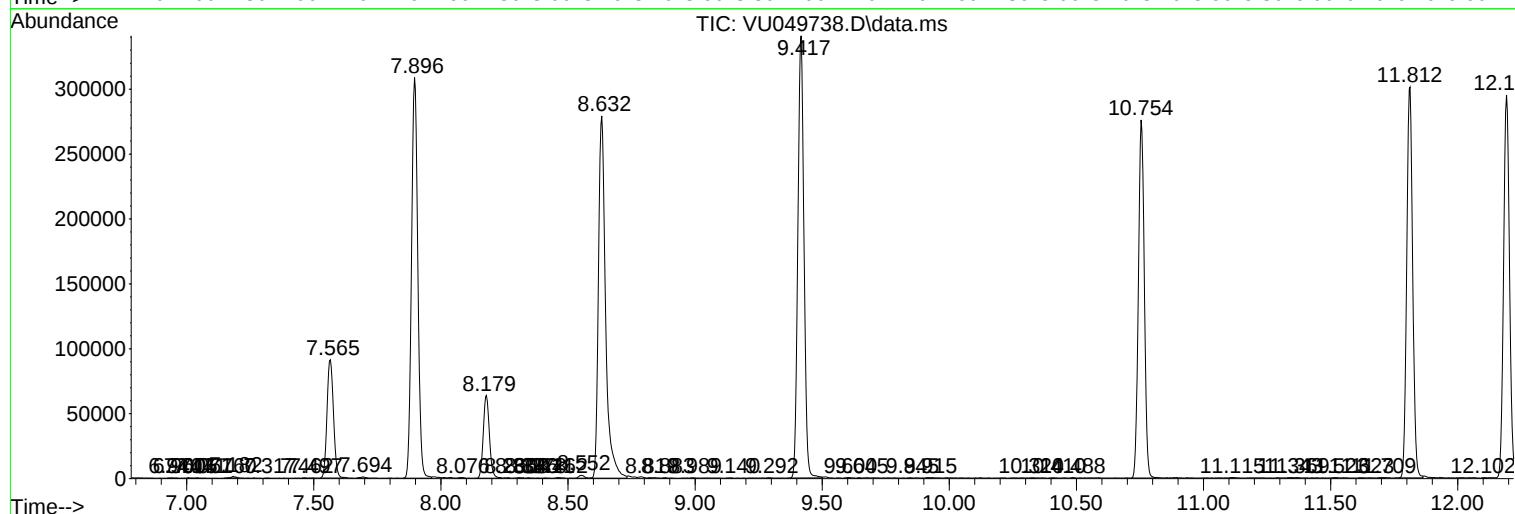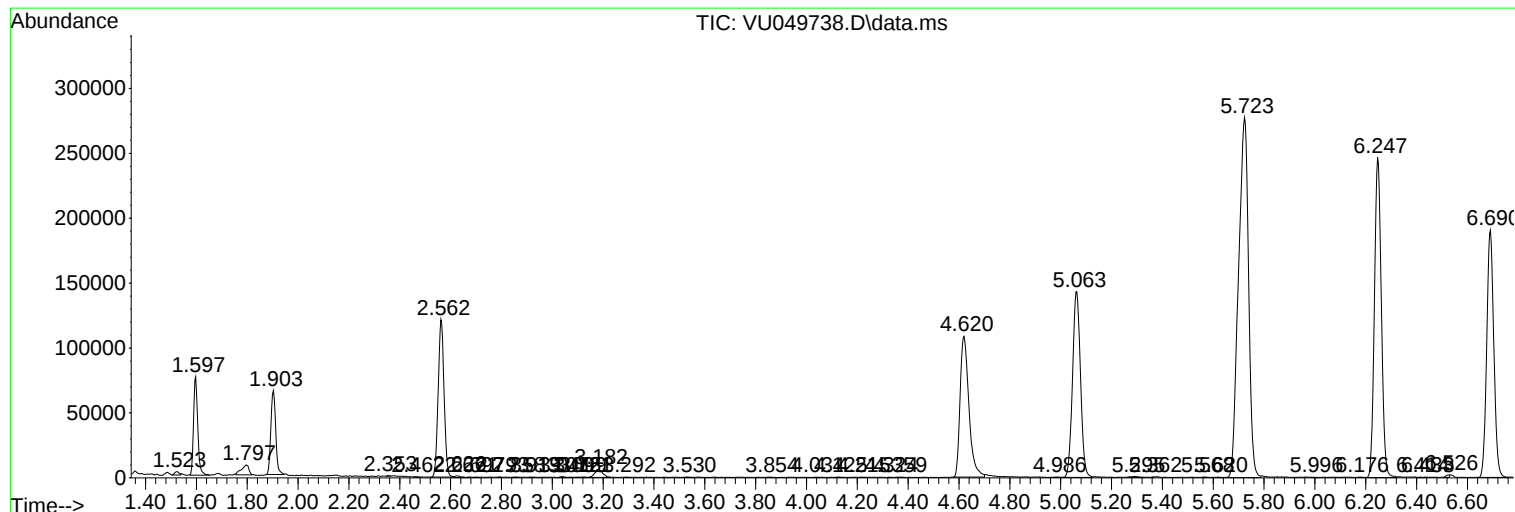

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
Data File : VU049738.D
Acq On : 15 Jul 2022 15:48
Operator : SY/MD
Sample : N3748-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH0E3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
Data File : VU049738.D
Acq On : 15 Jul 2022 15:48
Operator : SY/MD
Sample : N3748-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH0E3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------