
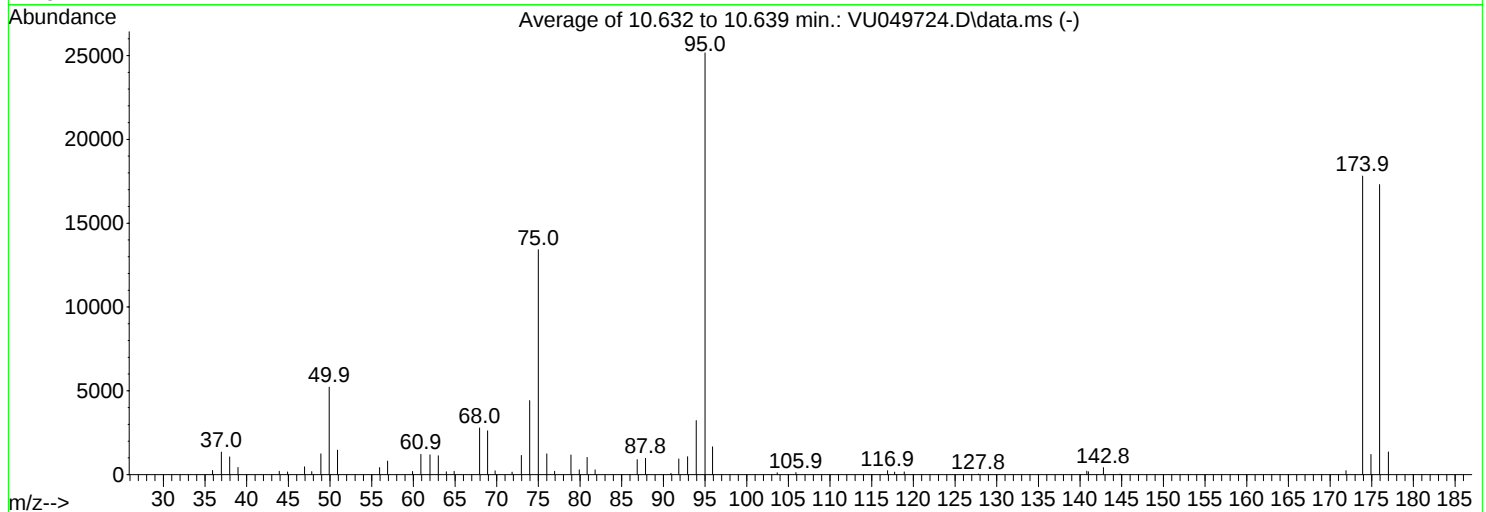


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071522\
Data File : VU049724.D
Acq On : 15 Jul 2022 08:49
Operator : SY/MD
Sample : BFB105
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB105

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM071122WMA.M
Title : VOC Analysis
Last Update : Fri Jul 15 23:03:46 2022

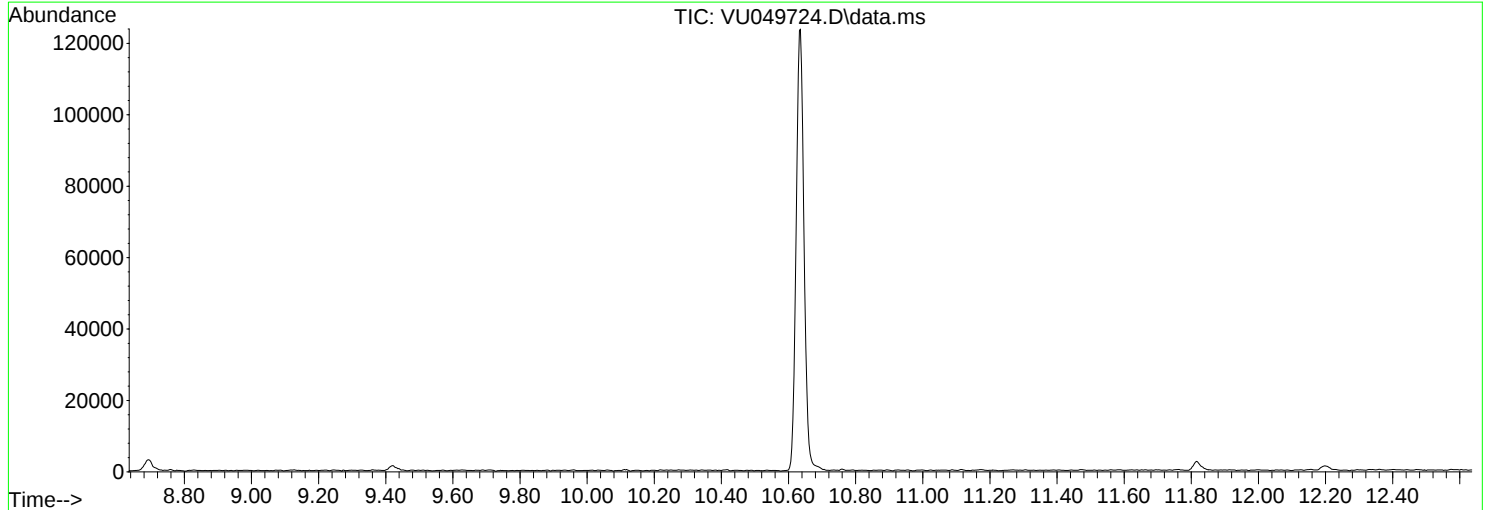

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.8	5225	PASS
75	95	30	80	53.3	13421	PASS
95	95	100	100	100.0	25163	PASS
96	95	5	9	6.6	1658	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.8	17813	PASS
175	174	5	9	6.8	1205	PASS
176	174	95	101	97.2	17307	PASS
177	176	5	9	7.8	1358	PASS

m/z	Abundance
39.80	165.0
43.90	247.0

Instrument :
MSVOA_U
ClientSampleId :
BFB105

m/z	Abundance
35.90	304.0
36.90	1503.0
38.00	1151.0
38.90	435.0
39.90	166.0
44.00	493.0
44.90	151.0
47.00	533.0
47.80	215.0
48.90	1334.0
49.90	5594.0
50.90	1537.0
56.00	478.0
56.90	804.0
59.80	224.0
60.90	1148.0
62.00	1277.0
63.00	1237.0
64.00	167.0
64.90	193.0
68.00	2870.0
68.90	2725.0
69.80	198.0
71.80	181.0
73.00	1214.0
74.00	4664.0
75.00	13745.0
76.00	1369.0
77.00	154.0
78.90	1212.0
79.90	264.0
80.80	1142.0
81.80	289.0
86.90	967.0
87.80	992.0
90.90	108.0
91.90	1024.0
92.90	1055.0
93.90	3240.0
95.00	25992.0
95.90	1816.0
103.70	119.0
105.90	127.0
116.90	206.0
117.70	167.0
118.90	147.0
127.80	108.0
140.80	333.0
142.80	421.0
171.80	226.0
173.90	17912.0
174.90	1252.0
175.90	17000.0
177.00	1312.0

Instrument :
MSVOA_U
ClientSampleId :
BFB105

m/z	Abundance
35.90	269.0
37.00	1360.0
38.00	1065.0
39.00	423.0
39.90	134.0
44.00	427.0
44.90	166.0
46.90	490.0
47.80	175.0
48.90	1293.0
49.90	5424.0
50.90	1507.0
55.90	436.0
56.90	835.0
59.90	183.0
60.90	1215.0
62.00	1213.0
63.00	1158.0
63.90	178.0
64.90	218.0
68.00	2862.0
68.90	2715.0
69.80	226.0
71.90	159.0
72.90	1163.0
74.00	4552.0
75.00	13850.0
76.00	1296.0
77.00	232.0
78.90	1180.0
79.90	271.0
80.80	1051.0
81.80	302.0
86.90	895.0
87.90	995.0
90.90	108.0
91.90	955.0
92.90	1099.0
94.00	3300.0
95.00	26120.0
95.90	1684.0
103.60	118.0
105.90	132.0
116.90	253.0
117.70	147.0
118.90	172.0
140.80	284.0
141.00	285.0
142.80	418.0
171.90	246.0
173.90	18248.0
174.90	1206.0
176.00	17904.0
177.00	1388.0

Instrument :
MSVOA_U
ClientSampleId :
BFB105

m/z	Abundance
35.90	185.0
37.00	1178.0
37.90	967.0
38.90	432.0
40.00	114.0
43.90	408.0
44.90	178.0
46.90	387.0
47.80	149.0
48.90	1107.0
49.90	4656.0
50.90	1328.0
55.90	362.0
56.90	783.0
60.00	171.0
60.90	1281.0
62.00	1063.0
63.00	987.0
63.90	164.0
64.90	201.0
67.90	2623.0
68.90	2397.0
69.80	253.0
71.90	131.0
72.90	1057.0
73.90	4030.0
75.00	12668.0
76.00	1058.0
76.90	224.0
78.90	1118.0
79.90	320.0
80.90	895.0
81.80	265.0
86.80	837.0
87.90	937.0
91.80	840.0
92.90	1051.0
94.00	3145.0
95.00	23376.0
95.90	1475.0
103.70	117.0
105.90	111.0
116.90	252.0
117.80	145.0
118.90	169.0
141.00	241.0
142.80	408.0
144.80	101.0
172.00	257.0
173.90	17280.0
174.90	1157.0
176.00	17016.0
177.00	1373.0

Instrument :
MSVOA_U
ClientSampleId :
BFB105