

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
 Data File : VU059938.D
 Acq On : 15 Jul 2024 10:08
 Operator : MD/SY
 Sample : VU0715WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK094

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M

Title : VOC Analysis

Signal : TIC: VU059938.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	114	rVB	99977	121053	13.74%	1.721%
2	1.766	143	148	155	rVB3	6438	7494	0.85%	0.107%
3	1.907	184	192	208	rBV	80629	112109	12.72%	1.594%
4	2.518	378	382	383	rBV2	467	336	0.04%	0.005%
5	2.560	383	395	411	rVV	170727	280479	31.83%	3.989%
6	2.788	458	466	474	rVB2	1668	2562	0.29%	0.036%
7	2.930	504	510	513	rBV2	231	247	0.03%	0.004%
8	3.033	537	542	546	rBV2	1271	1448	0.16%	0.021%
9	3.174	577	586	593	rBV4	762	1201	0.14%	0.017%
10	3.232	600	604	609	rBV2	233	247	0.03%	0.004%
11	3.284	614	620	623	rBV2	319	296	0.03%	0.004%
12	3.309	624	628	633	rVB2	226	235	0.03%	0.003%
13	3.351	633	641	647	rBV5	1193	1695	0.19%	0.024%
14	3.869	798	802	805	rBV2	333	298	0.03%	0.004%
15	3.975	832	835	846	rVB2	259	350	0.04%	0.005%
16	4.068	860	864	871	rBV2	287	284	0.03%	0.004%
17	4.216	904	910	913	rBV2	218	256	0.03%	0.004%
18	4.264	922	925	931	rVB2	255	272	0.03%	0.004%
19	4.615	1025	1034	1072	rBV	91035	233940	26.55%	3.327%
20	4.875	1112	1115	1120	rBV2	290	276	0.03%	0.004%
21	4.978	1142	1147	1152	rVB4	753	713	0.08%	0.010%
22	5.055	1152	1171	1196	rBV	159107	351677	39.91%	5.001%
23	5.232	1224	1226	1233	rVB4	393	314	0.04%	0.004%
24	5.296	1244	1246	1249	rVV2	685	531	0.06%	0.008%
25	5.312	1249	1251	1254	rVV	627	415	0.05%	0.006%
26	5.390	1273	1275	1280	rVB3	434	401	0.05%	0.006%
27	5.428	1280	1287	1292	rVB3	391	501	0.06%	0.007%
28	5.518	1310	1315	1319	rBV2	623	720	0.08%	0.010%
29	5.647	1349	1355	1358	rBV2	267	257	0.03%	0.004%
30	5.718	1358	1377	1417	rVV2	323360	881281	100.00%	12.532%
31	5.881	1426	1428	1431	rVB	393	232	0.03%	0.003%
32	6.123	1497	1503	1514	rVB3	639	1066	0.12%	0.015%
33	6.242	1528	1540	1573	rBV	299095	583929	66.26%	8.304%
34	6.528	1621	1629	1631	rBV6	2648	3043	0.35%	0.043%
35	6.602	1648	1652	1655	rBV3	328	250	0.03%	0.004%
36	6.685	1664	1678	1694	rBV	197607	390383	44.30%	5.551%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
 Data File : VU059938.D
 Acq On : 15 Jul 2024 10:08
 Operator : MD/SY
 Sample : VU0715WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK094

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	6.801	1711	1714	1720	rVB4	1145	934	0.11%	0.013%
38	6.975	1762	1768	1772	rBV2	269	365	0.04%	0.005%
39	7.110	1801	1810	1815	rBV2	624	934	0.11%	0.013%
40	7.193	1829	1836	1837	rBV2	369	363	0.04%	0.005%
41	7.267	1855	1859	1862	rVV2	332	257	0.03%	0.004%
42	7.357	1883	1887	1893	rVB	358	398	0.05%	0.006%
43	7.428	1903	1909	1913	rBV2	244	270	0.03%	0.004%
44	7.560	1937	1950	1974	rBV	103681	189863	21.54%	2.700%
45	7.788	2014	2021	2022	rBV3	783	778	0.09%	0.011%
46	7.801	2022	2025	2029	rVB2	576	405	0.05%	0.006%
47	7.894	2041	2054	2073	rBV	377937	664962	75.45%	9.456%
48	8.177	2128	2142	2162	rBV	70863	126603	14.37%	1.800%
49	8.332	2187	2190	2196	rBV3	452	371	0.04%	0.005%
50	8.396	2206	2210	2216	rVB4	653	768	0.09%	0.011%
51	8.473	2225	2234	2237	rBV2	608	963	0.11%	0.014%
52	8.512	2242	2246	2251	rVB3	442	365	0.04%	0.005%
53	8.550	2251	2258	2267	rBV5	1271	2157	0.24%	0.031%
54	8.627	2271	2282	2317	rBV	250612	476209	54.04%	6.772%
55	8.798	2333	2335	2336	rBV3	641	271	0.03%	0.004%
56	8.852	2349	2352	2356	rBV2	465	259	0.03%	0.004%
57	8.920	2369	2373	2380	rBV3	645	814	0.09%	0.012%
58	9.309	2488	2494	2499	rVB2	235	299	0.03%	0.004%
59	9.412	2514	2526	2550	rBV	437919	748420	84.92%	10.643%
60	9.569	2570	2575	2581	rBV3	1278	1353	0.15%	0.019%
61	9.701	2607	2616	2619	rBV2	1402	2143	0.24%	0.030%
62	9.875	2665	2670	2675	rVB	243	234	0.03%	0.003%
63	10.055	2722	2726	2730	rBV2	318	251	0.03%	0.004%
64	10.106	2734	2742	2746	rBV4	1246	1645	0.19%	0.023%
65	10.161	2757	2759	2766	rVB2	292	257	0.03%	0.004%
66	10.286	2795	2798	2802	rBV2	562	345	0.04%	0.005%
67	10.483	2853	2859	2866	rBV4	1047	1469	0.17%	0.021%
68	10.647	2907	2910	2916	rVB4	567	513	0.06%	0.007%
69	10.749	2924	2942	2959	rBV	316918	519127	58.91%	7.382%
70	10.884	2981	2984	2986	rBV2	531	355	0.04%	0.005%
71	11.097	3041	3050	3059	rVB4	1067	1655	0.19%	0.024%
72	11.409	3144	3147	3150	rBV	334	246	0.03%	0.003%
73	11.470	3158	3166	3176	rBV4	995	1550	0.18%	0.022%
74	11.749	3245	3253	3260	rBV4	1925	2837	0.32%	0.040%
75	11.807	3260	3271	3289	rBV	399832	661999	75.12%	9.414%
76	11.936	3309	3311	3316	rBV3	417	361	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
 Data File : VU059938.D
 Acq On : 15 Jul 2024 10:08
 Operator : MD/SY
 Sample : VU0715WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK094

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	12.087	3355	3358	3362	rBV3	322	244	0.03%	0.003%
78	12.190	3377	3390	3415	rBV	365075	615621	69.86%	8.754%
79	12.447	3467	3470	3473	rVB2	343	235	0.03%	0.003%
80	12.466	3473	3476	3480	rBV2	454	341	0.04%	0.005%
81	12.929	3616	3620	3622	rBV2	303	234	0.03%	0.003%
82	13.225	3707	3712	3714	rBV2	721	632	0.07%	0.009%
83	13.315	3737	3740	3745	rBV	306	344	0.04%	0.005%
84	13.544	3807	3811	3815	rVB2	474	425	0.05%	0.006%
85	13.572	3816	3820	3825	rVV2	371	402	0.05%	0.006%
86	13.659	3843	3847	3852	rBV2	305	380	0.04%	0.005%
87	13.685	3852	3855	3860	rVV	302	255	0.03%	0.004%
88	13.817	3893	3896	3900	rBV	286	246	0.03%	0.003%
89	13.852	3900	3907	3918	rVV5	2409	3719	0.42%	0.053%
90	14.100	3976	3984	3998	rBV3	2735	6081	0.69%	0.086%
91	14.222	4019	4022	4024	rBV2	406	297	0.03%	0.004%
92	14.335	4048	4057	4065	rVV5	2518	4114	0.47%	0.059%
93	14.447	4089	4092	4097	rBV2	435	412	0.05%	0.006%
94	14.492	4102	4106	4109	rVB2	385	290	0.03%	0.004%
95	14.508	4109	4111	4114	rBV2	361	245	0.03%	0.003%
96	14.736	4179	4182	4185	rBV2	423	373	0.04%	0.005%
97	15.048	4275	4279	4281	rBV2	428	400	0.05%	0.006%
98	15.251	4335	4342	4347	rBV5	1239	1830	0.21%	0.026%
99	15.354	4371	4374	4377	rBV2	476	304	0.03%	0.004%
100	15.418	4390	4394	4395	rBV2	688	536	0.06%	0.008%




Sum of corrected areas: 7032119

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
Data File : VU059938.D
Acq On : 15 Jul 2024 10:08
Operator : MD/SY
Sample : VU0715WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK094

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

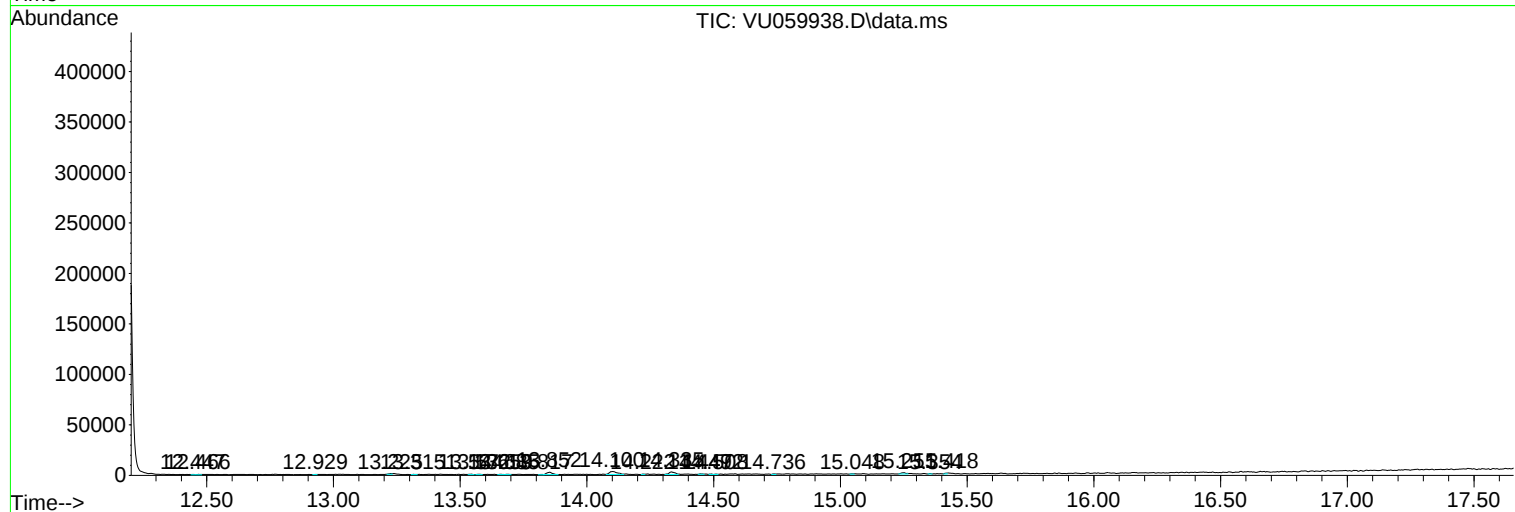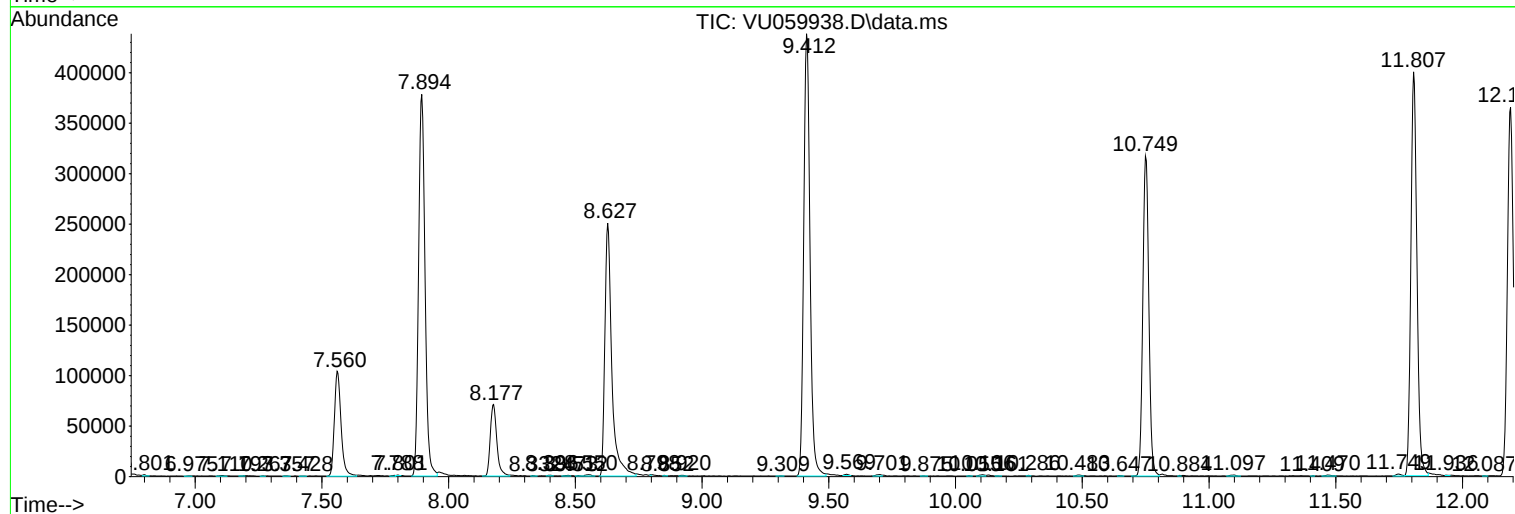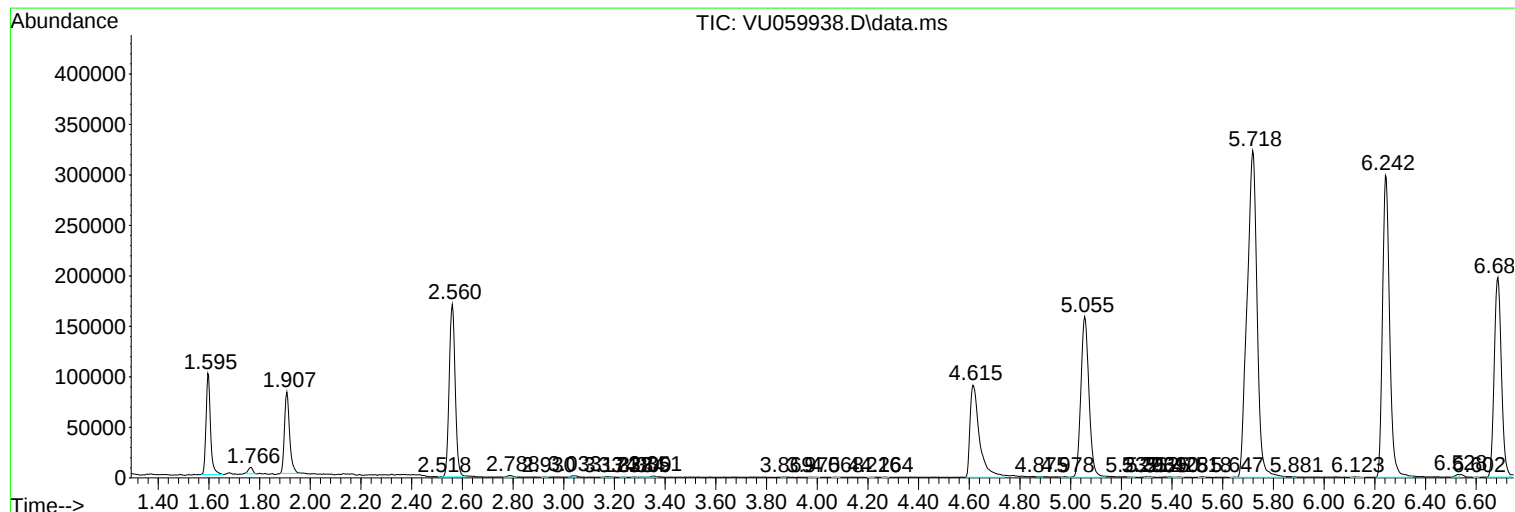

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
Data File : VU059938.D
Acq On : 15 Jul 2024 10:08
Operator : MD/SY
Sample : VU0715WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK094

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
Data File : VU059938.D
Acq On : 15 Jul 2024 10:08
Operator : MD/SY
Sample : VU0715WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK094

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------