

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
 Data File : VU059939.D
 Acq On : 15 Jul 2024 10:31
 Operator : MD/SY
 Sample : P3231-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08F0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

Signal : TIC: VU059939.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	111	rBV	97594	117077	13.50%	1.707%
2	1.679	115	121	131	rVB	16039	19771	2.28%	0.288%
3	1.908	184	192	206	rBV	82216	114356	13.19%	1.668%
4	2.560	380	395	410	rBV	165832	273625	31.56%	3.990%
5	2.756	450	456	459	rBV3	834	1012	0.12%	0.015%
6	3.036	538	543	552	rVB2	1013	1481	0.17%	0.022%
7	3.110	563	566	571	rVB2	290	257	0.03%	0.004%
8	3.178	571	587	601	rVB3	2239	5183	0.60%	0.076%
9	3.252	607	610	613	rBV2	249	224	0.03%	0.003%
10	3.348	637	640	642	rBV3	678	466	0.05%	0.007%
11	3.409	656	659	666	rVB2	292	260	0.03%	0.004%
12	3.451	666	672	673	rBV2	251	208	0.02%	0.003%
13	3.698	745	749	753	rBV2	289	289	0.03%	0.004%
14	3.811	779	784	786	rBV2	229	218	0.03%	0.003%
15	3.911	810	815	820	rBV2	286	349	0.04%	0.005%
16	4.007	842	845	849	rVB	272	202	0.02%	0.003%
17	4.518	991	1004	1005	rBV3	3378	3904	0.45%	0.057%
18	4.615	1021	1034	1070	rBV	92334	235261	27.13%	3.431%
19	5.055	1155	1171	1195	rBV2	158090	349941	40.36%	5.103%
20	5.158	1201	1203	1206	rBV3	369	244	0.03%	0.004%
21	5.412	1278	1282	1286	rBV2	251	317	0.04%	0.005%
22	5.612	1339	1344	1352	rBV2	226	264	0.03%	0.004%
23	5.718	1357	1377	1400	rBV2	321095	867031	100.00%	12.644%
24	5.920	1437	1440	1444	rBV3	278	248	0.03%	0.004%
25	6.033	1473	1475	1479	rBV4	291	254	0.03%	0.004%
26	6.123	1500	1503	1507	rVB3	493	368	0.04%	0.005%
27	6.245	1525	1541	1567	rBV	282263	549762	63.41%	8.017%
28	6.525	1622	1628	1629	rBV3	1560	1405	0.16%	0.020%
29	6.605	1648	1653	1656	rBV2	437	409	0.05%	0.006%
30	6.685	1664	1678	1696	rBV	194796	389230	44.89%	5.676%
31	6.814	1715	1718	1722	rVB3	658	533	0.06%	0.008%
32	6.885	1734	1740	1746	rVB	214	277	0.03%	0.004%
33	6.917	1746	1750	1754	rBV2	303	266	0.03%	0.004%
34	7.033	1779	1786	1790	rBV2	213	275	0.03%	0.004%
35	7.091	1798	1804	1808	rBV2	264	267	0.03%	0.004%
36	7.197	1831	1837	1839	rBV3	427	422	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
 Data File : VU059939.D
 Acq On : 15 Jul 2024 10:31
 Operator : MD/SY
 Sample : P3231-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08F0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	7.251	1850	1854	1861	rVB2	193	261	0.03%	0.004%
38	7.325	1872	1877	1880	rBV2	200	229	0.03%	0.003%
39	7.412	1898	1904	1907	rBV	275	296	0.03%	0.004%
40	7.560	1934	1950	1973	rBV	103536	188814	21.78%	2.753%
41	7.756	2007	2011	2014	rVB3	282	227	0.03%	0.003%
42	7.772	2014	2016	2020	rBV	310	211	0.02%	0.003%
43	7.894	2039	2054	2074	rBV	371490	661630	76.31%	9.648%
44	8.174	2130	2141	2166	rBV2	70612	126464	14.59%	1.844%
45	8.319	2180	2186	2188	rBV2	305	362	0.04%	0.005%
46	8.332	2188	2190	2193	rVV2	414	271	0.03%	0.004%
47	8.364	2197	2200	2207	rVV3	377	373	0.04%	0.005%
48	8.467	2218	2232	2244	rBV	4427	8055	0.93%	0.117%
49	8.554	2255	2259	2260	rBV	406	223	0.03%	0.003%
50	8.628	2271	2282	2315	rBV	244251	464447	53.57%	6.773%
51	8.824	2341	2343	2346	rVB	377	207	0.02%	0.003%
52	9.020	2401	2404	2410	rBV2	313	279	0.03%	0.004%
53	9.142	2440	2442	2447	rVB2	341	232	0.03%	0.003%
54	9.242	2469	2473	2479	rVB2	319	243	0.03%	0.004%
55	9.412	2514	2526	2555	rBV	413882	701516	80.91%	10.230%
56	9.608	2583	2587	2591	rBV3	464	465	0.05%	0.007%
57	9.673	2603	2607	2609	rBV2	302	228	0.03%	0.003%
58	9.689	2609	2612	2613	rVV	384	238	0.03%	0.003%
59	9.701	2613	2616	2624	rVB3	850	854	0.10%	0.012%
60	9.737	2624	2627	2632	rBV2	299	238	0.03%	0.003%
61	9.804	2642	2648	2652	rBV2	191	250	0.03%	0.004%
62	9.833	2654	2657	2661	rVB	307	219	0.03%	0.003%
63	10.110	2740	2743	2747	rVB2	565	389	0.04%	0.006%
64	10.264	2787	2791	2795	rVB	365	261	0.03%	0.004%
65	10.402	2831	2834	2837	rBV2	302	234	0.03%	0.003%
66	10.534	2870	2875	2877	rBV	231	209	0.02%	0.003%
67	10.570	2882	2886	2888	rVV2	380	238	0.03%	0.003%
68	10.689	2920	2923	2928	rVB2	276	265	0.03%	0.004%
69	10.750	2929	2942	2961	rBV	314222	513794	59.26%	7.493%
70	10.888	2975	2985	2995	rVB2	5657	9178	1.06%	0.134%
71	11.470	3162	3166	3169	rBV	274	203	0.02%	0.003%
72	11.557	3188	3193	3196	rBV2	291	239	0.03%	0.003%
73	11.750	3246	3253	3258	rBV4	831	1022	0.12%	0.015%
74	11.807	3258	3271	3291	rBV	379792	619581	71.46%	9.035%
75	12.010	3331	3334	3339	rVB3	243	251	0.03%	0.004%
76	12.071	3350	3353	3358	rVB2	385	330	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
 Data File : VU059939.D
 Acq On : 15 Jul 2024 10:31
 Operator : MD/SY
 Sample : P3231-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08F0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	12.190	3377	3390	3411	rBV	366332	606531	69.95%	8.845%
78	12.489	3480	3483	3487	rBV	404	277	0.03%	0.004%
79	12.602	3515	3518	3521	rBV	313	217	0.03%	0.003%
80	12.769	3563	3570	3582	rVB3	2170	3590	0.41%	0.052%
81	12.817	3582	3585	3587	rBV2	330	206	0.02%	0.003%
82	13.235	3710	3715	3723	rVB4	661	878	0.10%	0.013%
83	13.479	3789	3791	3795	rVB2	383	208	0.02%	0.003%
84	13.505	3796	3799	3802	rBV	409	267	0.03%	0.004%
85	13.753	3873	3876	3879	rBV	243	213	0.02%	0.003%
86	13.843	3901	3904	3906	rBV2	383	274	0.03%	0.004%
87	13.965	3938	3942	3945	rVB3	402	308	0.04%	0.004%
88	14.049	3966	3968	3972	rBV2	331	248	0.03%	0.004%
89	14.110	3984	3987	3991	rVB3	988	749	0.09%	0.011%
90	14.174	4004	4007	4011	rBV3	353	262	0.03%	0.004%
91	14.312	4045	4050	4053	rBV2	510	566	0.07%	0.008%
92	14.341	4054	4059	4062	rVV4	1045	982	0.11%	0.014%
93	14.486	4102	4104	4107	rBV2	339	221	0.03%	0.003%
94	14.515	4110	4113	4116	rBV2	442	283	0.03%	0.004%
95	14.676	4160	4163	4165	rBV2	416	227	0.03%	0.003%
96	14.692	4165	4168	4169	rBV2	382	202	0.02%	0.003%
97	14.746	4183	4185	4190	rVB2	430	252	0.03%	0.004%
98	14.920	4235	4239	4240	rBV2	545	375	0.04%	0.005%
99	14.955	4248	4250	4254	rBV3	336	273	0.03%	0.004%
100	15.251	4336	4342	4346	rBV4	856	1109	0.13%	0.016%




Sum of corrected areas: 6857400

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
Data File : VU059939.D
Acq On : 15 Jul 2024 10:31
Operator : MD/SY
Sample : P3231-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08F0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

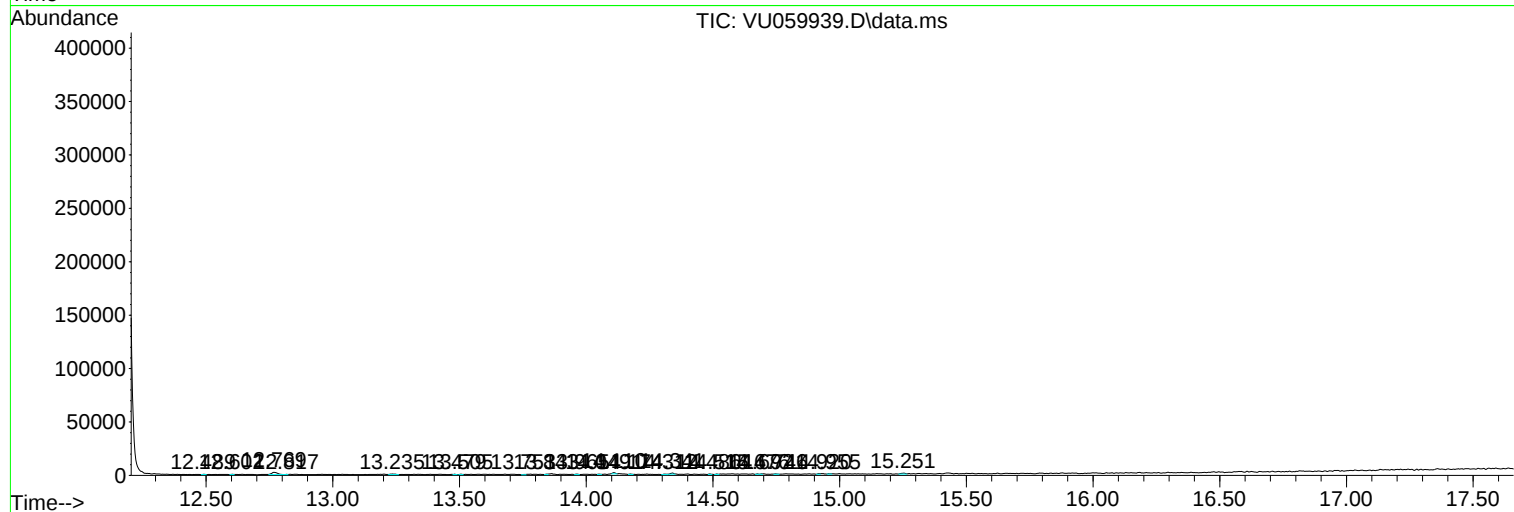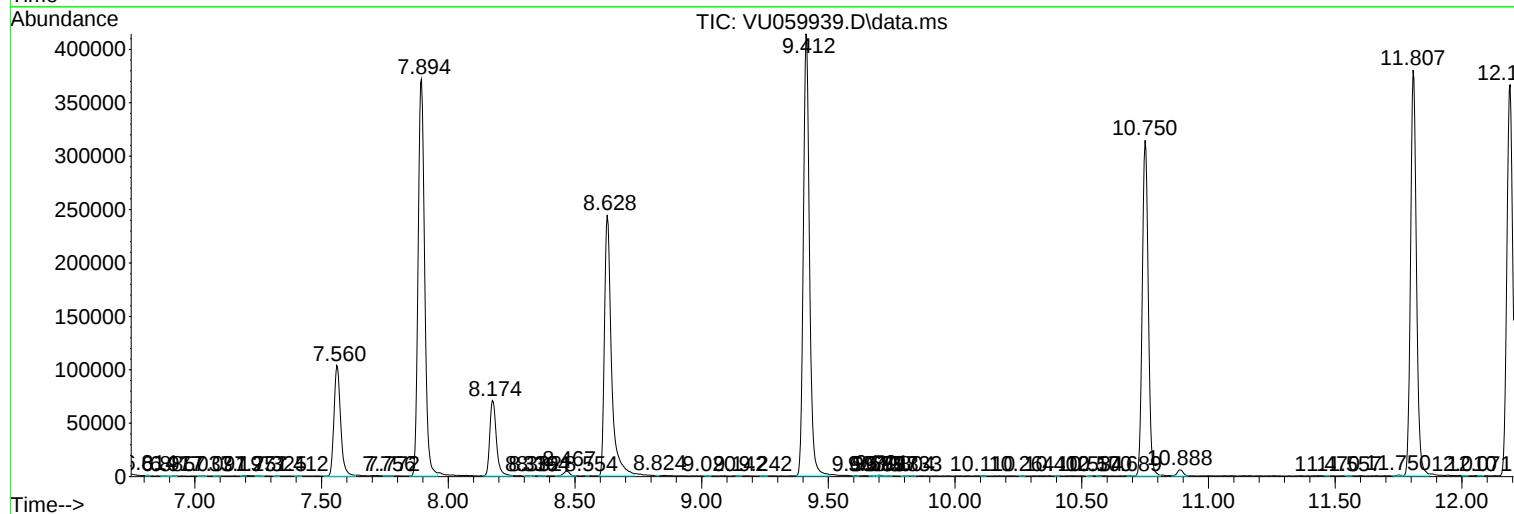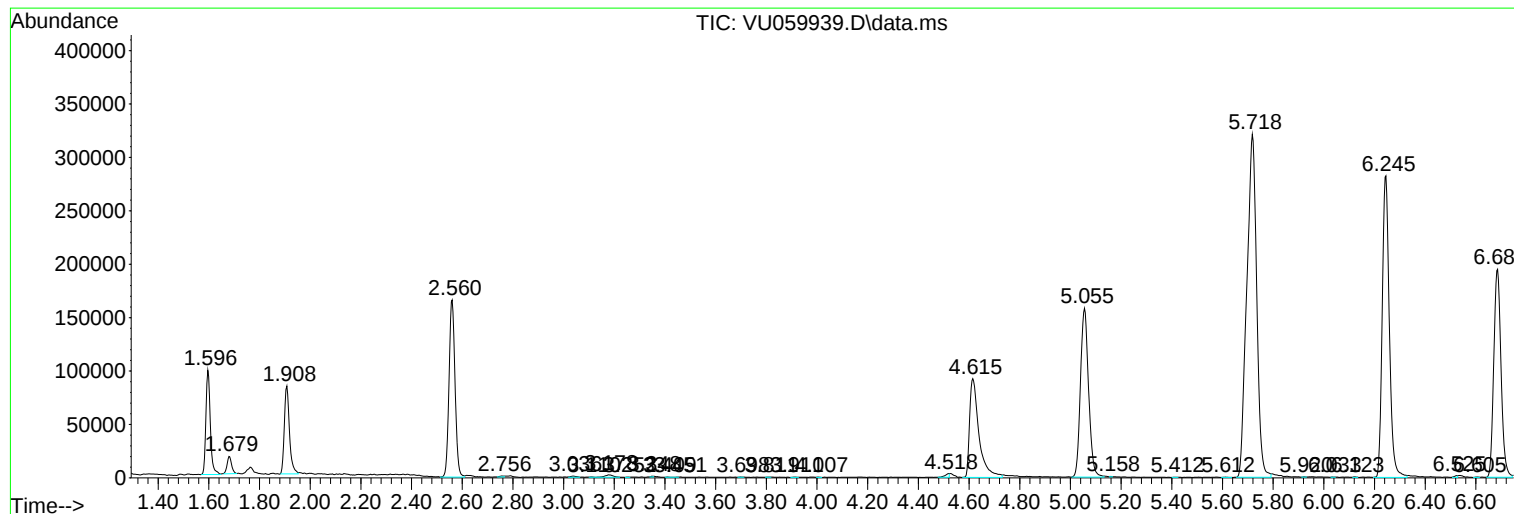

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
Data File : VU059939.D
Acq On : 15 Jul 2024 10:31
Operator : MD/SY
Sample : P3231-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08F0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
Data File : VU059939.D
Acq On : 15 Jul 2024 10:31
Operator : MD/SY
Sample : P3231-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08F0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc