

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
 Data File : VU059940.D
 Acq On : 15 Jul 2024 10:53
 Operator : MD/SY
 Sample : P3231-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08F3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

Signal : TIC: VU059940.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	89	95	106	rBV	90779	101895	12.34%	1.535%
2	1.679	116	121	131	rVB	17070	20474	2.48%	0.308%
3	1.907	185	192	211	rVB	76202	107362	13.00%	1.618%
4	2.560	383	395	409	rBV	157337	255543	30.95%	3.850%
5	2.991	526	529	532	rBV	292	165	0.02%	0.002%
6	3.026	537	540	542	rBV2	608	433	0.05%	0.007%
7	3.325	632	633	635	rBV2	71	26	0.00%	0.000%
8	3.393	651	654	656	rBV2	229	137	0.02%	0.002%
9	3.608	717	721	726	rBV2	280	284	0.03%	0.004%
10	3.634	726	729	735	rBV2	187	213	0.03%	0.003%
11	3.682	742	744	746	rBV	176	114	0.01%	0.002%
12	3.776	769	773	775	rBV2	170	140	0.02%	0.002%
13	3.866	797	801	805	rBV2	295	295	0.04%	0.004%
14	3.988	836	839	841	rBV	208	137	0.02%	0.002%
15	4.020	846	849	855	rVB2	311	231	0.03%	0.003%
16	4.113	875	878	881	rBV	209	157	0.02%	0.002%
17	4.222	907	912	914	rBV	201	200	0.02%	0.003%
18	4.358	951	954	957	rBV2	152	125	0.02%	0.002%
19	4.377	957	960	963	rVB	239	156	0.02%	0.002%
20	4.454	981	984	987	rBV	191	137	0.02%	0.002%
21	4.493	992	996	998	rBV2	293	249	0.03%	0.004%
22	4.615	1024	1034	1066	rBV2	86176	216933	26.27%	3.268%
23	5.055	1155	1171	1199	rBV	148519	330253	39.99%	4.976%
24	5.280	1238	1241	1244	rVB2	465	253	0.03%	0.004%
25	5.300	1244	1247	1249	rBV3	494	313	0.04%	0.005%
26	5.341	1258	1260	1263	rVB	132	66	0.01%	0.001%
27	5.406	1278	1280	1282	rBV	121	68	0.01%	0.001%
28	5.473	1298	1301	1305	rBV2	210	196	0.02%	0.003%
29	5.563	1327	1329	1333	rBV2	64	42	0.01%	0.001%
30	5.586	1333	1336	1338	rBV	202	137	0.02%	0.002%
31	5.718	1357	1377	1417	rBV2	300260	825762	100.00%	12.441%
32	5.968	1453	1455	1457	rBV	169	73	0.01%	0.001%
33	6.001	1462	1465	1467	rBV2	310	241	0.03%	0.004%
34	6.084	1489	1491	1494	rBV	252	184	0.02%	0.003%
35	6.110	1495	1499	1502	rVB	400	280	0.03%	0.004%
36	6.129	1502	1505	1508	rBV	148	128	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
 Data File : VU059940.D
 Acq On : 15 Jul 2024 10:53
 Operator : MD/SY
 Sample : P3231-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08F3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	6.161	1512	1515	1516	rBV3	324	196	0.02%	0.003%
38	6.242	1526	1540	1567	rBV	300522	574952	69.63%	8.662%
39	6.534	1623	1631	1636	rVB5	1783	2345	0.28%	0.035%
40	6.599	1648	1651	1653	rBV2	103	63	0.01%	0.001%
41	6.682	1664	1677	1704	rBV	190344	372185	45.07%	5.608%
42	6.914	1746	1749	1750	rBV	114	71	0.01%	0.001%
43	7.029	1782	1785	1789	rVB2	179	147	0.02%	0.002%
44	7.055	1790	1793	1798	rBV2	197	204	0.02%	0.003%
45	7.197	1831	1837	1848	rBV4	663	1240	0.15%	0.019%
46	7.335	1878	1880	1882	rBV	125	75	0.01%	0.001%
47	7.560	1939	1950	1975	rBV	96137	174306	21.11%	2.626%
48	7.798	2021	2024	2028	rVB2	260	157	0.02%	0.002%
49	7.891	2040	2053	2074	rBV	355451	627059	75.94%	9.448%
50	8.174	2131	2141	2159	rBV	67153	116095	14.06%	1.749%
51	8.345	2187	2194	2195	rBV3	421	397	0.05%	0.006%
52	8.386	2203	2207	2209	rBV3	237	189	0.02%	0.003%
53	8.550	2253	2258	2260	rBV3	355	341	0.04%	0.005%
54	8.627	2269	2282	2320	rBV	231274	447381	54.18%	6.740%
55	8.904	2367	2368	2373	rVB2	443	207	0.03%	0.003%
56	9.036	2404	2409	2412	rBV2	383	347	0.04%	0.005%
57	9.055	2413	2415	2417	rVB	331	125	0.02%	0.002%
58	9.081	2419	2423	2426	rBV	184	169	0.02%	0.003%
59	9.139	2433	2441	2444	rBV2	384	554	0.07%	0.008%
60	9.206	2459	2462	2463	rBV	168	103	0.01%	0.002%
61	9.258	2474	2478	2482	rBV	281	244	0.03%	0.004%
62	9.412	2513	2526	2550	rBV	433630	728981	88.28%	10.983%
63	9.637	2593	2596	2599	rBV2	233	150	0.02%	0.002%
64	9.676	2604	2608	2609	rBV	287	200	0.02%	0.003%
65	9.685	2609	2611	2615	rVV4	310	212	0.03%	0.003%
66	9.791	2641	2644	2646	rBV	152	88	0.01%	0.001%
67	9.907	2675	2680	2686	rBV	363	366	0.04%	0.006%
68	9.936	2686	2689	2691	rBV2	226	114	0.01%	0.002%
69	9.952	2691	2694	2696	rBV	306	204	0.02%	0.003%
70	9.994	2704	2707	2711	rVB	353	174	0.02%	0.003%
71	10.055	2723	2726	2727	rBV	204	129	0.02%	0.002%
72	10.145	2752	2754	2757	rBV	198	103	0.01%	0.002%
73	10.168	2758	2761	2765	rBV2	205	193	0.02%	0.003%
74	10.225	2776	2779	2781	rBV	234	154	0.02%	0.002%
75	10.361	2814	2821	2823	rBV2	191	230	0.03%	0.003%
76	10.611	2897	2899	2901	rBV	226	123	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
Data File : VU059940.D
Acq On : 15 Jul 2024 10:53
Operator : MD/SY
Sample : P3231-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08F3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M

Title : VOC Analysis

77	10.750	2929	2942	2964	rBV	299655	489030	59.22%	7.368%
78	10.891	2977	2986	2995	rBV4	3419	4950	0.60%	0.075%
79	10.936	2998	3000	3003	rBV2	190	101	0.01%	0.002%
80	11.174	3071	3074	3075	rBV	270	159	0.02%	0.002%
81	11.422	3143	3151	3154	rBV2	352	506	0.06%	0.008%
82	11.746	3250	3252	3257	rVB2	470	350	0.04%	0.005%
83	11.807	3259	3271	3297	rBV	391222	653688	79.16%	9.849%
84	11.978	3321	3324	3327	rBV3	544	374	0.05%	0.006%
85	12.007	3331	3333	3340	rVV2	302	259	0.03%	0.004%
86	12.190	3378	3390	3413	rBV	341642	573643	69.47%	8.643%
87	14.184	4007	4010	4012	rBV2	409	231	0.03%	0.003%




Sum of corrected areas: 6637266

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
Data File : VU059940.D
Acq On : 15 Jul 2024 10:53
Operator : MD/SY
Sample : P3231-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08F3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

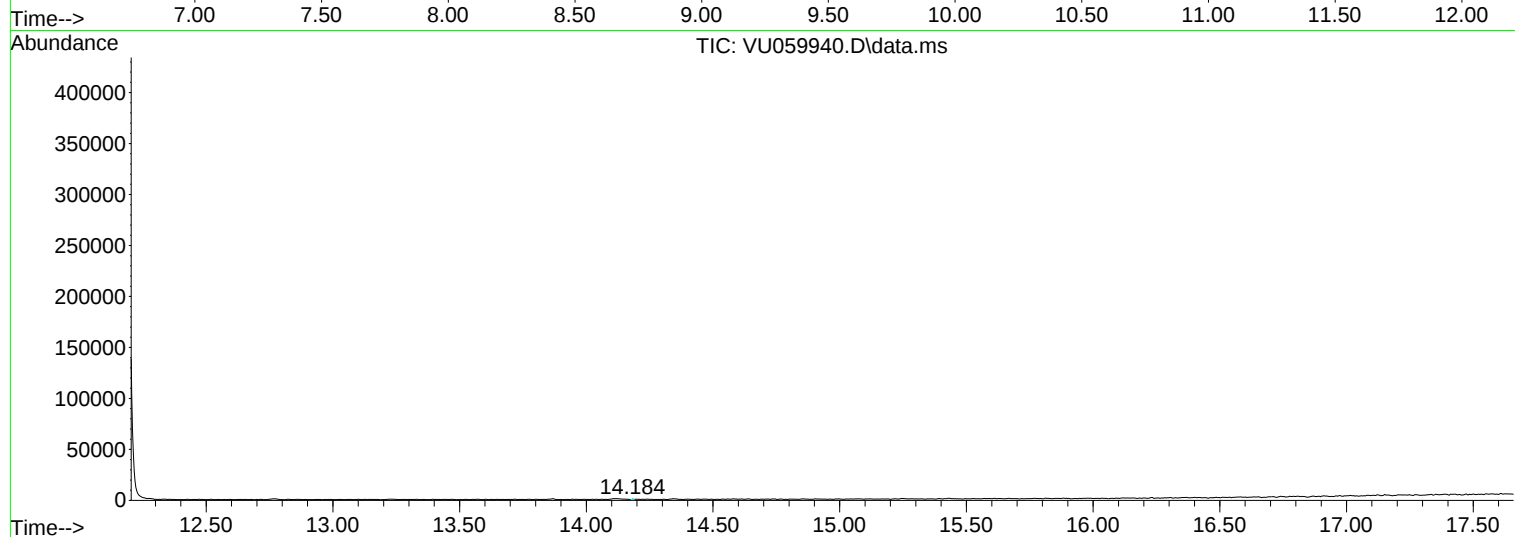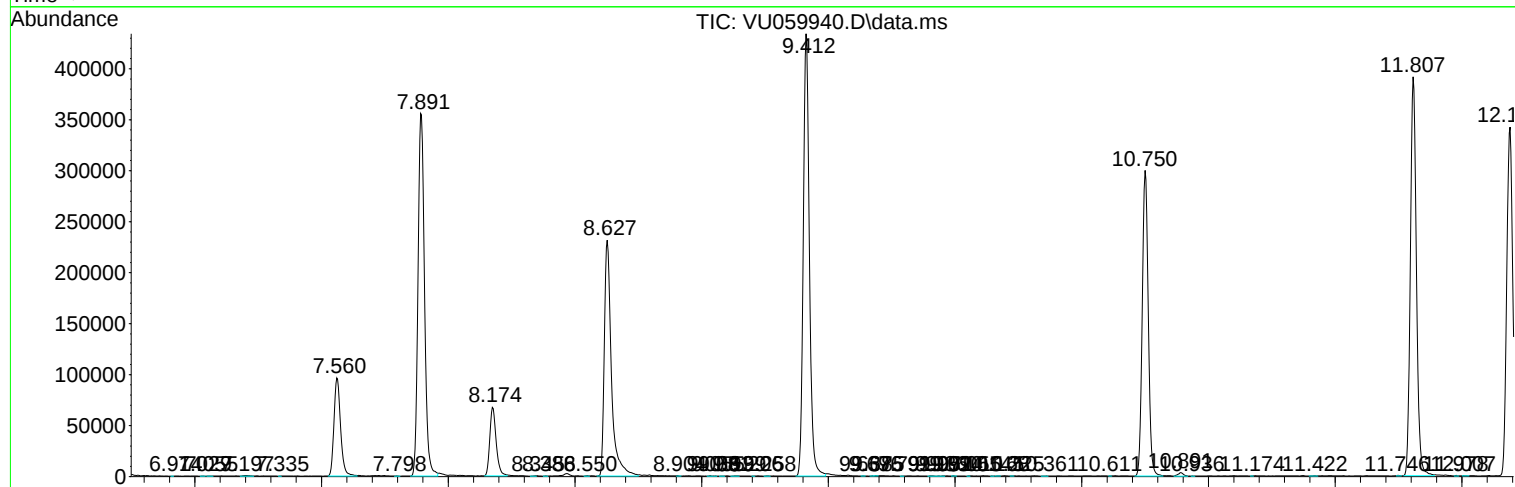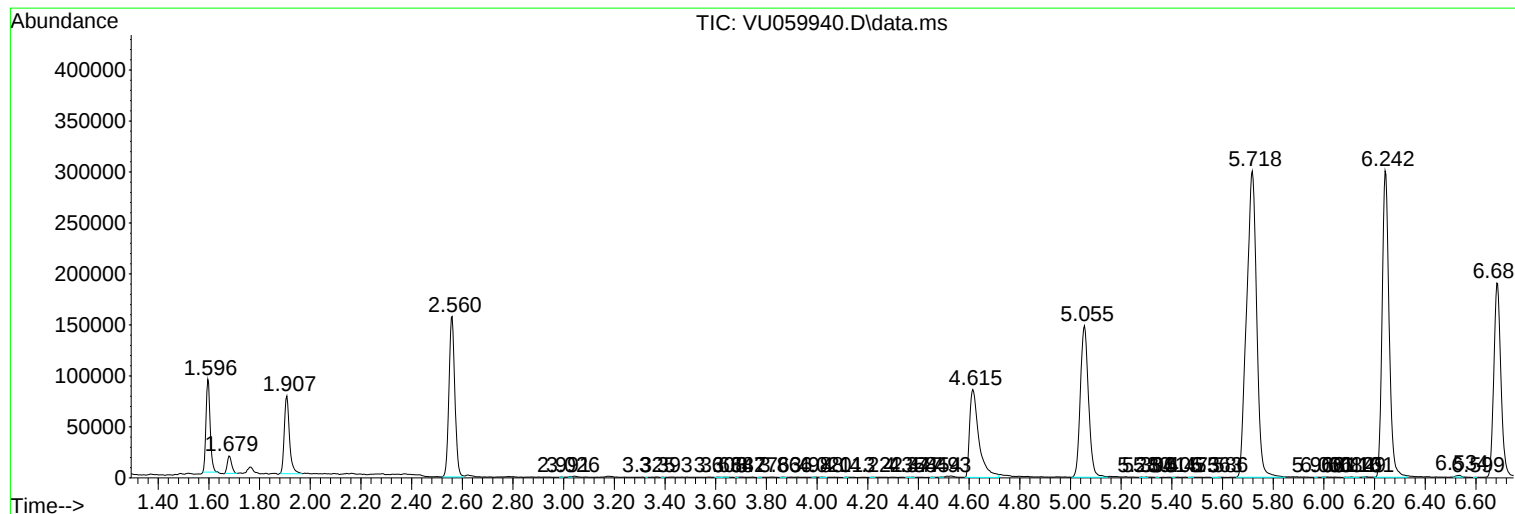

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
Data File : VU059940.D
Acq On : 15 Jul 2024 10:53
Operator : MD/SY
Sample : P3231-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08F3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
Data File : VU059940.D
Acq On : 15 Jul 2024 10:53
Operator : MD/SY
Sample : P3231-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08F3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc