

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
 Data File : VU059942.D
 Acq On : 15 Jul 2024 11:40
 Operator : MD/SY
 Sample : P3231-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08F2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

Signal : TIC: VU059942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	110	rBV	87749	104963	13.30%	1.670%
2	1.907	185	192	212	rVB	71789	103191	13.08%	1.642%
3	2.560	383	395	410	rBV	148720	240990	30.54%	3.835%
4	2.756	453	456	459	rBV2	870	649	0.08%	0.010%
5	2.872	489	492	493	rBV	163	77	0.01%	0.001%
6	3.046	537	546	554	rBV4	1002	1752	0.22%	0.028%
7	3.149	574	578	579	rBV2	290	195	0.02%	0.003%
8	3.306	622	627	630	rBV2	379	338	0.04%	0.005%
9	3.499	684	687	690	rVB	333	202	0.03%	0.003%
10	3.525	690	695	701	rBV2	383	505	0.06%	0.008%
11	3.702	746	750	754	rVB2	208	186	0.02%	0.003%
12	3.766	767	770	775	rVB2	238	160	0.02%	0.003%
13	3.891	806	809	816	rBV2	211	242	0.03%	0.004%
14	3.959	826	830	833	rVB2	210	155	0.02%	0.002%
15	3.985	834	838	842	rBV2	286	271	0.03%	0.004%
16	4.042	852	856	859	rBV2	243	193	0.02%	0.003%
17	4.094	870	872	874	rBV2	115	68	0.01%	0.001%
18	4.136	883	885	889	rBV	98	78	0.01%	0.001%
19	4.177	895	898	900	rBV	154	81	0.01%	0.001%
20	4.203	903	906	911	rVV2	134	121	0.02%	0.002%
21	4.267	921	926	929	rBV2	235	210	0.03%	0.003%
22	4.284	929	931	934	rBV	104	63	0.01%	0.001%
23	4.335	944	947	949	rBV2	112	65	0.01%	0.001%
24	4.402	963	968	970	rBV	210	206	0.03%	0.003%
25	4.476	989	991	993	rBV	131	78	0.01%	0.001%
26	4.486	993	994	999	rVB	324	110	0.01%	0.002%
27	4.557	1013	1016	1019	rVB2	119	77	0.01%	0.001%
28	4.615	1024	1034	1062	rBV	82044	204619	25.93%	3.256%
29	4.981	1146	1148	1150	rBV2	384	235	0.03%	0.004%
30	5.055	1156	1171	1195	rBV2	141261	314827	39.89%	5.010%
31	5.261	1233	1235	1242	rVB2	255	269	0.03%	0.004%
32	5.296	1242	1246	1249	rBV3	402	337	0.04%	0.005%
33	5.312	1249	1251	1256	rVB	184	142	0.02%	0.002%
34	5.348	1256	1262	1267	rBV2	210	282	0.04%	0.004%
35	5.386	1271	1274	1276	rBV	154	98	0.01%	0.002%
36	5.431	1286	1288	1290	rVB	151	64	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
 Data File : VU059942.D
 Acq On : 15 Jul 2024 11:40
 Operator : MD/SY
 Sample : P3231-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E08F2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	5.447	1291	1293	1295	rBV2	74	37	0.00%	0.001%
38	5.464	1295	1298	1304	rVB2	222	209	0.03%	0.003%
39	5.496	1304	1308	1310	rBV2	147	99	0.01%	0.002%
40	5.515	1310	1314	1315	rBV	385	281	0.04%	0.004%
41	5.579	1332	1334	1337	rBV	172	108	0.01%	0.002%
42	5.718	1358	1377	1406	rBV2	291142	789197	100.00%	12.559%
43	6.123	1501	1503	1507	rVB2	258	184	0.02%	0.003%
44	6.190	1520	1524	1526	rBV	163	106	0.01%	0.002%
45	6.242	1527	1540	1564	rBV	274990	534751	67.76%	8.510%
46	6.592	1647	1649	1652	rBV	259	145	0.02%	0.002%
47	6.685	1664	1678	1706	rBV	181311	357695	45.32%	5.692%
48	6.936	1751	1756	1759	rBV2	256	247	0.03%	0.004%
49	7.078	1791	1800	1803	rBV2	280	420	0.05%	0.007%
50	7.094	1803	1805	1807	rBV2	271	153	0.02%	0.002%
51	7.126	1813	1815	1818	rBV	76	49	0.01%	0.001%
52	7.200	1831	1838	1839	rBV	513	450	0.06%	0.007%
53	7.264	1857	1858	1861	rVB	185	72	0.01%	0.001%
54	7.338	1877	1881	1884	rBV2	143	133	0.02%	0.002%
55	7.512	1932	1935	1939	rBV2	224	195	0.02%	0.003%
56	7.560	1939	1950	1970	rBV	92517	166504	21.10%	2.650%
57	7.708	1989	1996	2003	rBV4	693	1106	0.14%	0.018%
58	7.762	2011	2013	2015	rVV	171	70	0.01%	0.001%
59	7.779	2015	2018	2028	rVB3	319	377	0.05%	0.006%
60	7.894	2040	2054	2076	rBV	337474	598439	75.83%	9.524%
61	8.177	2130	2142	2168	rBV	63033	112648	14.27%	1.793%
62	8.335	2188	2191	2194	rVB	383	269	0.03%	0.004%
63	8.351	2194	2196	2197	rBV	131	35	0.00%	0.001%
64	8.383	2204	2206	2209	rBV2	239	129	0.02%	0.002%
65	8.409	2213	2214	2215	rVB2	108	21	0.00%	0.000%
66	8.425	2215	2219	2221	rBV	384	315	0.04%	0.005%
67	8.553	2255	2259	2263	rBV2	409	329	0.04%	0.005%
68	8.627	2271	2282	2319	rBV	221373	425067	53.86%	6.765%
69	8.885	2359	2362	2367	rBV2	327	234	0.03%	0.004%
70	8.959	2380	2385	2387	rBV	353	353	0.04%	0.006%
71	9.190	2454	2457	2459	rBV	162	91	0.01%	0.001%
72	9.261	2476	2479	2481	rBV2	254	158	0.02%	0.003%
73	9.315	2494	2496	2500	rBV	154	90	0.01%	0.001%
74	9.412	2514	2526	2555	rBV	404335	688833	87.28%	10.962%
75	9.698	2609	2615	2621	rVB4	613	849	0.11%	0.014%
76	9.801	2643	2647	2652	rBV2	297	357	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
Data File : VU059942.D
Acq On : 15 Jul 2024 11:40
Operator : MD/SY
Sample : P3231-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08F2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M

Title : VOC Analysis

77	9.959	2693	2696	2701	rBV2	196	166	0.02%	0.003%
78	10.110	2739	2743	2751	rVB3	608	733	0.09%	0.012%
79	10.258	2786	2789	2790	rBV2	192	120	0.02%	0.002%
80	10.338	2811	2814	2816	rBV	281	180	0.02%	0.003%
81	10.544	2874	2878	2880	rBV2	154	125	0.02%	0.002%
82	10.750	2930	2942	2962	rBV	286995	467012	59.18%	7.432%
83	11.807	3260	3271	3298	rBV	371804	606391	76.84%	9.650%
84	12.077	3353	3355	3357	rBV2	338	159	0.02%	0.003%
85	12.190	3377	3390	3411	rBV	328178	550733	69.78%	8.764%
86	12.910	3611	3614	3619	rVB5	675	544	0.07%	0.009%
87	12.975	3631	3634	3638	rBV2	362	284	0.04%	0.005%
88	14.720	4174	4177	4179	rBV	624	425	0.05%	0.007%


Sum of corrected areas: 6283776

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
Data File : VU059942.D
Acq On : 15 Jul 2024 11:40
Operator : MD/SY
Sample : P3231-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08F2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

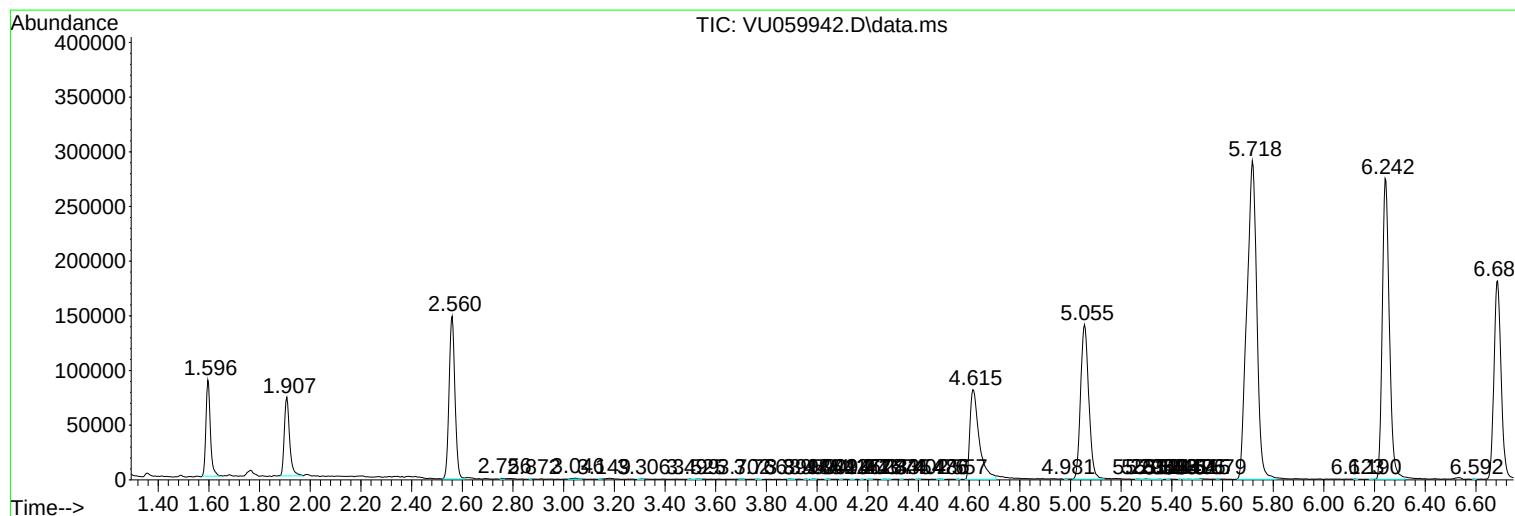

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
Data File : VU059942.D
Acq On : 15 Jul 2024 11:40
Operator : MD/SY
Sample : P3231-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08F2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
Data File : VU059942.D
Acq On : 15 Jul 2024 11:40
Operator : MD/SY
Sample : P3231-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E08F2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc