

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
 Data File : VU059955.D
 Acq On : 15 Jul 2024 16:41
 Operator : MD/SY
 Sample : P3230-06ME 10X
 Misc : 5.13g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHB37ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M

Title : VOC Analysis

Signal : TIC: VU059955.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	88	94	122	rVB	60452	78697	12.58%	1.534%
2	1.888	180	186	198	rVB	46835	64545	10.32%	1.258%
3	2.554	381	393	411	rBV	107165	175796	28.11%	3.426%
4	2.834	475	480	481	rBV2	254	200	0.03%	0.004%
5	2.943	512	514	520	rVB	378	274	0.04%	0.005%
6	3.039	533	544	558	rBV5	1572	3279	0.52%	0.064%
7	3.178	574	587	599	rBV2	2871	6471	1.03%	0.126%
8	3.261	610	613	615	rBV	176	100	0.02%	0.002%
9	3.332	630	635	637	rBV2	364	278	0.04%	0.005%
10	3.602	716	719	722	rBV2	234	162	0.03%	0.003%
11	3.711	747	753	756	rBV2	245	307	0.05%	0.006%
12	3.763	765	769	771	rBV	206	148	0.02%	0.003%
13	3.850	795	796	797	rBV	257	59	0.01%	0.001%
14	3.920	813	818	820	rBV2	104	106	0.02%	0.002%
15	4.068	861	864	869	rBV2	261	205	0.03%	0.004%
16	4.100	872	874	875	rBV	129	62	0.01%	0.001%
17	4.142	885	887	890	rVB	137	67	0.01%	0.001%
18	4.181	894	899	903	rBV	282	264	0.04%	0.005%
19	4.203	903	906	908	rBV2	142	97	0.02%	0.002%
20	4.258	919	923	930	rVB2	265	259	0.04%	0.005%
21	4.329	942	945	947	rBV	180	121	0.02%	0.002%
22	4.361	952	955	959	rVB	387	277	0.04%	0.005%
23	4.390	959	964	968	rBV2	184	195	0.03%	0.004%
24	4.441	977	980	983	rBV	173	103	0.02%	0.002%
25	4.615	1024	1034	1061	rBV	70235	176154	28.17%	3.433%
26	5.055	1154	1171	1195	rBV	108589	243353	38.91%	4.743%
27	5.165	1203	1205	1207	rBV	237	133	0.02%	0.003%
28	5.184	1207	1211	1213	rVB2	278	206	0.03%	0.004%
29	5.203	1213	1217	1219	rBV	173	101	0.02%	0.002%
30	5.242	1228	1229	1231	rVB	152	47	0.01%	0.001%
31	5.383	1271	1273	1280	rVB2	95	84	0.01%	0.002%
32	5.412	1280	1282	1283	rBV	88	41	0.01%	0.001%
33	5.579	1330	1334	1339	rBV2	174	211	0.03%	0.004%
34	5.621	1344	1347	1352	rVV	218	153	0.02%	0.003%
35	5.718	1357	1377	1404	rBV3	213940	589994	94.34%	11.499%
36	5.901	1431	1434	1436	rBV2	260	190	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
 Data File : VU059955.D
 Acq On : 15 Jul 2024 16:41
 Operator : MD/SY
 Sample : P3230-06ME 10X
 Misc : 5.13g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHB37ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

37	5.949	1445	1449	1451	rBV	310	178	0.03%	0.003%
38	6.033	1473	1475	1478	rVB2	187	97	0.02%	0.002%
39	6.052	1478	1481	1484	rVB	165	90	0.01%	0.002%
40	6.068	1484	1486	1487	rBV2	80	40	0.01%	0.001%
41	6.184	1519	1522	1525	rBV2	211	110	0.02%	0.002%
42	6.242	1526	1540	1568	rBV	252782	489109	78.20%	9.533%
43	6.502	1612	1621	1622	rBV3	367	486	0.08%	0.009%
44	6.534	1623	1631	1641	rVB8	2148	3932	0.63%	0.077%
45	6.608	1652	1654	1656	rBV	92	44	0.01%	0.001%
46	6.682	1664	1677	1700	rBV	139190	272332	43.54%	5.308%
47	6.811	1713	1717	1718	rBV	208	127	0.02%	0.002%
48	6.846	1725	1728	1731	rBV	171	101	0.02%	0.002%
49	6.882	1737	1739	1742	rBV	169	122	0.02%	0.002%
50	6.968	1760	1766	1770	rBV2	190	245	0.04%	0.005%
51	7.026	1779	1784	1787	rBV	233	245	0.04%	0.005%
52	7.062	1792	1795	1797	rBV2	231	152	0.02%	0.003%
53	7.116	1811	1812	1818	rVB2	352	187	0.03%	0.004%
54	7.145	1819	1821	1823	rBV2	94	47	0.01%	0.001%
55	7.165	1823	1827	1830	rBV2	181	156	0.02%	0.003%
56	7.206	1833	1840	1843	rBV3	651	818	0.13%	0.016%
57	7.300	1865	1869	1871	rBV2	135	115	0.02%	0.002%
58	7.319	1872	1875	1878	rVB	301	184	0.03%	0.004%
59	7.505	1929	1933	1936	rBV2	165	123	0.02%	0.002%
60	7.521	1936	1938	1940	rVV	191	105	0.02%	0.002%
61	7.560	1940	1950	1976	rVV	69656	123591	19.76%	2.409%
62	7.673	1983	1985	1989	rVB2	362	211	0.03%	0.004%
63	7.695	1989	1992	1993	rBV	200	102	0.02%	0.002%
64	7.766	2010	2014	2018	rVB2	297	261	0.04%	0.005%
65	7.785	2018	2020	2021	rBV2	213	94	0.02%	0.002%
66	7.814	2026	2029	2032	rBV2	169	96	0.02%	0.002%
67	7.830	2032	2034	2037	rBV	177	109	0.02%	0.002%
68	7.894	2041	2054	2082	rBV	242157	424842	67.93%	8.280%
69	8.113	2120	2122	2124	rBV2	169	102	0.02%	0.002%
70	8.177	2130	2142	2160	rBV2	48941	82285	13.16%	1.604%
71	8.399	2208	2211	2214	rBV	235	136	0.02%	0.003%
72	8.460	2226	2230	2233	rBV3	412	333	0.05%	0.006%
73	8.550	2245	2258	2272	rBV2	52998	87744	14.03%	1.710%
74	8.628	2272	2282	2306	rBV	190710	341685	54.63%	6.659%
75	8.972	2385	2389	2392	rBV2	328	268	0.04%	0.005%
76	9.068	2413	2419	2422	rBV2	182	197	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
 Data File : VU059955.D
 Acq On : 15 Jul 2024 16:41
 Operator : MD/SY
 Sample : P3230-06ME 10X
 Misc : 5.13g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHB37ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
 Title : VOC Analysis

77	9.103	2427	2430	2432	rBV2	233	130	0.02%	0.003%
78	9.206	2459	2462	2467	rVB	290	232	0.04%	0.005%
79	9.412	2514	2526	2548	rBV	374523	625424	100.00%	12.190%
80	9.865	2664	2667	2669	rBV	155	105	0.02%	0.002%
81	9.901	2675	2678	2681	rBV	190	140	0.02%	0.003%
82	10.090	2733	2737	2739	rBV2	353	271	0.04%	0.005%
83	10.119	2744	2746	2748	rBV2	173	103	0.02%	0.002%
84	10.753	2930	2943	2960	rBV	233488	378100	60.45%	7.369%
85	10.878	2979	2982	2985	rBV3	674	536	0.09%	0.010%
86	11.135	3061	3062	3067	rVB2	201	135	0.02%	0.003%
87	11.451	3157	3160	3163	rBV2	218	172	0.03%	0.003%
88	11.541	3185	3188	3191	rBV2	318	188	0.03%	0.004%
89	11.557	3191	3193	3196	rBV2	270	176	0.03%	0.003%
90	11.807	3259	3271	3294	rBV	326916	541024	86.51%	10.545%
91	12.190	3378	3390	3416	rBV	247400	409889	65.54%	7.989%
92	14.640	4149	4152	4153	rBV	395	243	0.04%	0.005%




Sum of corrected areas: 5130808

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
Data File : VU059955.D
Acq On : 15 Jul 2024 16:41
Operator : MD/SY
Sample : P3230-06ME 10X
Misc : 5.13g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHB37ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

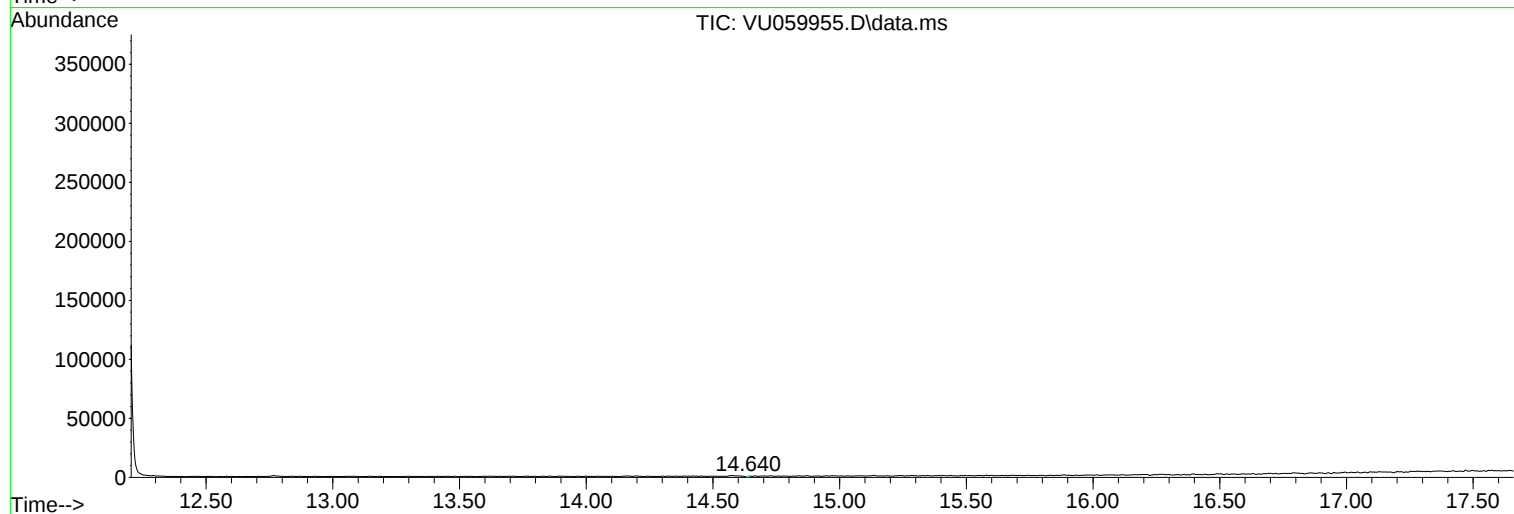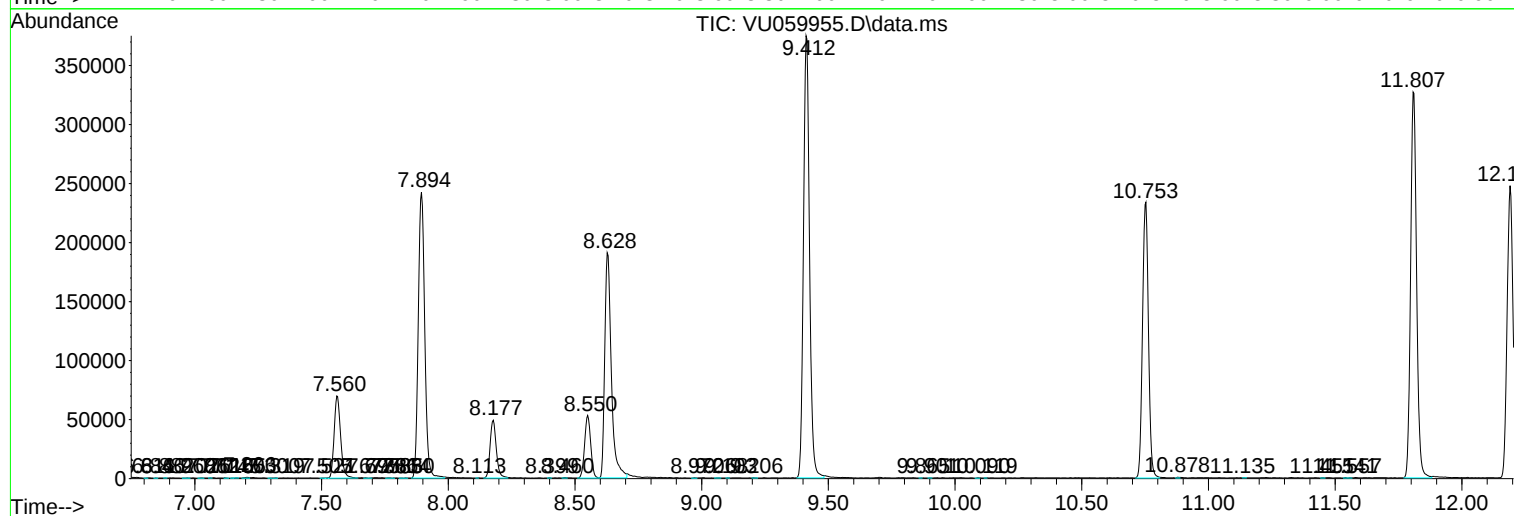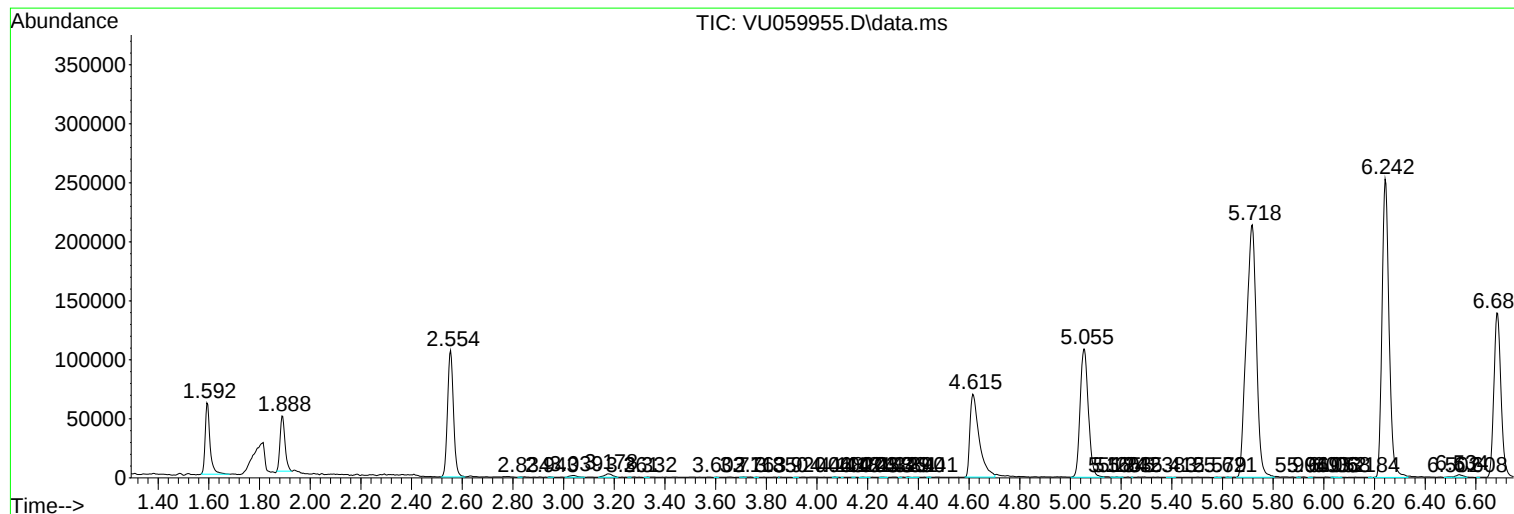

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
Data File : VU059955.D
Acq On : 15 Jul 2024 16:41
Operator : MD/SY
Sample : P3230-06ME 10X
Misc : 5.13g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHB37ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
Data File : VU059955.D
Acq On : 15 Jul 2024 16:41
Operator : MD/SY
Sample : P3230-06ME 10X
Misc : 5.13g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHB37ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc