


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071524\
Data File : VU059935.D
Acq On : 15 Jul 2024 08:15
Operator : MD/SY
Sample : BFB072
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB072

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM070224WMA.M
Title : VOC Analysis
Last Update : Tue Jul 16 05:46:09 2024

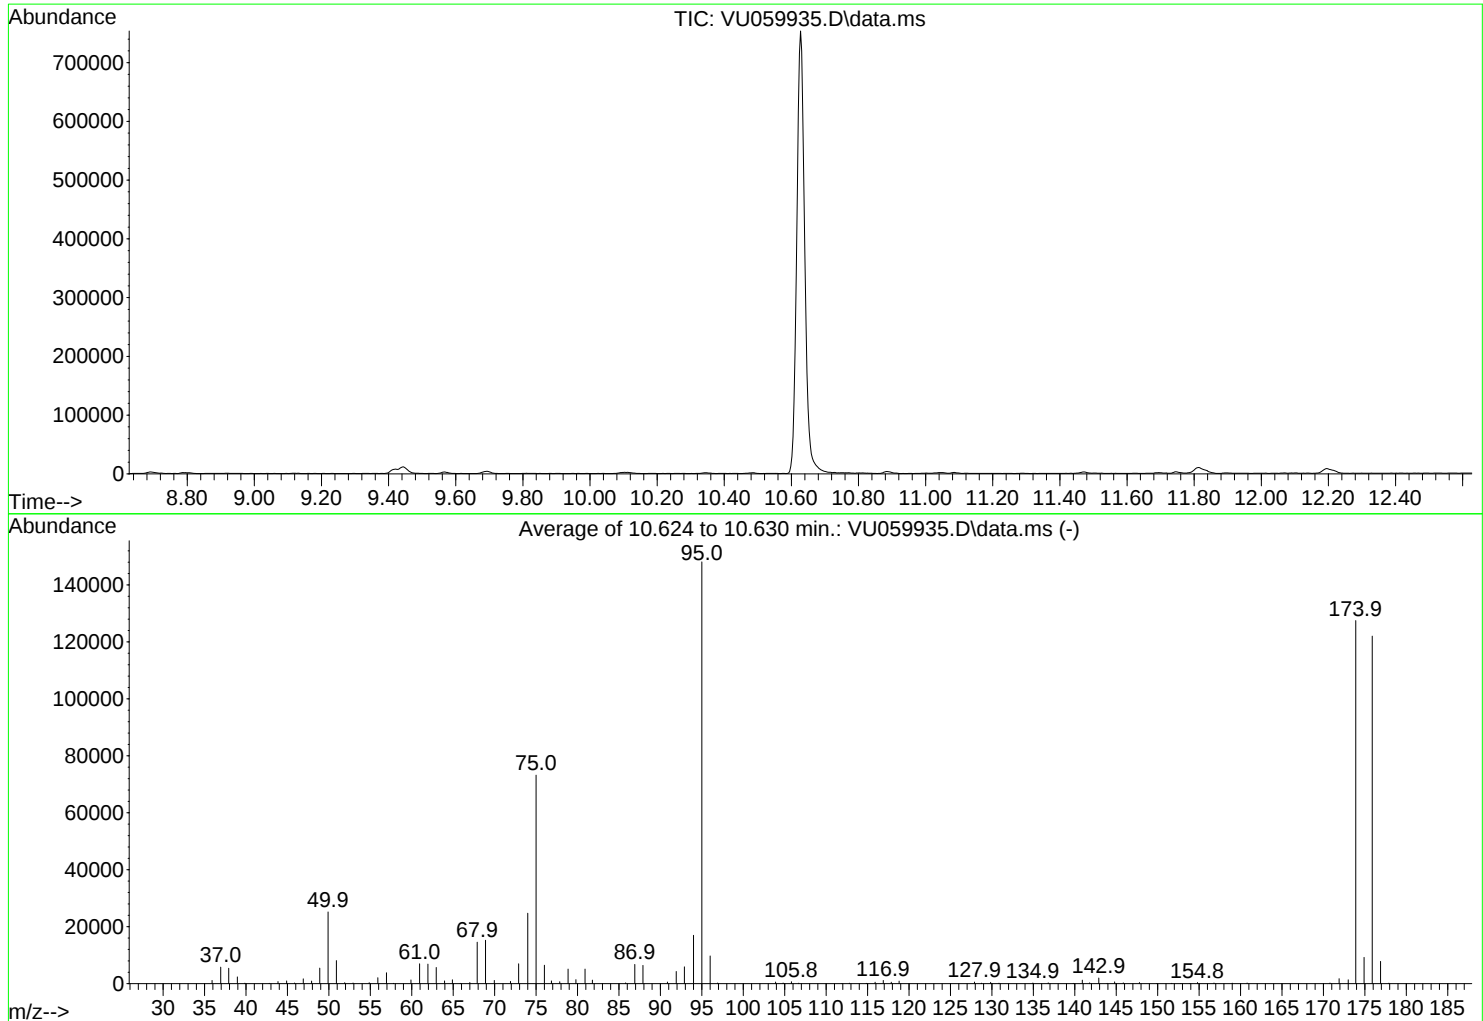

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.0	25160	PASS
75	95	30	80	49.4	73219	PASS
95	95	100	100	100.0	148117	PASS
96	95	5	9	6.6	9728	PASS
173	174	0.00	2	1.1	1352	PASS
174	95	50	120	86.1	127501	PASS
175	174	5	9	7.2	9205	PASS
176	174	95	101	95.7	122019	PASS
177	176	5	9	6.4	7828	PASS

m/z	Abundance
39.80	215.0
43.80	399.0

Instrument :
MSVOA_U
ClientSampleId :
BFB072

m/z	Abundance
35.90	1169.0
37.00	5706.0
37.90	5370.0
38.90	2410.0
39.90	424.0
42.80	118.0
43.90	1055.0
44.90	877.0
45.90	192.0
46.90	1821.0
47.90	870.0
48.90	5531.0
49.90	25128.0
50.90	8125.0
51.90	336.0
52.90	223.0
54.80	377.0
55.90	2117.0
57.00	3978.0
57.80	160.0
59.90	1332.0
60.90	6879.0
62.00	6730.0
63.00	5808.0
63.90	1031.0
64.90	1366.0
65.80	132.0
67.00	325.0
67.90	14907.0
68.90	14964.0
69.90	1157.0
71.90	834.0
72.90	7196.0
74.00	24776.0
75.00	72664.0
76.00	6666.0
76.80	901.0
77.80	714.0
78.90	5184.0
79.80	1414.0
80.90	5097.0
81.80	1330.0
83.00	125.0
85.80	231.0
86.90	6658.0
87.90	6320.0
90.90	635.0
91.90	4121.0
92.90	5868.0
94.00	16488.0
95.00	145280.0
96.00	9680.0
96.90	255.0
103.90	532.0
104.80	187.0
105.80	625.0
106.70	182.0
112.80	138.0
114.80	115.0
115.90	498.0
116.90	1096.0
117.90	489.0
118.80	842.0
127.90	568.0
128.80	187.0
129.80	541.0
130.80	145.0
134.90	220.0
136.80	280.0
140.90	1102.0
141.80	314.0
142.90	1990.0
143.90	176.0
144.80	602.0
145.80	257.0
147.80	353.0
154.80	393.0
156.80	215.0
159.00	140.0
160.80	241.0
170.80	237.0
171.90	1793.0
173.00	1339.0
173.90	122304.0
174.90	9164.0
175.90	117176.0
176.90	7672.0
177.90	231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB072

m/z	Abundance
35.90	1132.0
36.90	6009.0
37.90	5582.0
39.00	2459.0
39.90	380.0
42.80	127.0
43.90	1167.0
44.90	1006.0
45.80	240.0
46.90	1753.0
47.90	899.0
48.90	5624.0
49.90	25928.0
50.90	8395.0
51.90	383.0
52.90	218.0
54.80	357.0
55.90	2130.0
57.00	3936.0
57.80	138.0
59.90	1354.0
60.90	7253.0
62.00	7107.0
63.00	5927.0
63.90	996.0
64.90	1387.0
65.90	149.0
67.00	378.0
67.90	14893.0
68.90	15802.0
69.90	1162.0
71.90	808.0
72.90	7237.0
74.00	25512.0
75.00	75616.0
76.00	6674.0
76.90	1001.0
77.80	690.0
78.90	5250.0
79.80	1464.0
80.90	5326.0
81.80	1304.0
85.80	279.0
86.90	6942.0
87.90	6673.0
90.90	601.0
91.90	4386.0
92.90	6076.0
94.00	17520.0
95.00	153088.0
96.00	9965.0
96.90	252.0
103.90	566.0
104.80	202.0
105.80	723.0
106.70	146.0
111.90	114.0
112.80	164.0
114.80	144.0
115.90	524.0
116.90	1153.0
117.80	504.0
118.80	929.0
127.90	612.0
128.70	154.0
129.80	485.0
130.90	177.0
134.90	207.0
136.80	301.0
139.80	122.0
140.90	1278.0
141.80	291.0
142.90	2023.0
143.90	130.0
144.80	610.0
145.90	265.0
147.80	407.0
149.90	117.0
151.70	124.0
153.90	111.0
154.80	442.0
156.80	270.0
159.00	167.0
160.80	226.0
170.80	259.0
171.90	1795.0
173.00	1427.0
173.90	131712.0
174.90	9509.0
175.90	126184.0
176.90	8051.0
178.00	179.0

Instrument :
MSVOA_U
ClientSampleId :
BFB072

m/z	Abundance
35.90	1036.0
36.90	5732.0
37.90	5215.0
38.90	2179.0
39.90	333.0
42.80	100.0
43.90	1157.0
44.90	1064.0
45.80	237.0
46.90	1562.0
47.90	882.0
48.90	5120.0
49.90	24424.0
50.90	7859.0
51.90	353.0
52.90	219.0
54.90	332.0
55.90	1972.0
56.90	3616.0
57.80	130.0
59.90	1296.0
61.00	6831.0
61.90	6758.0
62.90	5382.0
64.00	826.0
64.90	1247.0
65.90	128.0
67.00	439.0
67.90	13867.0
68.90	14957.0
70.00	1032.0
71.90	737.0
72.90	6464.0
74.00	23904.0
75.00	71376.0
76.00	6074.0
76.90	1007.0
77.90	668.0
78.80	4839.0
79.80	1376.0
80.90	4995.0
81.80	1180.0
85.80	299.0
86.90	6663.0
87.90	6237.0
90.80	528.0
91.90	4251.0
92.90	5810.0
94.00	16976.0
95.00	145984.0
96.00	9539.0
96.90	218.0
103.90	615.0
104.80	230.0
105.80	695.0
106.70	110.0
111.90	140.0
112.80	138.0
114.90	140.0
115.90	493.0
116.90	1089.0
117.80	524.0
118.80	941.0
127.90	582.0
128.80	145.0
129.90	407.0
130.90	170.0
135.00	183.0
136.80	263.0
139.80	147.0
140.90	1273.0
141.80	222.0
142.90	1879.0
144.80	566.0
145.90	289.0
147.80	387.0
149.90	145.0
151.70	182.0
152.80	102.0
153.90	115.0
154.80	432.0
156.80	280.0
159.00	204.0
160.80	154.0
170.80	223.0
171.90	1659.0
173.00	1289.0
173.90	128488.0
174.90	8942.0
175.90	122696.0
176.90	7760.0
177.80	143.0

Instrument :
MSVOA_U
ClientSampleId :
BFB072