

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071618\
 Data File : VU025443.D
 Acq On : 16 Jul 2018 22:59
 Operator : MD/SY
 Sample : J3984-09DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB183DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071618WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.773	54	57	61	rVB4	511	475	0.03%	0.004%
2	0.870	85	87	91	rVB5	698	414	0.02%	0.004%
3	1.031	133	137	140	rBV2	838	686	0.04%	0.006%
4	1.085	140	154	177	rBV	1436119	1775313	100.00%	15.679%
5	1.400	245	252	264	rVB	124604	134701	7.59%	1.190%
6	1.677	331	338	358	rVB	90532	130331	7.34%	1.151%
7	2.272	513	523	535	rVB	215169	328575	18.51%	2.902%
8	2.564	612	614	620	rVB3	926	613	0.03%	0.005%
9	2.696	649	655	667	rVB7	2363	4182	0.24%	0.037%
10	2.844	688	701	713	rBV2	7266	16077	0.91%	0.142%
11	3.101	778	781	786	rBV3	646	441	0.02%	0.004%
12	3.130	786	790	797	rBV7	1054	1211	0.07%	0.011%
13	3.191	805	809	810	rBV2	629	452	0.03%	0.004%
14	3.346	854	857	858	rBV2	835	441	0.02%	0.004%
15	3.432	880	884	885	rBV2	991	619	0.03%	0.005%
16	3.561	921	924	927	rVB3	673	477	0.03%	0.004%
17	3.725	972	975	977	rBV3	567	437	0.02%	0.004%
18	3.812	999	1002	1008	rVB6	935	863	0.05%	0.008%
19	3.924	1030	1037	1041	rVV6	1037	1171	0.07%	0.010%
20	4.178	1100	1116	1127	rBV	109622	299937	16.89%	2.649%
21	4.583	1239	1242	1245	rVV3	1082	738	0.04%	0.007%
22	4.651	1245	1263	1286	rVV2	192833	450896	25.40%	3.982%
23	4.735	1286	1289	1294	rVV4	798	581	0.03%	0.005%
24	4.982	1364	1366	1369	rBV3	554	433	0.02%	0.004%
25	5.053	1383	1388	1390	rBV5	844	881	0.05%	0.008%
26	5.082	1394	1397	1401	rVB2	597	469	0.03%	0.004%
27	5.188	1427	1430	1434	rVB4	604	462	0.03%	0.004%
28	5.207	1434	1436	1442	rBV5	638	647	0.04%	0.006%
29	5.233	1442	1444	1448	rVB5	701	422	0.02%	0.004%
30	5.342	1454	1478	1497	rBV2	366551	1116016	62.86%	9.856%
31	5.734	1597	1600	1603	rBV4	595	516	0.03%	0.005%
32	5.818	1623	1626	1629	rBV4	537	509	0.03%	0.004%
33	5.889	1633	1648	1669	rBV	401273	781064	44.00%	6.898%
34	6.111	1714	1717	1720	rBV5	976	614	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U071618\
 Data File : VU025443.D
 Acq On : 16 Jul 2018 22:59
 Operator : MD/SY
 Sample : J3984-09DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB183DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071618WMA.M
 Title : VOC Analysis

35	6.188	1728	1741	1758	rBV	78550	149821	8.44%	1.323%
36	6.333	1772	1786	1809	rBV	252990	510896	28.78%	4.512%
37	6.615	1870	1874	1876	rBV4	703	680	0.04%	0.006%
38	6.683	1892	1895	1899	rBV3	685	614	0.03%	0.005%
39	6.722	1905	1907	1912	rVB4	702	458	0.03%	0.004%
40	6.834	1938	1942	1943	rBV3	778	582	0.03%	0.005%
41	6.915	1965	1967	1970	rBV3	892	550	0.03%	0.005%
42	6.995	1990	1992	1998	rVB5	607	492	0.03%	0.004%
43	7.059	2008	2012	2015	rBV4	712	714	0.04%	0.006%
44	7.082	2015	2019	2021	rVB3	745	645	0.04%	0.006%
45	7.117	2026	2030	2036	rBV5	529	495	0.03%	0.004%
46	7.230	2053	2065	2081	rBV	137830	243307	13.71%	2.149%
47	7.468	2133	2139	2145	rBV9	1407	1732	0.10%	0.015%
48	7.567	2157	2170	2206	rVV	505831	902987	50.86%	7.975%
49	7.850	2247	2258	2274	rBV2	93517	160786	9.06%	1.420%
50	8.140	2345	2348	2351	rBV4	633	483	0.03%	0.004%
51	8.175	2354	2359	2363	rBV4	808	987	0.06%	0.009%
52	8.230	2363	2376	2389	rBV	318891	542387	30.55%	4.790%
53	8.313	2391	2402	2427	rVB	352434	614438	34.61%	5.426%
54	8.561	2477	2479	2482	rBV3	659	430	0.02%	0.004%
55	8.686	2514	2518	2520	rBV2	844	576	0.03%	0.005%
56	8.702	2520	2523	2526	rVV3	911	615	0.03%	0.005%
57	8.734	2529	2533	2536	rBV6	493	458	0.03%	0.004%
58	8.773	2541	2545	2549	rBV5	1025	1005	0.06%	0.009%
59	8.892	2577	2582	2586	rBV5	638	578	0.03%	0.005%
60	9.091	2631	2644	2682	rVV	533229	911787	51.36%	8.052%
61	9.284	2701	2704	2707	rBV3	510	419	0.02%	0.004%
62	9.329	2714	2718	2721	rBV4	585	433	0.02%	0.004%
63	9.381	2729	2734	2739	rVB4	1080	1248	0.07%	0.011%
64	9.554	2785	2788	2792	rVB4	625	570	0.03%	0.005%
65	9.577	2792	2795	2796	rBV3	857	546	0.03%	0.005%
66	9.612	2802	2806	2812	rBV5	964	1198	0.07%	0.011%
67	9.702	2831	2834	2838	rBV2	814	615	0.03%	0.005%
68	9.799	2859	2864	2866	rBV4	1011	869	0.05%	0.008%
69	9.824	2870	2872	2874	rBV2	807	524	0.03%	0.005%
70	9.914	2896	2900	2901	rBV2	634	482	0.03%	0.004%
71	10.072	2943	2949	2954	rBV6	1231	1364	0.08%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071618\
 Data File : VU025443.D
 Acq On : 16 Jul 2018 22:59
 Operator : MD/SY
 Sample : J3984-09DL 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB183DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071618WMA.M
 Title : VOC Analysis

72	10.101	2954	2958	2963	rVV4	600	735	0.04%	0.006%
73	10.130	2963	2967	2969	rVV3	757	672	0.04%	0.006%
74	10.201	2982	2989	2991	rBV5	714	659	0.04%	0.006%
75	10.435	3048	3062	3078	rBV	369985	589924	33.23%	5.210%
76	10.519	3085	3088	3093	rVB3	879	884	0.05%	0.008%
77	10.548	3093	3097	3098	rBV	964	673	0.04%	0.006%
78	10.586	3106	3109	3112	rBV2	702	542	0.03%	0.005%
79	10.625	3118	3121	3123	rBV3	1009	664	0.04%	0.006%
80	10.680	3134	3138	3140	rBV3	510	428	0.02%	0.004%
81	10.721	3148	3151	3155	rBV3	935	640	0.04%	0.006%
82	10.741	3155	3157	3161	rVB4	769	544	0.03%	0.005%
83	10.770	3161	3166	3168	rBV3	480	450	0.03%	0.004%
84	10.786	3168	3171	3174	rBV4	1033	762	0.04%	0.007%
85	10.821	3178	3182	3187	rVB5	1031	857	0.05%	0.008%
86	10.847	3188	3190	3193	rBV3	496	412	0.02%	0.004%
87	10.934	3212	3217	3221	rBV4	945	971	0.05%	0.009%
88	11.139	3277	3281	3285	rBV3	541	566	0.03%	0.005%
89	11.255	3310	3317	3321	rBV2	925	1037	0.06%	0.009%
90	11.332	3338	3341	3346	rBV4	538	504	0.03%	0.004%
91	11.355	3346	3348	3354	rVB2	708	439	0.02%	0.004%
92	11.487	3377	3389	3407	rVV	502242	791141	44.56%	6.987%
93	11.863	3494	3506	3528	rBV	496697	802332	45.19%	7.086%
94	12.207	3607	3613	3620	rVB3	845	1128	0.06%	0.010%
95	12.406	3670	3675	3678	rBV4	749	658	0.04%	0.006%
96	12.570	3715	3726	3736	rBV4	9325	14510	0.82%	0.128%
97	13.046	3872	3874	3879	rVB2	1162	841	0.05%	0.007%
98	13.326	3958	3961	3962	rBV	795	480	0.03%	0.004%
99	13.673	4065	4069	4071	rBV3	858	696	0.04%	0.006%
100	14.007	4170	4173	4176	rBV3	732	606	0.03%	0.005%


Sum of corrected areas: 11323190

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU071618\
Data File : VU025443.D
Acq On : 16 Jul 2018 22:59
Operator : MD/SY
Sample : J3984-09DL 40X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB183DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071618WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

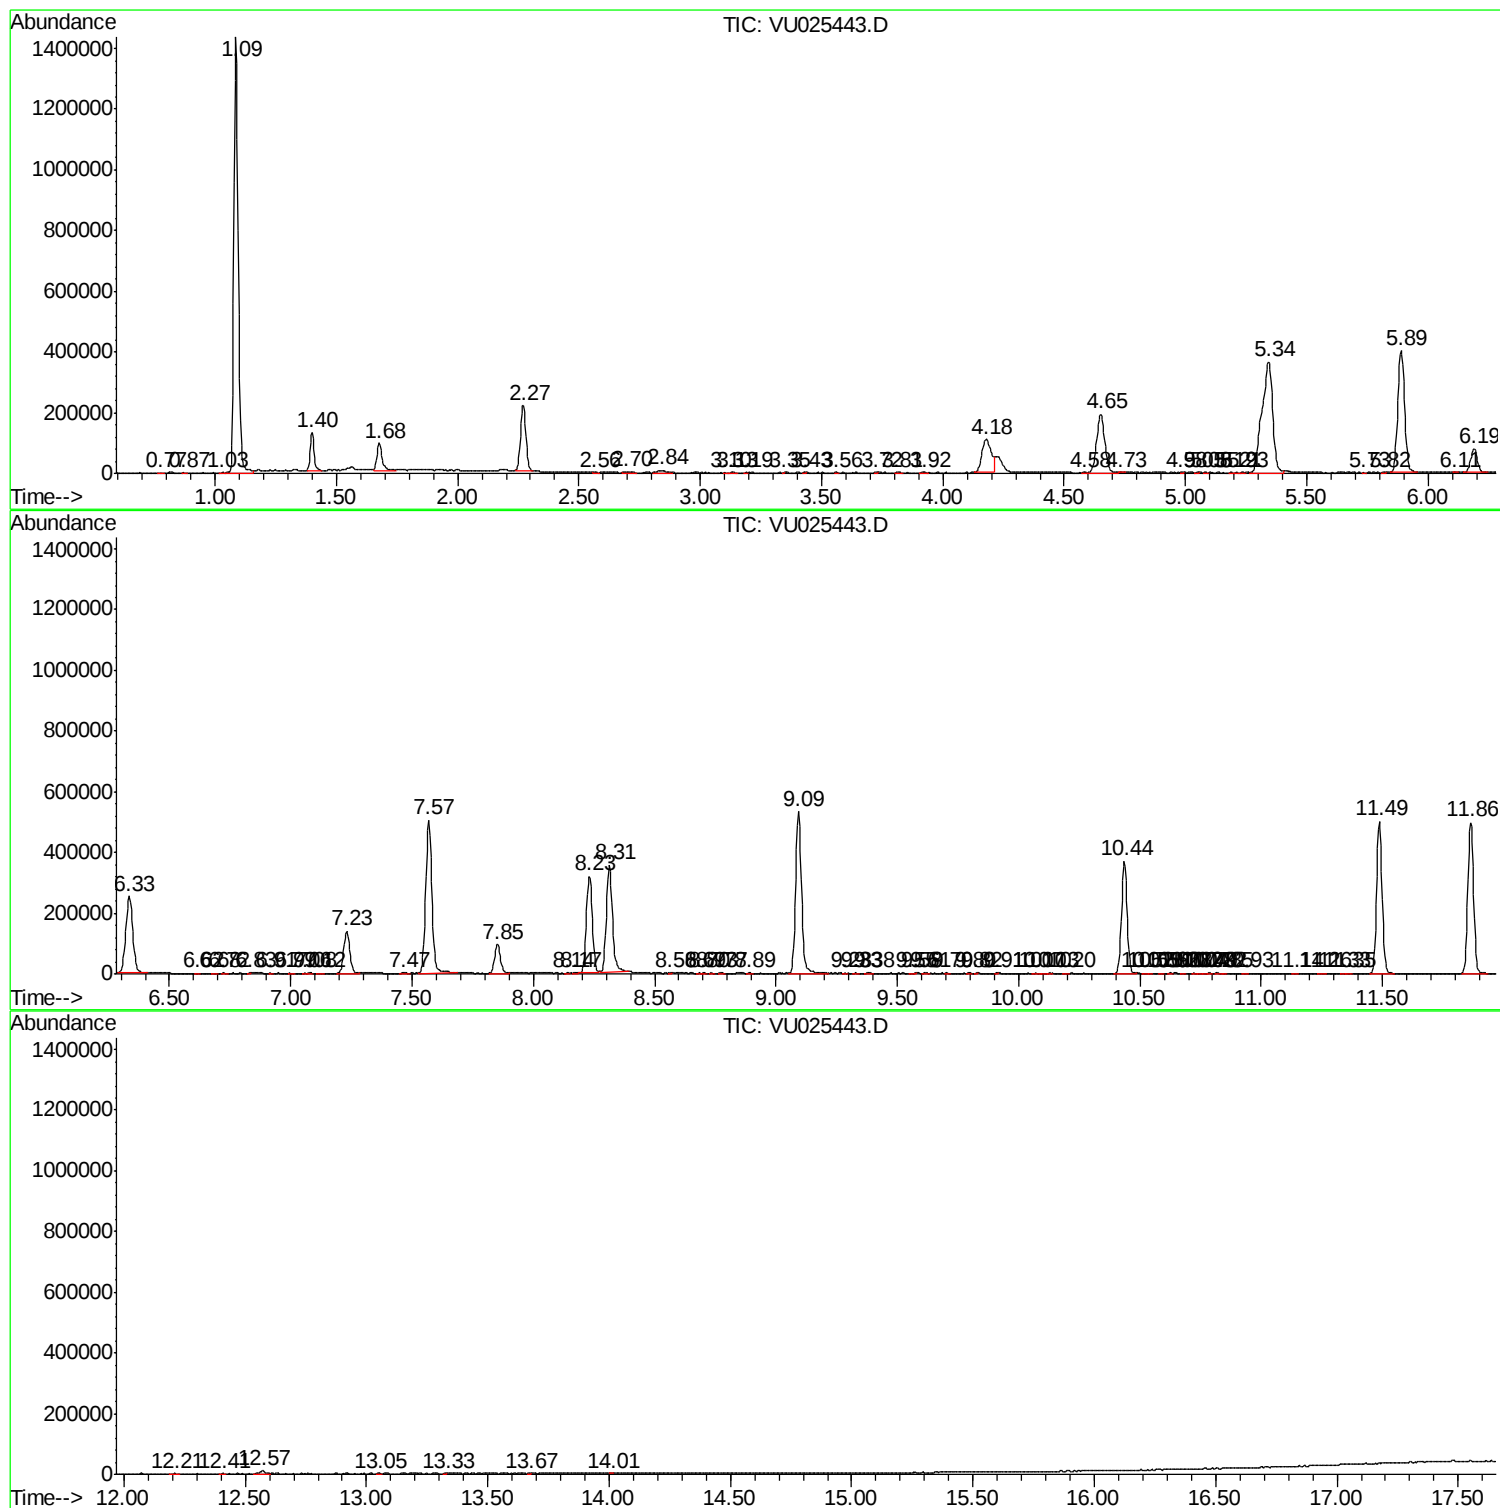

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071618\
Data File : VU025443.D
Acq On : 16 Jul 2018 22:59
Operator : MD/SY
Sample : J3984-09DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB183DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071618WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071618\
Data File : VU025443.D
Acq On : 16 Jul 2018 22:59
Operator : MD/SY
Sample : J3984-09DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB183DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071618WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc