


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071618\
 Data File : VU025413.D
 Acq On : 16 Jul 2018 09:27
 Operator : MD/SY
 Sample : BFB43
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB43

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM071618WMA.M
 Title : VOC Analysis
 Last Update : Tue Jul 17 02:54:19 2018

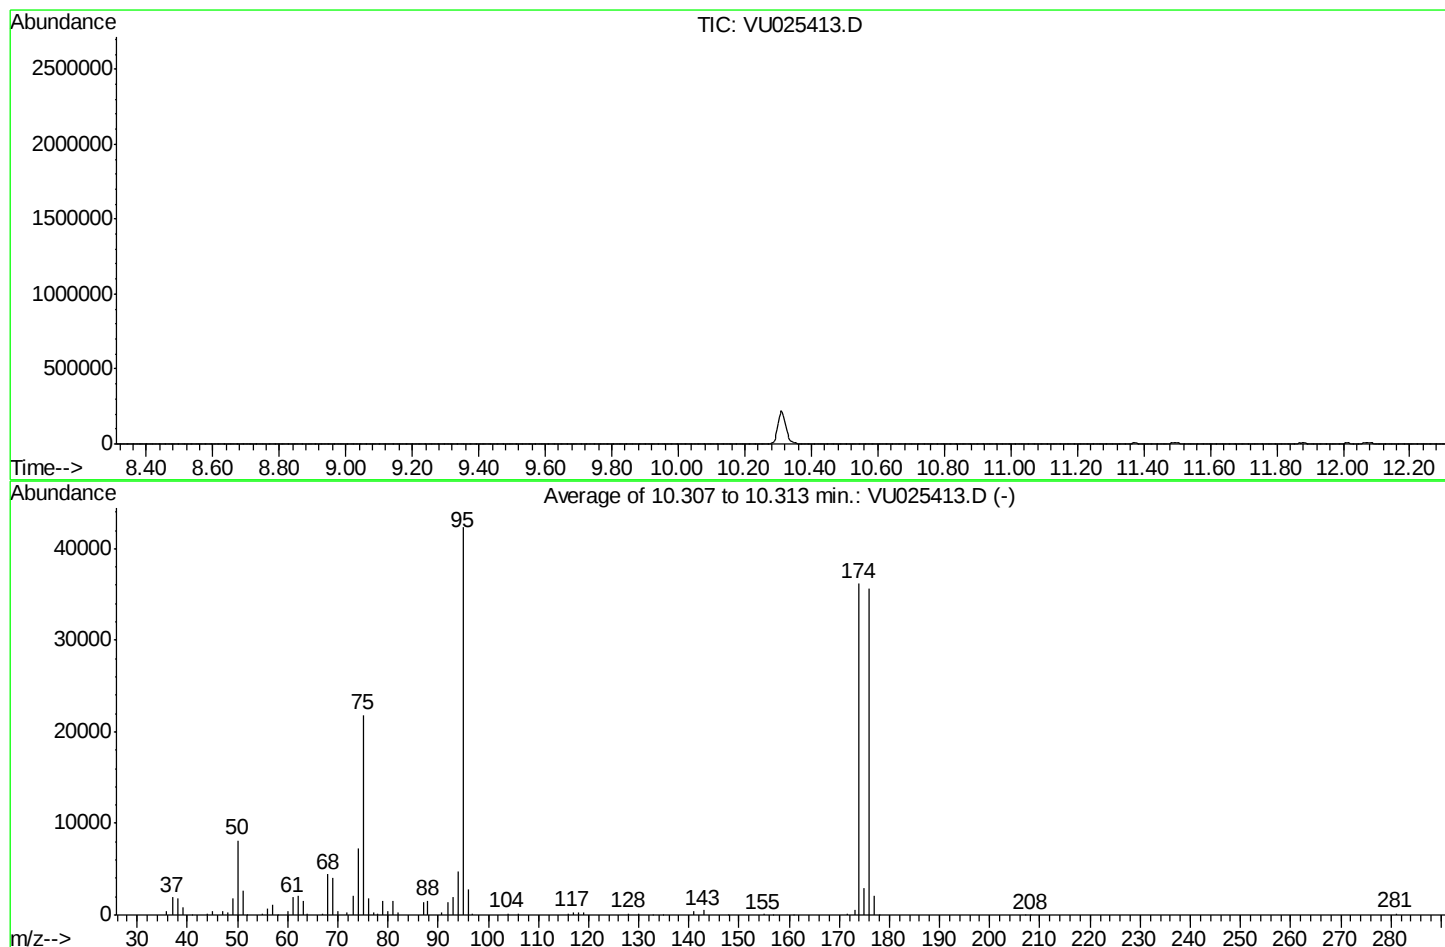

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	8166	PASS
75	95	30	80	51.6	21861	PASS
95	95	100	100	100.0	42330	PASS
96	95	5	9	6.6	2807	PASS
173	174	0.00	2	1.5	544	PASS
174	95	50	120	85.5	36194	PASS
175	174	5	9	8.0	2881	PASS
176	174	95	101	98.5	35664	PASS
177	176	5	9	6.0	2123	PASS

Scan 3010 (10.268 min): VU025413.D
BFB43

m/z	Abundance
39.90	165.0
40.90	101.0
43.90	469.0
95.80	171.0
190.80	110.0
207.00	1003.0
208.00	241.0
209.00	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
35.90	516.0
37.00	2001.0
38.00	1784.0
39.00	874.0
39.80	142.0
41.00	129.0
44.00	556.0
44.90	430.0
47.10	471.0
48.00	306.0
49.00	1801.0
50.00	8071.0
51.00	2576.0
52.10	107.0
55.00	178.0
56.00	626.0
57.00	1108.0
60.00	390.0
61.00	2017.0
62.00	2094.0
63.00	1520.0
63.90	150.0
66.90	154.0
68.00	4531.0
69.00	3949.0
70.10	393.0
71.90	254.0
73.00	2033.0
74.00	7075.0
75.00	21744.0
76.00	1908.0
77.10	291.0
77.90	153.0
78.90	1417.0
79.90	398.0
80.90	1457.0
81.90	253.0
87.00	1375.0
87.90	1642.0
90.80	238.0
92.00	1338.0
93.00	2026.0
94.00	4741.0
95.00	41320.0
96.00	2879.0
96.80	161.0
103.90	249.0
106.00	201.0
115.80	112.0
116.90	261.0
117.90	260.0
118.90	250.0
128.00	223.0
129.90	165.0
134.80	107.0
140.90	470.0
142.90	560.0
147.90	116.0
154.90	135.0
171.70	159.0
173.10	536.0
174.00	34304.0
174.90	2868.0
176.00	34584.0
177.00	2154.0
207.00	1091.0
207.90	203.0
209.00	140.0
281.10	135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
35.90	485.0
37.00	2024.0
38.00	1792.0
39.00	907.0
39.80	131.0
41.00	119.0
44.00	573.0
45.00	476.0
47.00	436.0
48.00	355.0
49.00	1884.0
50.00	8452.0
51.10	2701.0
51.90	109.0
54.90	155.0
56.00	669.0
57.00	1109.0
58.10	106.0
60.00	366.0
61.00	1999.0
62.00	2103.0
63.00	1669.0
63.90	133.0
66.90	141.0
68.00	4572.0
69.00	4196.0
70.10	396.0
71.90	272.0
73.00	2171.0
74.00	7608.0
75.00	22608.0
76.00	1927.0
77.10	369.0
77.90	196.0
78.90	1566.0
79.90	432.0
80.90	1551.0
81.90	271.0
87.00	1423.0
88.00	1592.0
90.80	283.0
92.00	1429.0
93.00	2015.0
94.00	4789.0
95.00	43656.0
96.00	2853.0
96.90	126.0
103.90	216.0
105.90	200.0
115.80	123.0
117.00	287.0
117.90	310.0
118.90	276.0
128.00	204.0
129.90	178.0
140.90	509.0
142.90	545.0
154.90	133.0
156.90	106.0
171.70	113.0
173.10	574.0
174.00	37456.0
174.90	3018.0
176.00	36616.0
177.00	2159.0
177.90	102.0
207.00	1055.0
207.90	194.0
209.00	109.0
281.00	162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
35.90	431.0
37.00	1835.0
38.00	1727.0
39.00	814.0
39.70	123.0
41.10	102.0
44.10	566.0
45.00	434.0
47.00	345.0
48.00	319.0
49.00	1808.0
50.00	7976.0
51.10	2638.0
54.90	101.0
56.00	679.0
57.00	1084.0
58.10	105.0
60.00	332.0
61.00	1803.0
62.00	1985.0
63.00	1629.0
64.00	112.0
67.00	134.0
68.00	4136.0
69.00	4155.0
70.00	331.0
71.90	293.0
73.00	2091.0
74.00	7284.0
75.00	21232.0
76.00	1723.0
77.10	382.0
77.90	207.0
78.90	1521.0
79.90	450.0
80.90	1496.0
81.90	256.0
87.00	1452.0
88.00	1431.0
90.80	272.0
92.00	1392.0
93.00	1822.0
94.00	4682.0
95.00	42016.0
96.10	2689.0
103.90	146.0
105.90	150.0
115.90	132.0
117.00	294.0
117.90	263.0
118.90	286.0
128.00	140.0
129.90	171.0
132.90	114.0
140.90	463.0
142.90	528.0
154.90	112.0
156.90	106.0
160.90	101.0
173.10	524.0
174.00	36824.0
174.90	2759.0
176.00	35792.0
177.00	2057.0
177.90	105.0
207.00	968.0
208.10	160.0
281.00	172.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43