

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071619\
 Data File : VU033268.D
 Acq On : 16 Jul 2019 17:25
 Operator : JC/SP
 Sample : K3772-05
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A52M8

Quant Time: Jul 17 05:44:11 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR071619WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jul 17 04:42:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	130091	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	134351	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.47	152	58569	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	54562	4.16	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.20%
7) Chloroethane-d5	1.67	69	48093	4.40	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.00%
11) 1,1-Dichloroethene-d2	2.26	63	88064	3.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.60%
20) 2-Butanone-d5	4.17	46	126759	51.34	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.68%
24) Chloroform-d	4.62	84	90142	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.20%
26) 1,2-Dichloroethane-d4	5.29	65	51243	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.00%
32) Benzene-d6	5.32	84	175688	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
36) 1,2-Dichloropropane-d6	6.31	67	58697	4.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.60%
41) Toluene-d8	7.55	98	154406	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.20%
43) trans-1,3-Dichloropropene-	7.83	79	23026	4.83	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.60%
46) 2-Hexanone-d5	8.30	63	102046	52.07	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.14%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	49717	5.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.60%
64) 1,2-Dichlorobenzene-d4	11.85	152	59749	5.24	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.80%

Target Compounds


					Ovalue
5) Vinyl chloride	1.39	62	10080	0.720 ug/L	86
8) Chloroethane	1.69	64	2423	0.270 ug/L	97
13) Acetone	2.31	43	3007	1.391 ug/L	88
22) cis-1,2-Dichloroethene	4.20	96	163742	16.411 ug/L	95
34) Trichloroethene	6.16	95	29900	2.970 ug/L	98
42) Toluene	7.62	91	6984	0.171 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071619\
Data File : VU033268.D
Acq On : 16 Jul 2019 17:25
Operator : JC/SP
Sample : K3772-05
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A52M8

Quant Time: Jul 17 05:44:11 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR071619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jul 17 04:42:24 2019
Response via : Initial Calibration

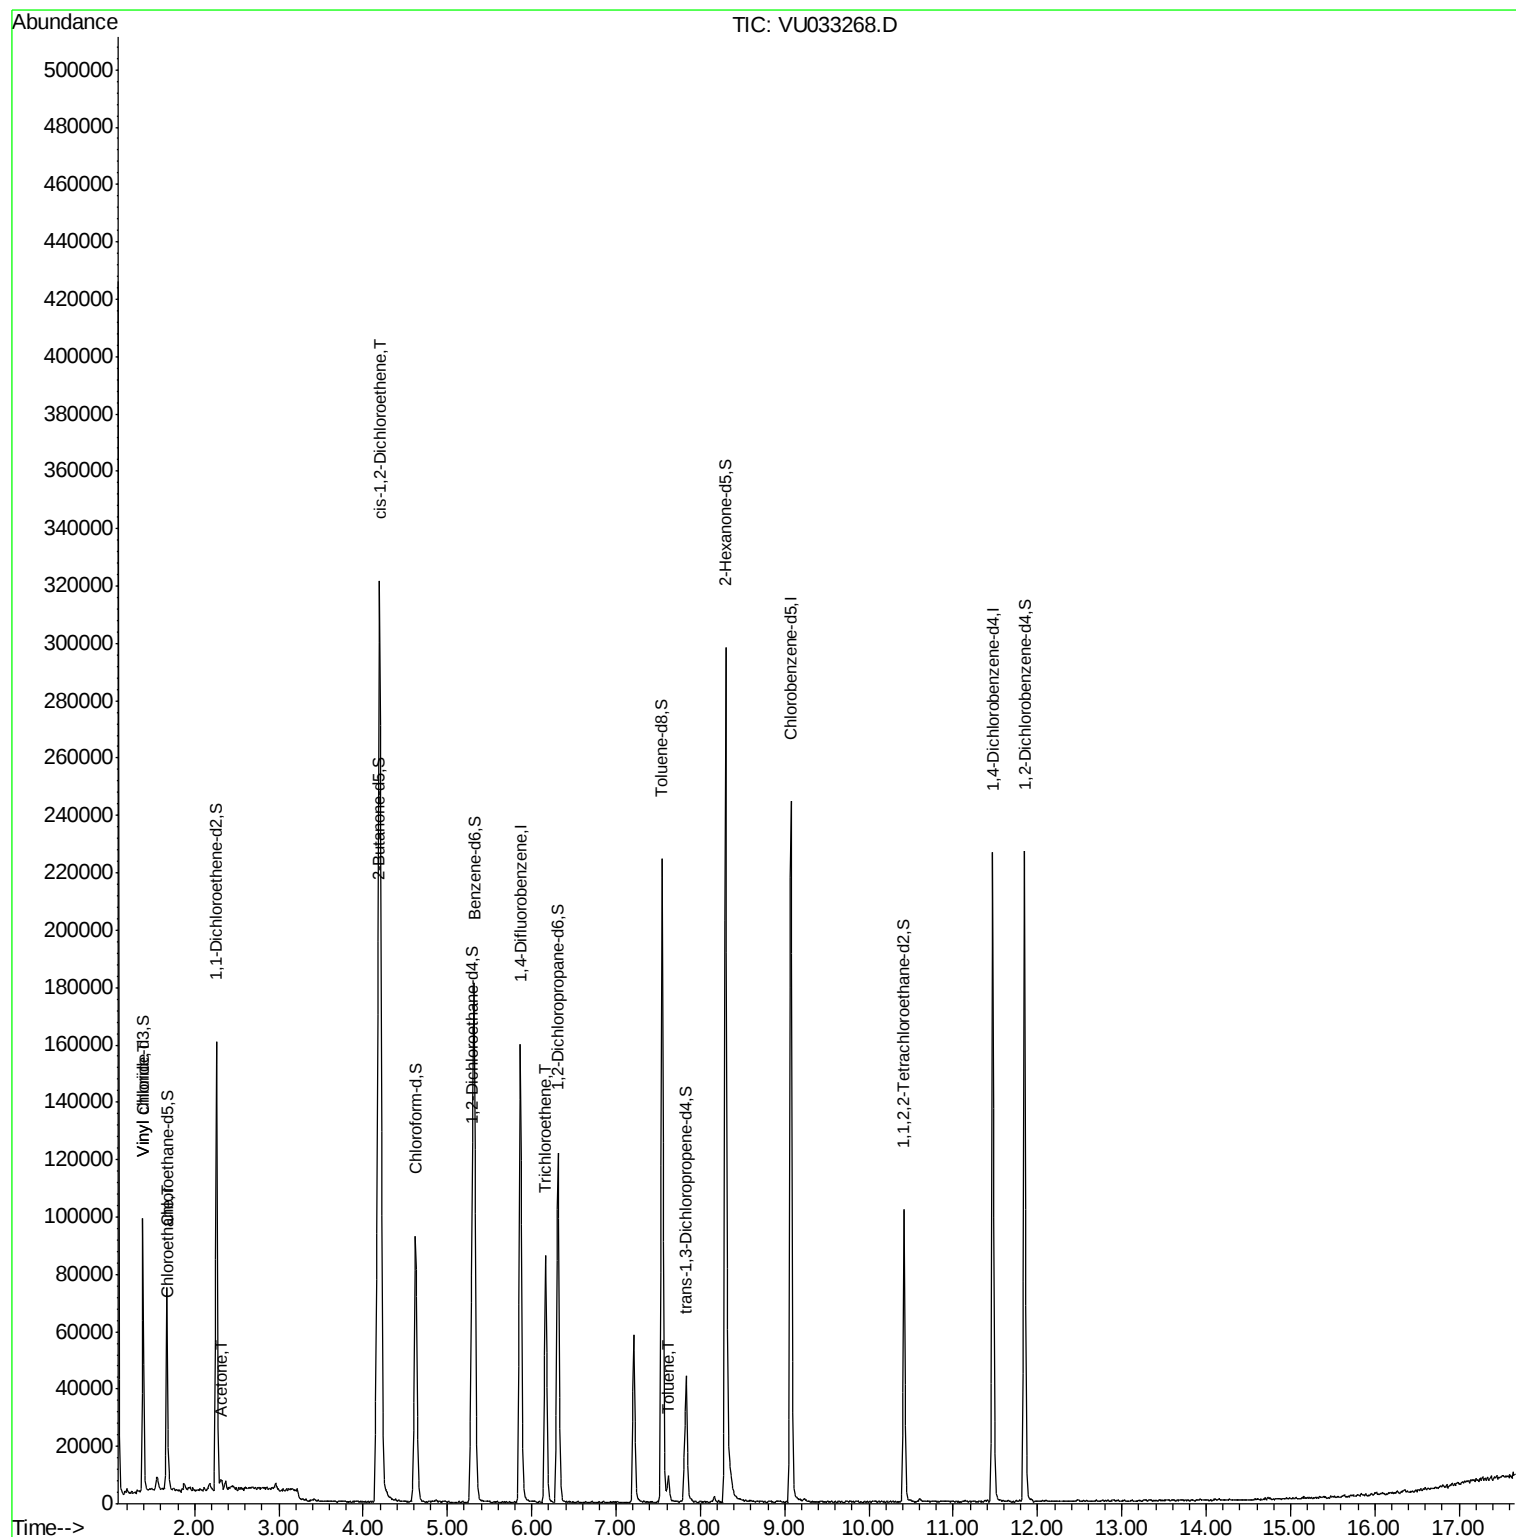

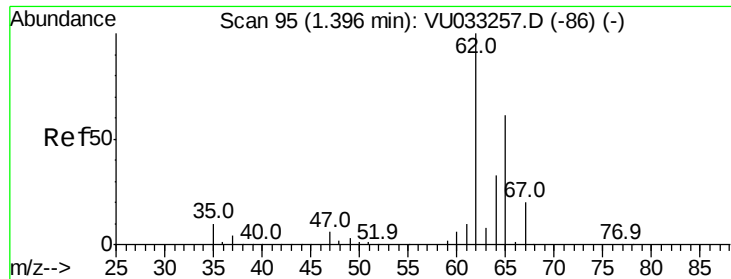

#5

Vinyl chloride

Concen: 0.720 ug/L

RT: 1.39 min Scan# 94

Delta R.T. -0.00 min

Lab File: VU033268.D

Acq: 16 Jul 2019 17:25

Instrument :

MSVOA_U

ClientSampleId :


A52M8

Tot Ion: 62 Resp: 10080

Ion Ratio Lower Upper




62 100

64 40.3 22.8 42.4

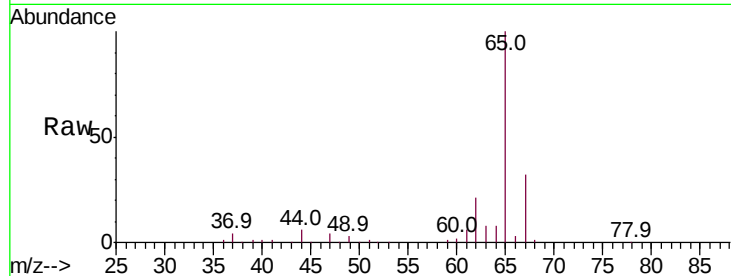

Abundance Ion 62.00 (61.70 to 62.70): VU033257.D (-86) (-)

Ion 64.10 (63.80 to 64.80): VU033268.D (-94) (-)

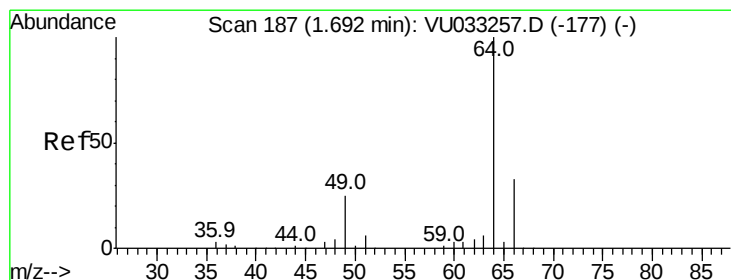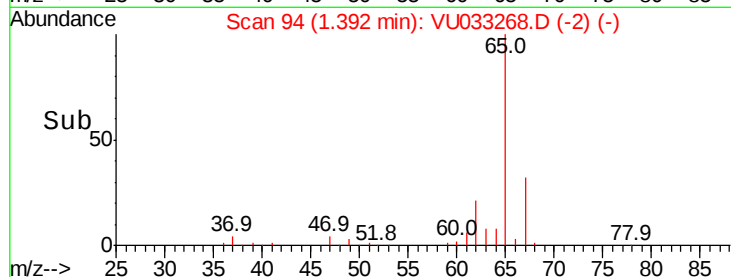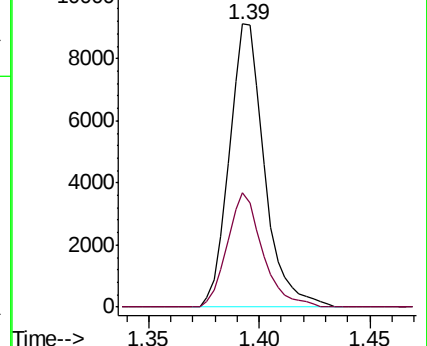

#8

Chloroethane

Concen: 0.270 ug/L

RT: 1.69 min Scan# 186

Delta R.T. -0.00 min

Lab File: VU033268.D


Acq: 16 Jul 2019 17:25

Tgt Ion: 64 Resp: 2423

Ion Ratio Lower Upper



64 100


66 35.0 23.2 43.2

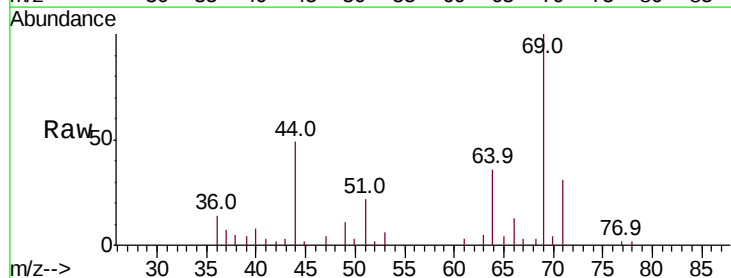

Abundance Ion 64.10 (63.80 to 64.80): VU033257.D (-177) (-)

Ion 66.05 (65.75 to 66.75): VU033268.D (-94) (-)

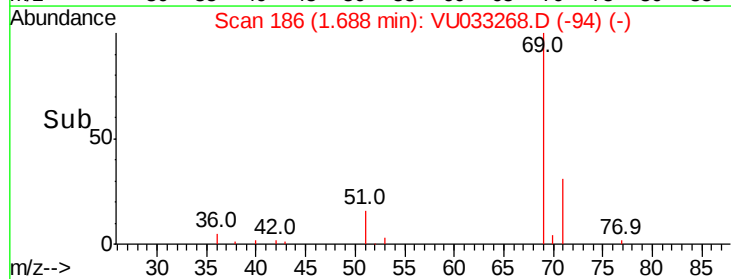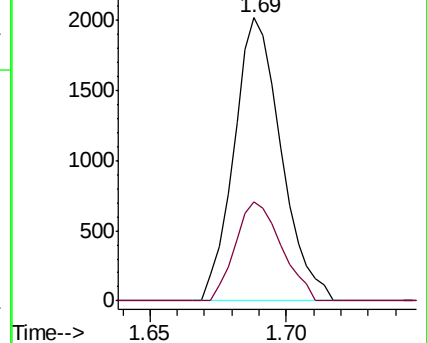

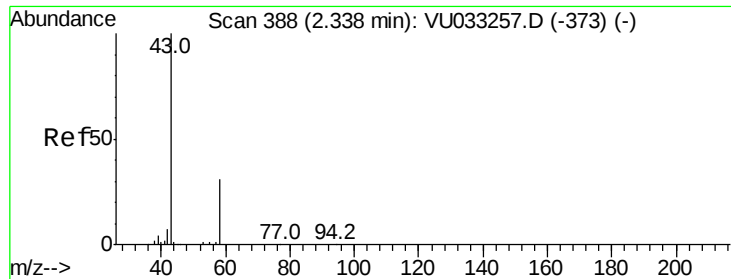

#13

Acetone

Concen: 1.391 ug/L

RT: 2.31 min Scan# 380

Delta R.T. -0.03 min

Lab File: VU033268.D

Acq: 16 Jul 2019 17:25

Instrument :

MSVOA_U

ClientSampled :


A52M8

Tot Ion: 43 Resp: 3007

Ion Ratio Lower Upper




43 100

58 26.8 0.0 66.6

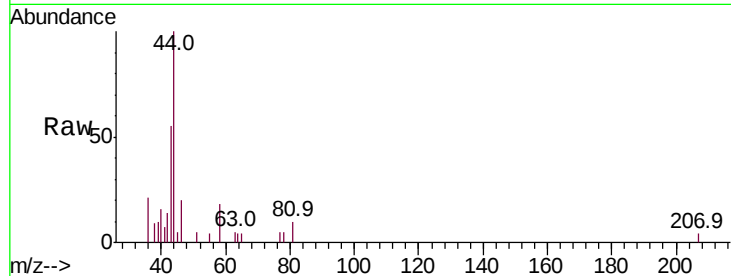

Abundance Ion 43.05 (42.75 to 43.75): VU0

Ion 58.05 (57.75 to 58.75): VU0

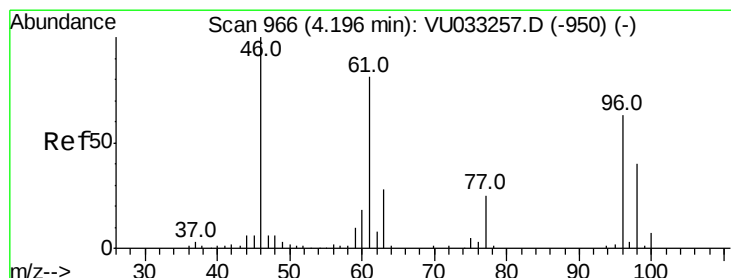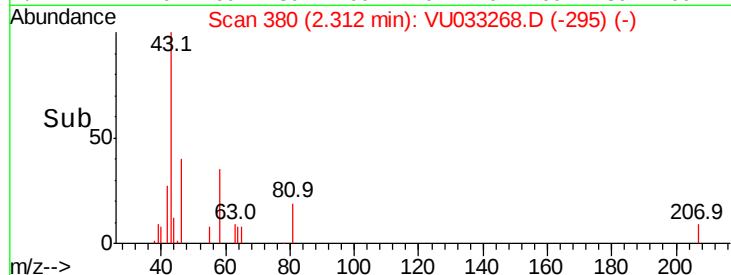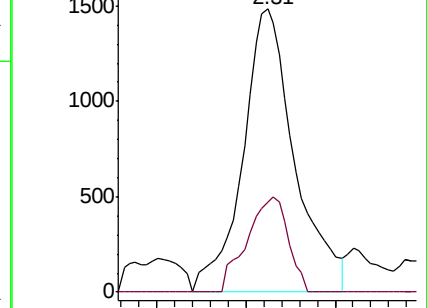

#22

cis-1,2-Dichloroethene

Concen: 16.411 ug/L

RT: 4.20 min Scan# 966

Delta R.T. -0.00 min

Lab File: VU033268.D

Acq: 16 Jul 2019 17:25


Tgt Ion: 96 Resp: 163742

Ion Ratio Lower Upper

96 100

61 132.7 89.2 165.6



68 0.0 0.0 0.0

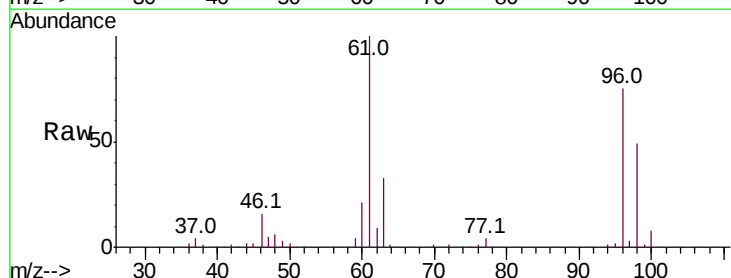


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 61.05 (60.75 to 61.75): VU0

Ion 68.15 (67.85 to 68.85): VU0

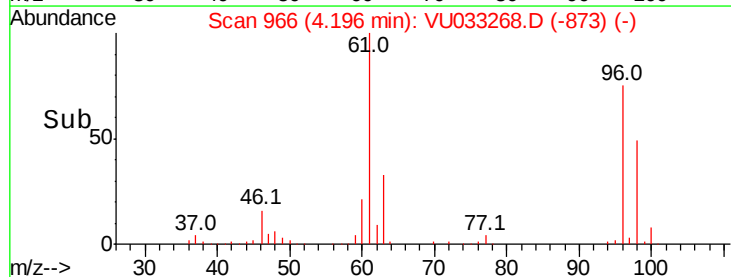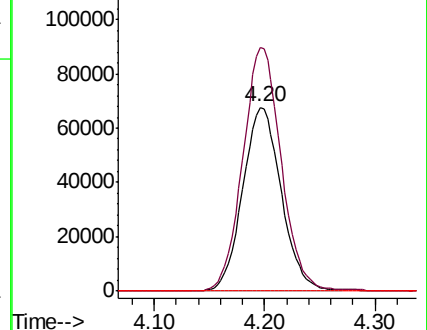


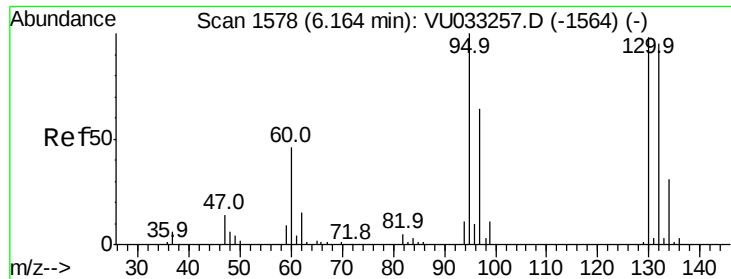




#34
 Trichloroethene
 Concen: 2.970 ug/L
 RT: 6.16 min Scan# 1578
 Delta R.T. -0.00 min
 Lab File: VU033268.D
 Acq: 16 Jul 2019 17:25

Instrument :
 MSVOA_U
 ClientSampleId :
 A52M8

Tot Ion:	95	Resp:	29900
Ion	Ratio	Lower	Upper
95	100		
97	67.5	44.5	82.7
132	95.1	66.6	123.8
130	97.2	68.9	127.9

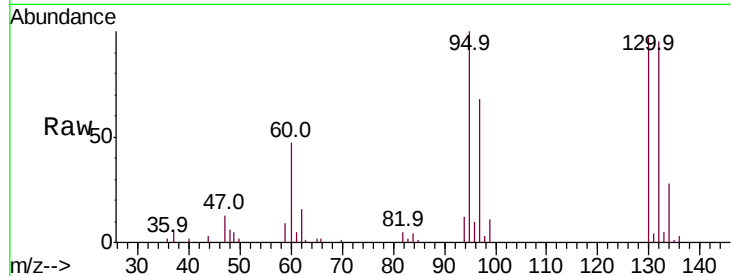


Abundance Ion 95.00 (94.70 to 95.70): VU0
 Ion 96.95 (96.65 to 97.65): VU0
 Ion 131.95 (131.65 to 132.65): V
 Ion 129.95 (129.65 to 130.65): V

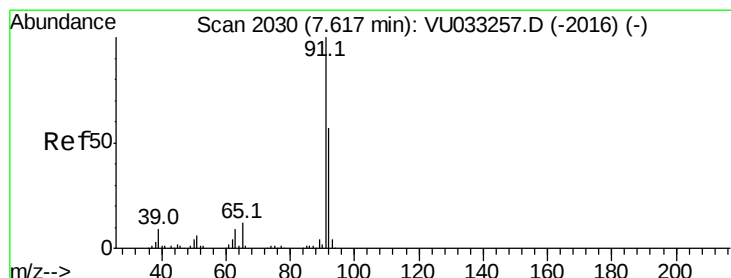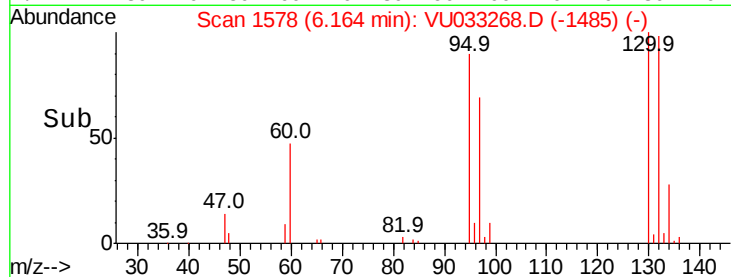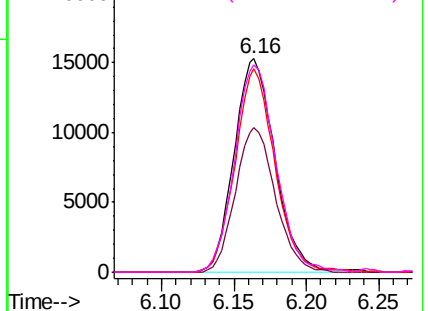

#42
 Toluene
 Concen: 0.171 ug/L
 RT: 7.62 min Scan# 2032
 Delta R.T. 0.01 min
 Lab File: VU033268.D
 Acq: 16 Jul 2019 17:25

Tgt Ion:	91	Resp:	6984
Ion	Ratio	Lower	Upper
91	100		
92	54.6	40.0	74.2

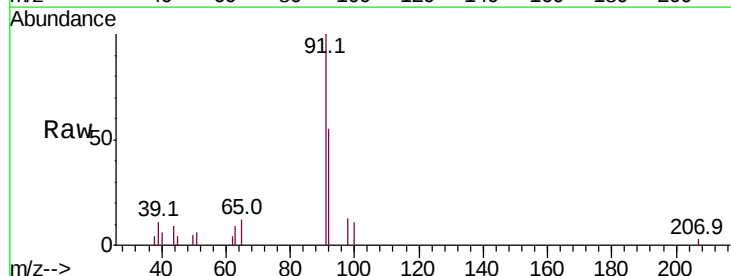

Abundance Ion 91.15 (90.85 to 91.85): VU0
 Ion 92.15 (91.85 to 92.85): VU0

