


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU071619\
 Data File : VU033254.D
 Acq On : 16 Jul 2019 08:25
 Operator : JC/SP
 Sample : BFB25
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB25

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR071619WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Jul 18 08:01:21 2019

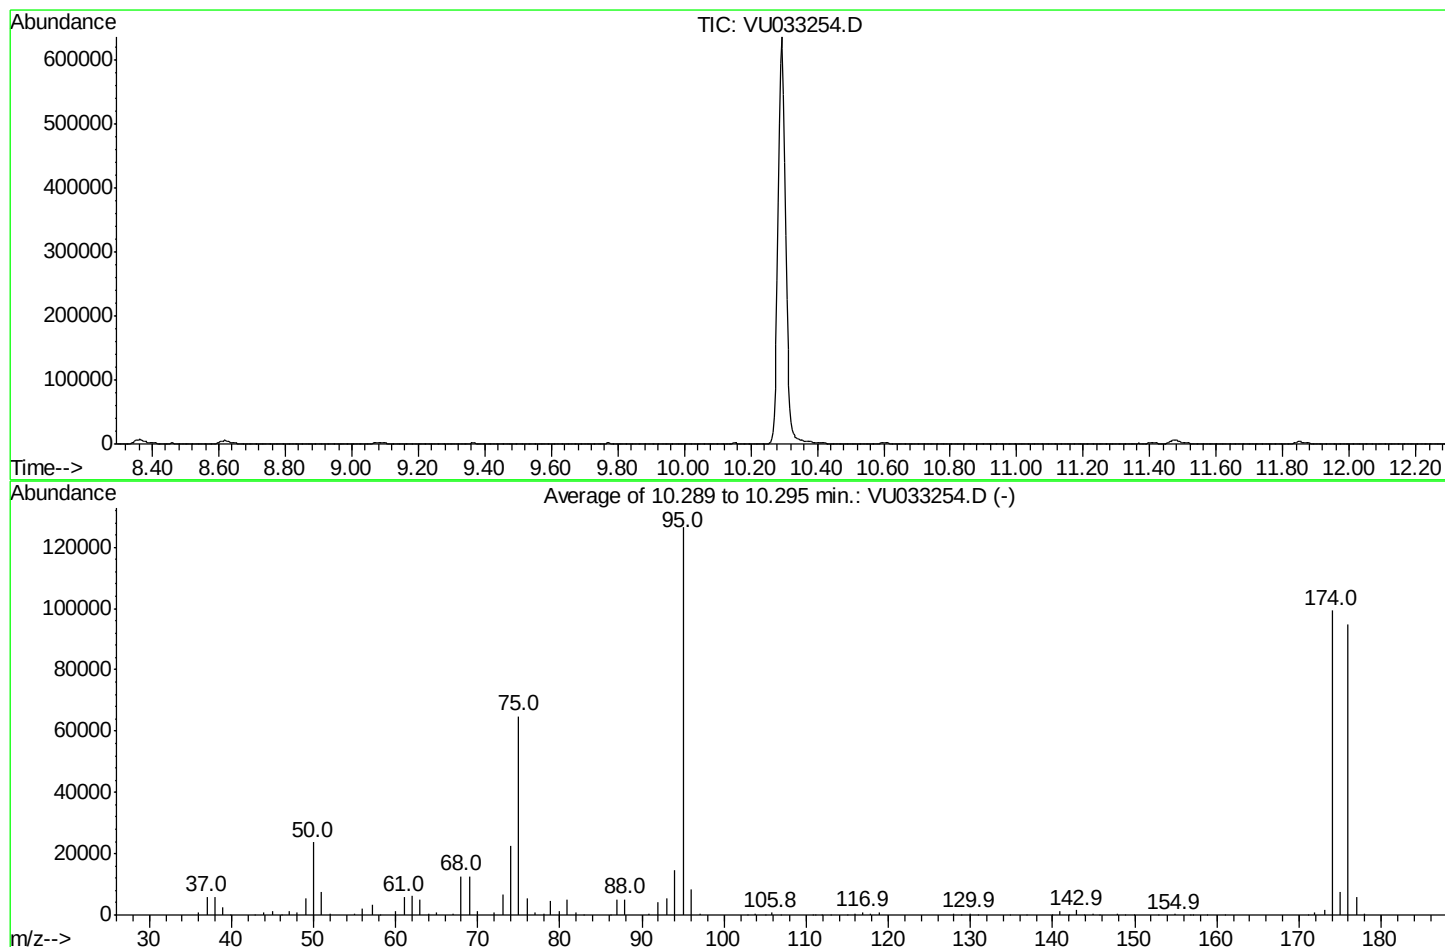

AutoFind: Scans 2861, 2862, 2863; Background Corrected with Scan 2848

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	23624	PASS
75	95	30	80	51.2	64794	PASS
95	95	100	100	100.0	126485	PASS
96	95	5	9	6.7	8487	PASS
173	174	0.00	2	1.9	1875	PASS
174	95	50	120	78.4	99213	PASS
175	174	5	9	7.7	7651	PASS
176	174	95	101	95.7	94906	PASS
177	176	5	9	6.4	6068	PASS

Scan 2848 (10.247 min): VU033254.D
BFB25

m/z	Abundance
39.80	251.0
44.10	378.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
36.00	1011.0
37.00	5777.0
38.00	5704.0
39.00	2374.0
39.90	328.0
43.90	1290.0
45.00	1138.0
46.20	159.0
47.10	1238.0
48.00	847.0
49.00	5619.0
50.00	23008.0
51.00	7352.0
51.90	392.0
55.00	562.0
56.00	1941.0
57.10	3319.0
58.10	106.0
60.00	1101.0
61.00	5747.0
62.00	6314.0
63.00	5039.0
64.00	601.0
65.00	718.0
67.00	438.0
68.00	12100.0
69.00	13086.0
70.00	1048.0
72.00	744.0
73.00	6471.0
74.00	22080.0
75.00	62592.0
76.00	5526.0
76.90	719.0
78.10	519.0
78.90	4491.0
80.00	1187.0
80.90	4792.0
81.90	892.0
82.90	129.0
86.10	224.0
86.90	4697.0
88.00	4961.0
90.80	432.0
92.00	3859.0
93.00	5382.0
94.00	14163.0
95.00	122760.0
96.00	8297.0
97.10	212.0
103.80	573.0
105.00	189.0
105.80	604.0
106.90	116.0
111.10	118.0
114.90	185.0
115.90	496.0
116.90	890.0
117.80	452.0
118.90	750.0
127.90	445.0
128.80	169.0
129.90	475.0
130.80	163.0
134.80	249.0
136.70	210.0
140.00	118.0
140.90	1354.0
141.90	199.0
143.00	1676.0
143.80	108.0
144.90	366.0
145.80	216.0
147.90	317.0
150.00	106.0
154.90	320.0
156.80	150.0
158.80	152.0
160.90	176.0
171.20	221.0
172.00	954.0
173.10	1839.0
174.00	93240.0
175.00	7168.0
176.00	90040.0
177.00	5764.0
178.00	232.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
36.00	1022.0
37.00	6276.0
38.00	6012.0
39.00	2395.0
39.90	360.0
43.90	1313.0
45.00	1235.0
46.10	104.0
47.00	1170.0
48.00	839.0
49.00	5634.0
50.00	24360.0
51.00	7676.0
51.90	392.0
55.00	548.0
56.00	2028.0
57.10	3419.0
60.00	1205.0
61.00	6066.0
62.00	6683.0
63.00	5414.0
64.10	644.0
65.00	757.0
67.10	426.0
68.00	12925.0
69.00	13108.0
70.00	1206.0
72.00	776.0
73.00	6745.0
74.00	23496.0
75.00	66928.0
76.10	5744.0
77.00	682.0
78.10	495.0
78.90	4855.0
80.00	1281.0
80.90	5176.0
81.90	982.0
82.90	142.0
86.10	142.0
86.90	5001.0
87.90	5387.0
90.80	474.0
92.00	4146.0
93.00	5707.0
94.00	14889.0
95.00	130968.0
96.00	8790.0
97.00	281.0
103.90	598.0
105.00	198.0
105.80	683.0
106.90	124.0
111.10	110.0
114.90	159.0
115.90	499.0
116.90	966.0
117.90	522.0
118.90	804.0
127.90	439.0
128.80	201.0
129.90	508.0
130.80	128.0
134.80	233.0
136.80	209.0
140.00	129.0
140.90	1389.0
142.00	217.0
142.90	1688.0
143.80	128.0
144.80	366.0
145.70	214.0
148.00	370.0
148.80	116.0
149.90	127.0
152.80	114.0
154.90	365.0
156.80	121.0
158.80	160.0
161.00	210.0
171.20	212.0
172.00	998.0
173.10	1941.0
174.00	102280.0
175.00	7909.0
176.00	97952.0
177.00	6209.0
178.00	246.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
36.00	957.0
37.00	6058.0
38.00	5523.0
39.00	2274.0
39.90	351.0
42.90	101.0
44.00	1199.0
45.00	1153.0
46.90	1086.0
48.00	735.0
49.00	5105.0
50.00	23504.0
51.00	7366.0
52.00	394.0
55.00	437.0
56.00	1924.0
57.10	3351.0
60.00	1125.0
61.00	5834.0
62.00	6340.0
63.00	5081.0
64.10	607.0
65.00	680.0
67.10	392.0
68.00	12636.0
69.00	12014.0
70.00	1159.0
72.00	737.0
73.00	6273.0
74.00	22600.0
75.00	64864.0
76.10	5511.0
77.00	697.0
78.00	451.0
78.90	4747.0
80.00	1322.0
80.90	5154.0
81.90	984.0
82.90	129.0
86.90	4944.0
87.90	5069.0
90.80	478.0
92.00	4014.0
93.00	5401.0
94.00	14386.0
95.00	125728.0
96.00	8376.0
97.00	341.0
102.90	102.0
103.90	591.0
104.90	198.0
105.80	687.0
106.90	118.0
110.80	126.0
111.90	107.0
112.90	124.0
115.00	129.0
115.90	464.0
116.90	870.0
117.90	505.0
118.90	767.0
127.90	437.0
128.90	274.0
130.00	507.0
130.90	116.0
134.90	186.0
136.80	205.0
140.90	1327.0
141.90	157.0
142.90	1631.0
143.90	112.0
144.80	353.0
145.70	182.0
148.00	372.0
148.80	117.0
149.80	133.0
154.90	364.0
157.10	142.0
158.90	159.0
160.90	205.0
171.10	171.0
171.90	915.0
173.10	1845.0
174.00	102120.0
175.00	7878.0
176.00	96728.0
177.00	6232.0
177.90	264.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25