

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071620\
 Data File : VU039532.D
 Acq On : 16 Jul 2020 18:23
 Operator : SY/MD
 Sample : L3292-15DL 20X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFT90DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.607	75	83	93	rVB	28765	32545	7.86%	0.979%
2	1.925	173	182	192	rBV	36563	48223	11.65%	1.450%
3	2.581	374	386	403	rBV2	60319	109072	26.35%	3.279%
4	3.067	526	537	549	rVB3	9009	17183	4.15%	0.517%
5	3.202	565	579	593	rBV2	5863	12639	3.05%	0.380%
6	4.658	1015	1032	1069	rBV2	63489	217204	52.48%	6.530%
7	5.086	1150	1165	1184	rBV3	58043	133068	32.15%	4.001%
8	5.742	1348	1369	1385	rBV2	114699	303474	73.32%	9.124%
9	6.266	1516	1532	1557	rBV	122570	230364	55.66%	6.926%
10	6.555	1610	1622	1637	rVB2	51428	94541	22.84%	2.842%
11	6.706	1656	1669	1686	rBV2	77864	148309	35.83%	4.459%
12	7.575	1927	1939	1956	rBV2	38512	66929	16.17%	2.012%
13	7.909	2030	2043	2058	rBV	132710	229746	55.51%	6.908%
14	8.189	2119	2130	2143	rVB	24245	40594	9.81%	1.221%
15	8.558	2233	2245	2259	rBV	185455	314016	75.87%	9.441%
16	8.642	2259	2271	2300	rVV	218998	413877	100.00%	12.444%
17	9.420	2499	2513	2538	rBV	174567	295074	71.30%	8.872%
18	10.758	2917	2929	2941	rBV	65182	104099	25.15%	3.130%
19	11.809	3244	3256	3271	rBV	173835	283236	68.43%	8.516%
20	12.189	3363	3374	3391	rBV	144288	231812	56.01%	6.970%


Sum of corrected areas: 3326005

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU071620\
Data File : VU039532.D
Acq On : 16 Jul 2020 18:23
Operator : SY/MD
Sample : L3292-15DL 20X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFT90DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

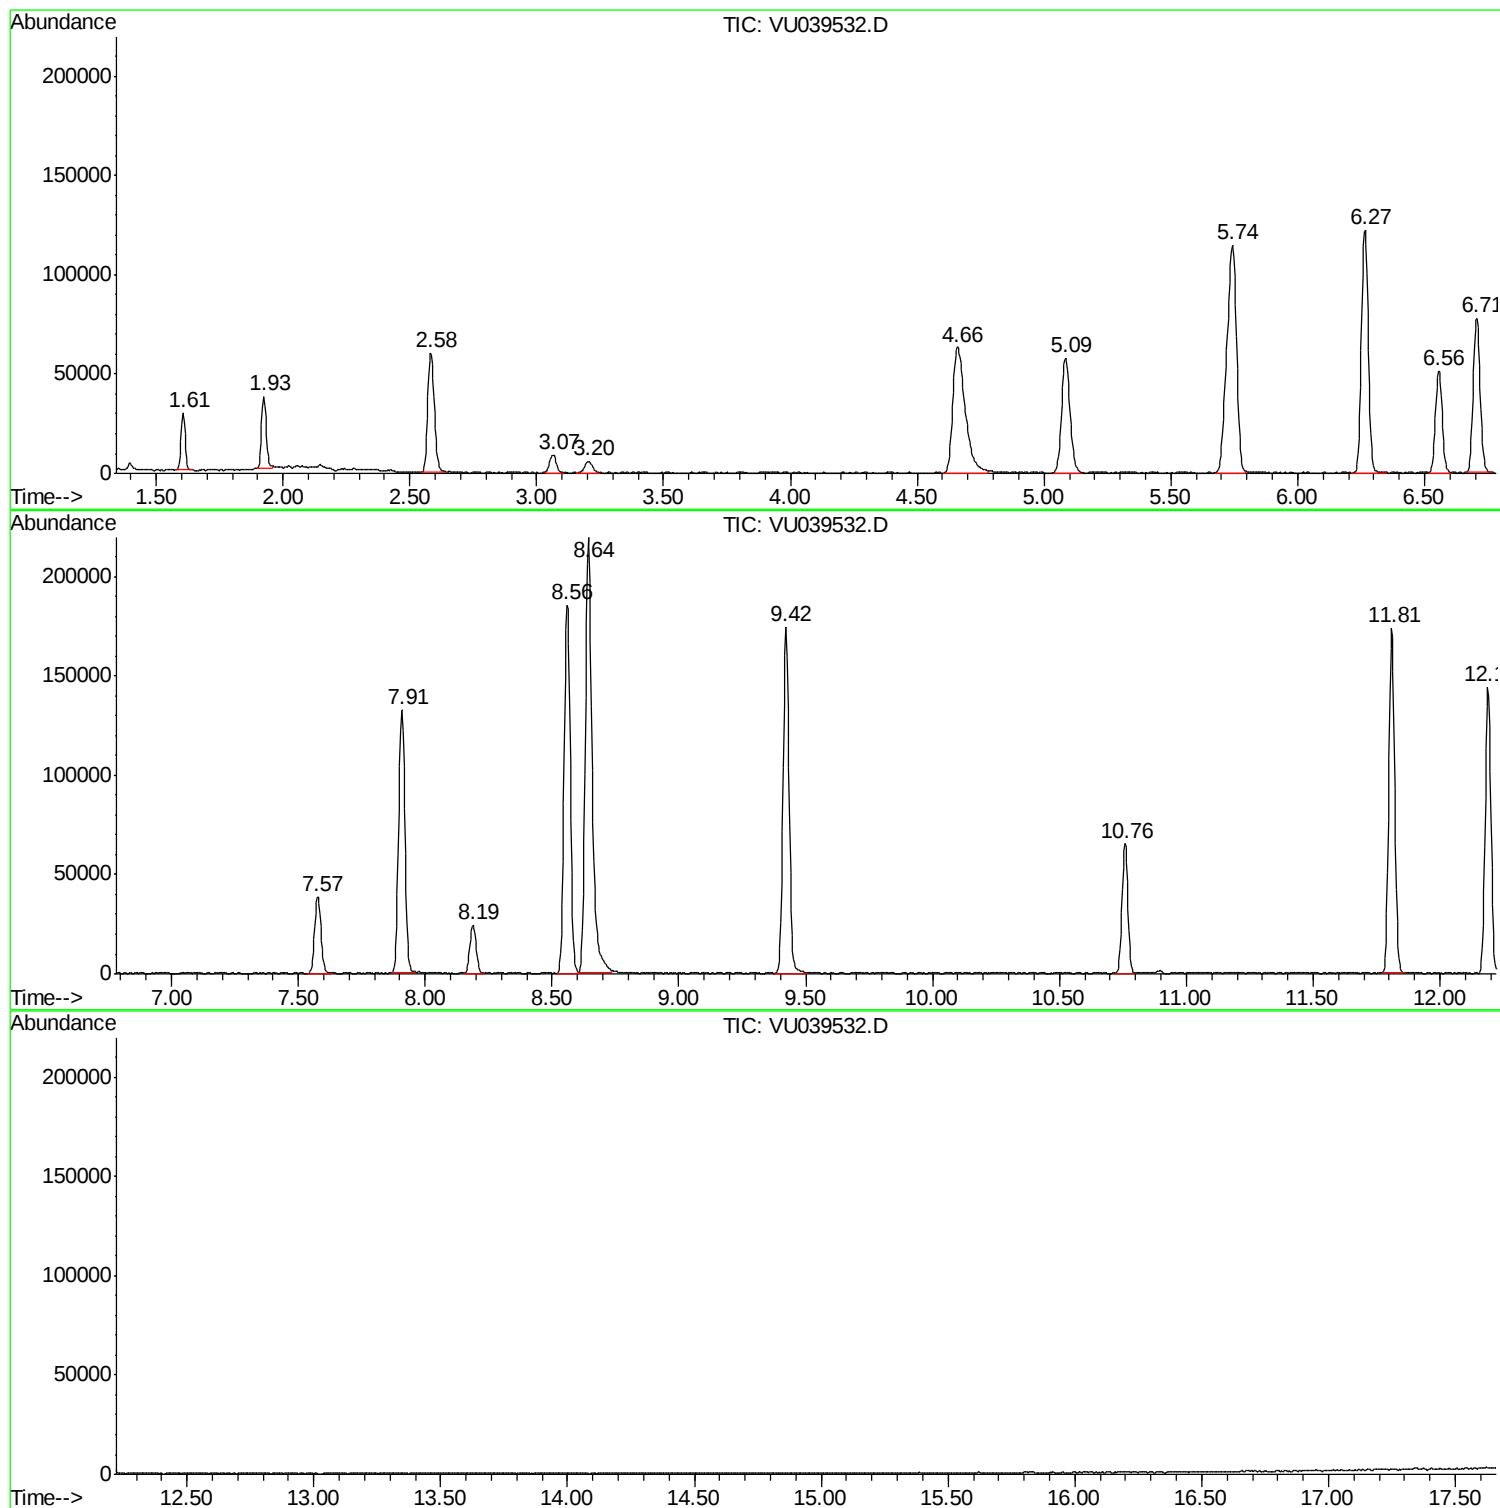

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071620\
Data File : VU039532.D
Acq On : 16 Jul 2020 18:23
Operator : SY/MD
Sample : L3292-15DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFT90DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU071620\
Data File : VU039532.D
Acq On : 16 Jul 2020 18:23
Operator : SY/MD
Sample : L3292-15DL 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFT90DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc