


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU071620\
 Data File : VU039512.D
 Acq On : 16 Jul 2020 08:44
 Operator : SY/MD
 Sample : BFB03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB03

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR070720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Jul 20 11:02:35 2020

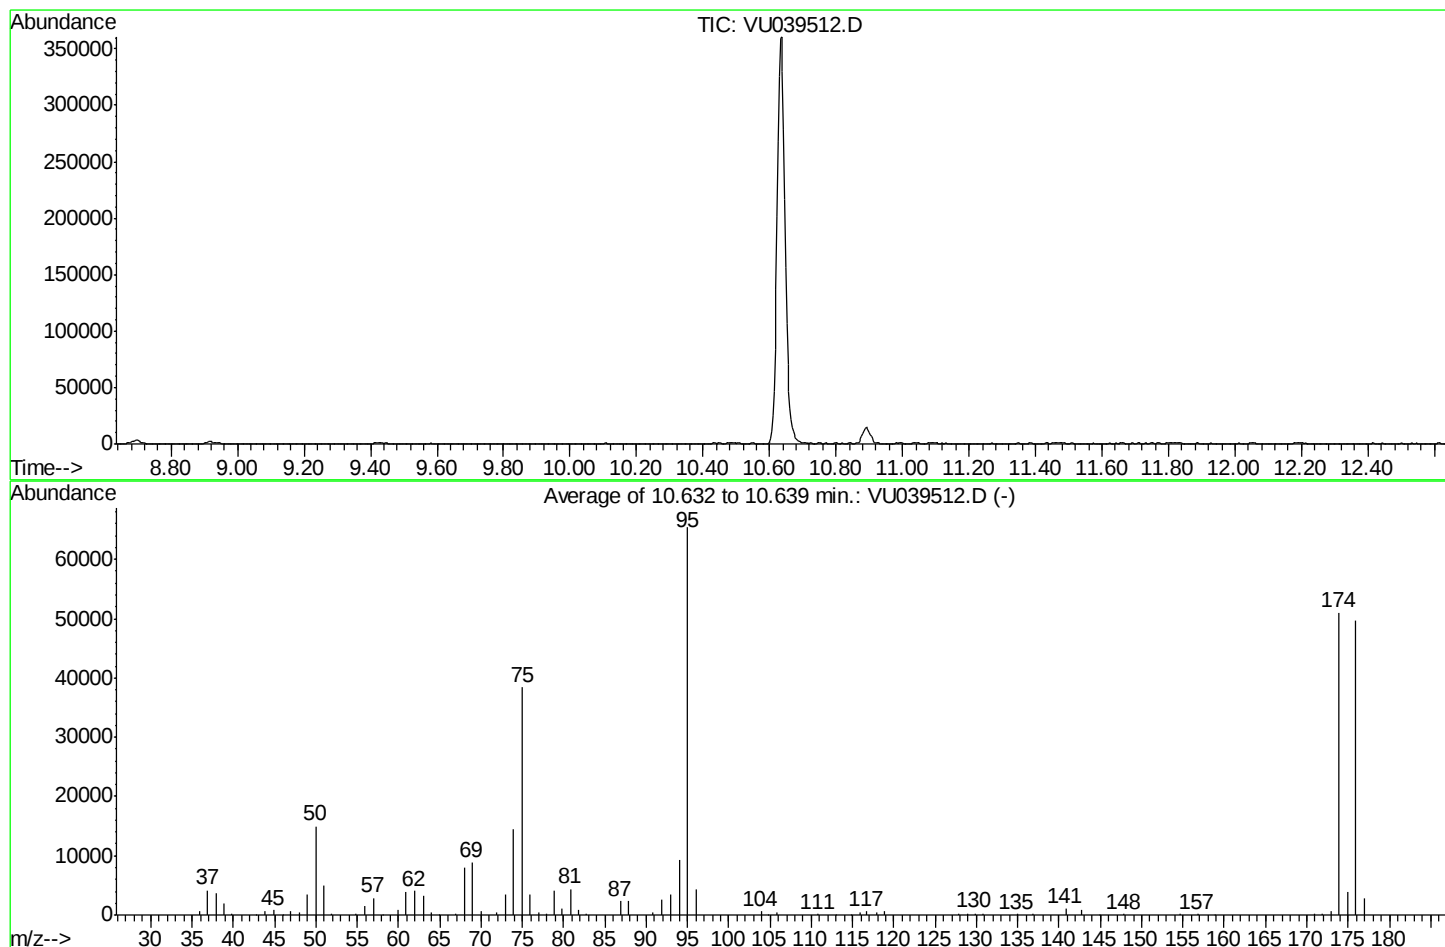

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	14988	PASS
75	95	30	80	58.7	38376	PASS
95	95	100	100	100.0	65416	PASS
96	95	5	9	6.7	4403	PASS
173	174	0.00	2	1.3	650	PASS
174	95	50	120	78.0	50994	PASS
175	174	5	9	7.7	3938	PASS
176	174	95	101	97.4	49669	PASS
177	176	5	9	5.7	2829	PASS

m/z	Abundance
35.90	811.0
36.90	4523.0
37.90	3790.0
38.90	1968.0
39.80	196.0
42.80	103.0
43.90	901.0
44.90	798.0
46.90	817.0
47.90	502.0
48.90	3683.0
50.00	15683.0
50.90	5219.0
51.90	224.0
54.90	356.0
55.90	1790.0
57.00	2876.0
58.00	155.0
60.00	796.0
60.90	4118.0
61.90	4037.0
63.00	3357.0
64.00	414.0
64.90	163.0
66.90	235.0
68.00	8389.0
68.90	9135.0
69.90	715.0
71.90	381.0
73.00	3854.0
73.90	14579.0
75.00	39736.0
75.90	3843.0
77.00	472.0
78.00	341.0
78.90	4156.0
79.80	1025.0
80.80	4381.0
81.80	891.0
82.70	219.0
86.90	2350.0
87.90	2437.0
90.80	467.0
91.90	2780.0
93.00	3688.0
94.00	9606.0
95.00	67328.0
96.00	4781.0
103.90	614.0
104.70	107.0
105.80	434.0
110.80	159.0
112.90	107.0
114.70	120.0
115.90	374.0
116.70	571.0
117.90	342.0
118.80	607.0
127.80	264.0
128.80	146.0
129.80	312.0
130.80	126.0
134.90	197.0
136.90	248.0
140.80	1090.0
142.80	944.0
144.90	128.0
147.90	187.0
154.70	127.0
156.80	212.0
170.90	123.0
171.80	310.0
173.00	569.0
173.90	50992.0
174.90	4037.0
175.90	49992.0
176.90	2995.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

m/z	Abundance
35.90	852.0
36.90	4234.0
37.90	3683.0
38.90	1960.0
39.80	186.0
42.80	122.0
43.90	933.0
44.90	820.0
46.00	121.0
46.80	779.0
47.90	582.0
48.90	3629.0
50.00	15419.0
51.00	5103.0
51.90	219.0
54.90	310.0
55.90	1646.0
57.00	2943.0
58.10	116.0
60.00	826.0
60.90	4017.0
61.90	4112.0
63.00	3275.0
64.10	409.0
64.90	141.0
66.90	201.0
67.90	8247.0
68.90	9006.0
70.00	676.0
71.90	396.0
73.00	3504.0
73.90	14908.0
75.00	39464.0
75.90	3688.0
77.00	416.0
77.90	306.0
78.90	4211.0
79.80	1040.0
80.90	4559.0
81.80	913.0
82.70	189.0
86.90	2406.0
87.90	2431.0
90.80	542.0
92.00	2756.0
92.90	3451.0
94.00	9484.0
95.00	67472.0
96.00	4551.0
104.00	656.0
105.80	374.0
110.80	190.0
112.90	118.0
114.80	108.0
115.90	366.0
116.80	639.0
117.90	362.0
118.80	608.0
127.80	277.0
128.80	124.0
129.80	290.0
130.80	189.0
134.90	214.0
136.90	210.0
140.80	1101.0
142.70	902.0
144.80	103.0
147.80	173.0
154.70	124.0
156.70	185.0
158.90	108.0
171.00	129.0
171.80	313.0
172.90	661.0
173.90	52488.0
174.90	4092.0
175.90	51336.0
176.90	2844.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

m/z	Abundance
35.90	763.0
36.90	3814.0
37.90	3469.0
38.90	1657.0
39.90	148.0
42.80	100.0
43.90	917.0
44.90	840.0
45.90	107.0
46.80	644.0
48.00	478.0
48.90	3159.0
50.00	13863.0
51.00	4462.0
51.90	198.0
54.90	256.0
56.00	1338.0
56.90	2630.0
59.90	706.0
60.90	3601.0
61.90	3869.0
63.00	3008.0
64.10	367.0
66.90	176.0
67.90	7590.0
68.90	8233.0
69.90	625.0
71.90	397.0
73.00	3032.0
73.90	13800.0
75.00	35928.0
75.90	3153.0
76.90	377.0
77.90	260.0
78.90	3952.0
79.80	1023.0
80.90	4225.0
81.80	878.0
82.70	136.0
86.90	2371.0
87.90	2229.0
90.80	522.0
91.90	2420.0
92.90	3141.0
94.00	8515.0
95.00	61448.0
96.00	3878.0
104.00	567.0
105.80	390.0
110.80	193.0
112.90	100.0
115.90	339.0
116.80	610.0
117.80	329.0
118.80	517.0
127.90	249.0
128.90	130.0
129.90	245.0
130.80	185.0
134.90	214.0
136.90	134.0
140.80	1037.0
142.70	781.0
147.80	193.0
154.70	121.0
156.80	134.0
158.90	118.0
171.10	113.0
171.80	283.0
172.90	721.0
173.90	49504.0
174.90	3687.0
175.90	47680.0
176.90	2650.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

Scan 2877 (10.591 min): VU039512.D
BFB03

m/z	Abundance
35.80	134.0
43.90	315.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03