

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071621\
 Data File : VU044351.D
 Acq On : 16 Jul 2021 13:45
 Operator : SY/MD
 Sample : IBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 IBLK

Quant Time: Jul 16 14:32:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Jul 16 14:21:52 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.121	96	52650	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.639	95	19969	0.941	ug/l	0.00
Spiked Amount	1.000		Recovery	=	94.000%	
68) 1,2-Dichlorobenzene-d4	12.201	152	20005	0.953	ug/l	0.00
Spiked Amount	1.000		Recovery	=	95.000%	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071621\
 Data File : VU044351.D
 Acq On : 16 Jul 2021 13:45
 Operator : SY/MD
 Sample : IBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 IBLK


Quant Time: Jul 16 14:32:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U071621DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Jul 16 14:21:52 2021
 Response via : Initial Calibration

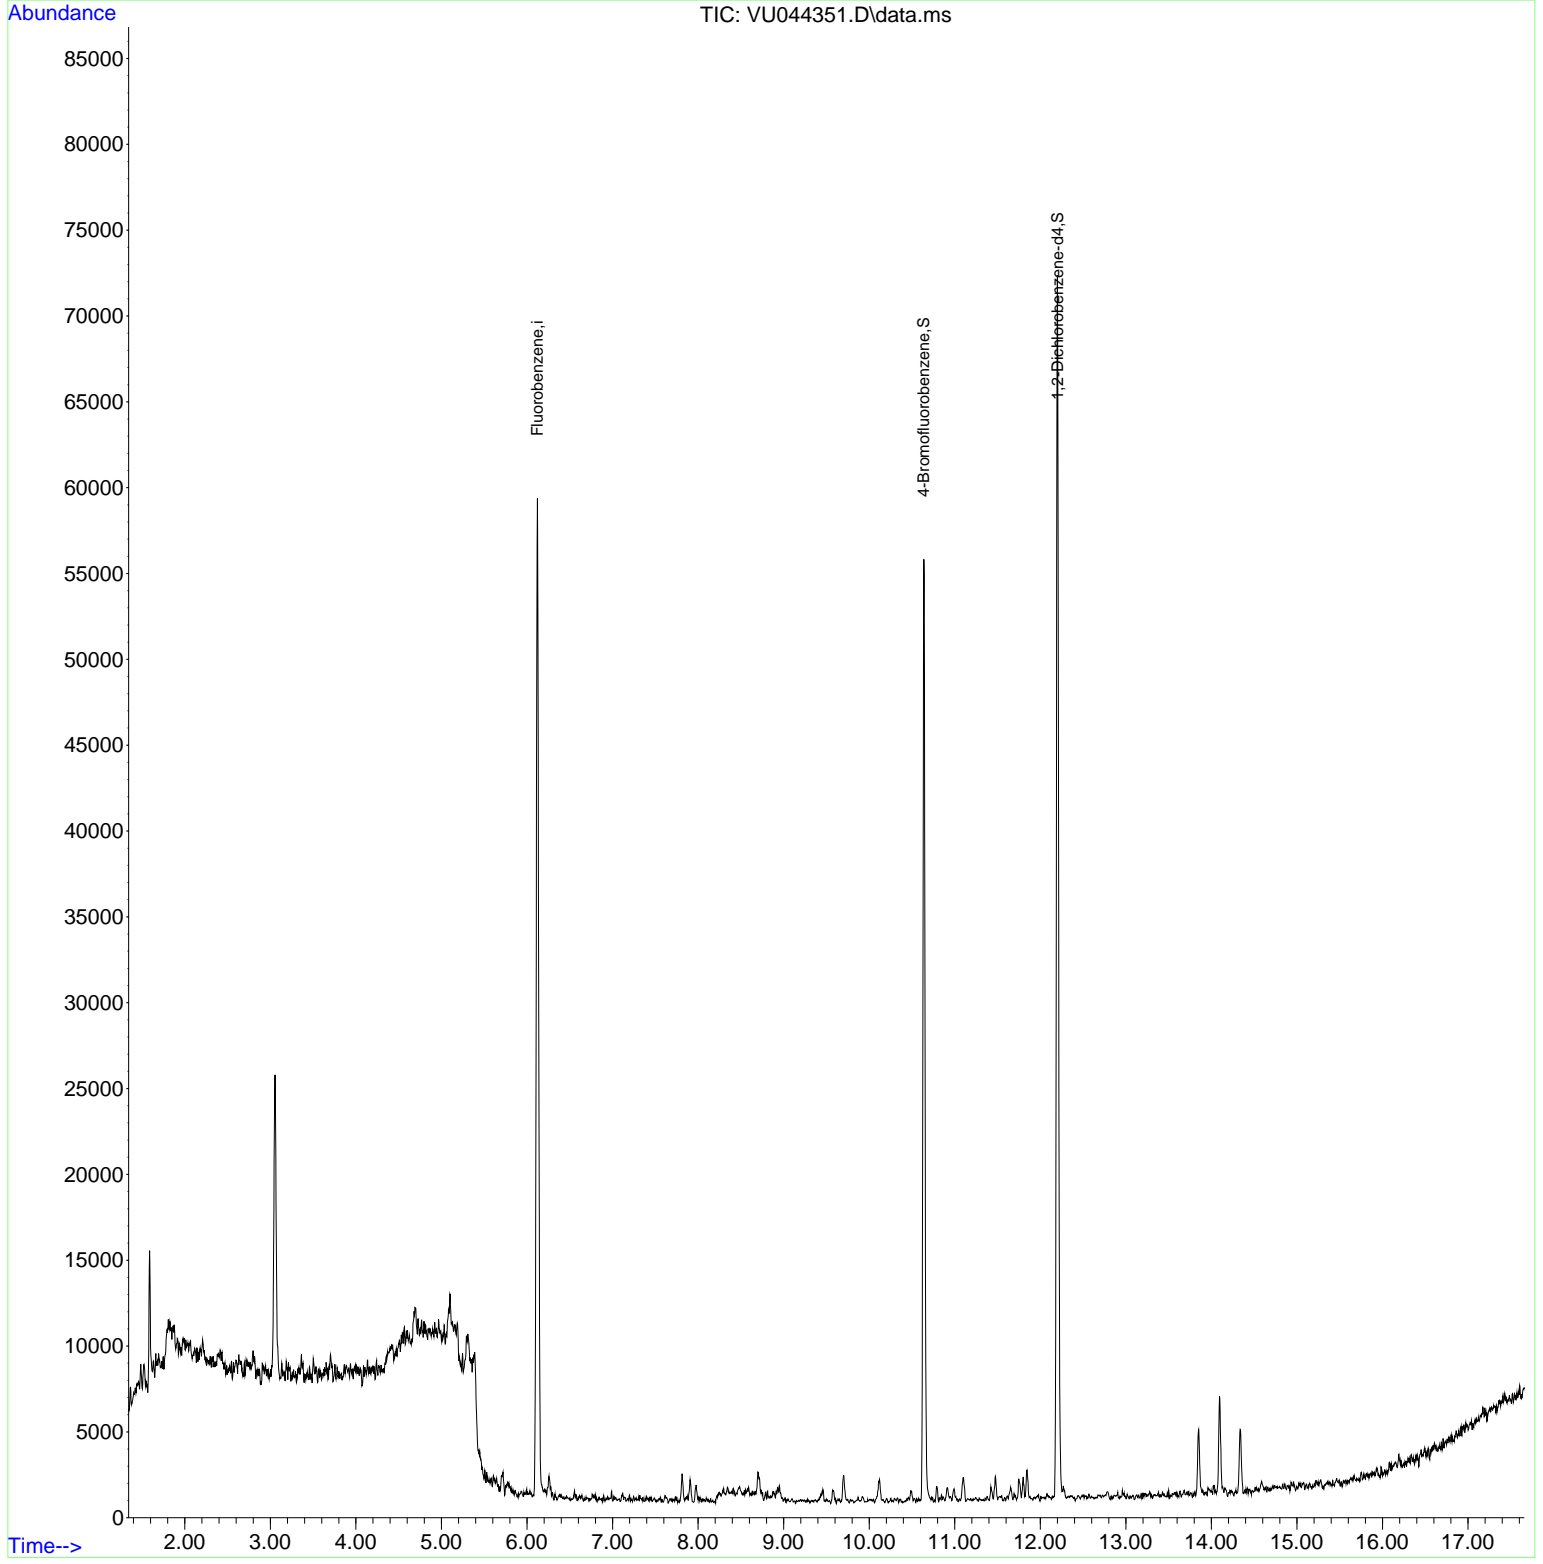

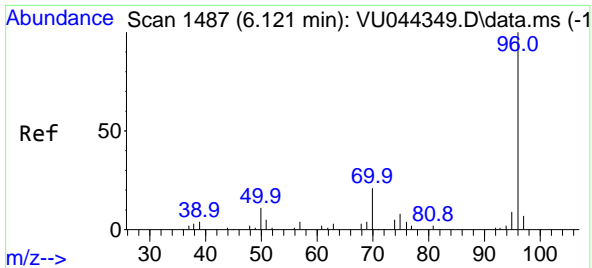




#1
 Fluorobenzene
 Concen: 1.000 ug/l
 RT: 6.121 min Scan# 1487
 Delta R.T. 0.000 min
 Lab File: VU044351.D
 Acq: 16 Jul 2021 13:45

Instrument : MSVOA_U
 ClientSampled : IBLK

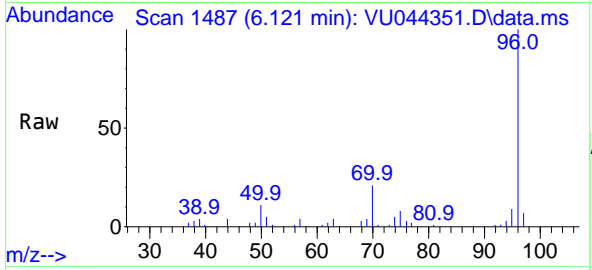


Tgt Ion: 96 Resp: 52650

Ion	Ratio	Lower	Upper
96	100		
70	20.7	16.2	24.2
95	9.2	7.3	10.9
97	6.7	0.0	0.0#

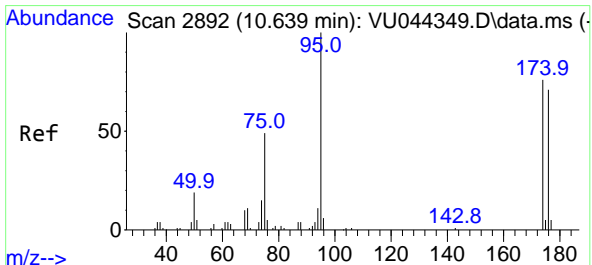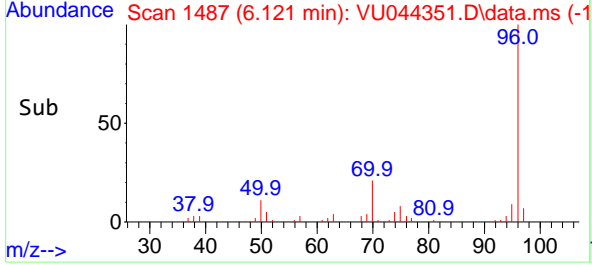
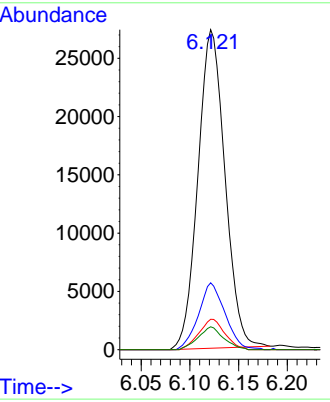



#57
 4-Bromofluorobenzene
 Concen: 0.941 ug/l
 RT: 10.639 min Scan# 2892
 Delta R.T. 0.000 min
 Lab File: VU044351.D
 Acq: 16 Jul 2021 13:45

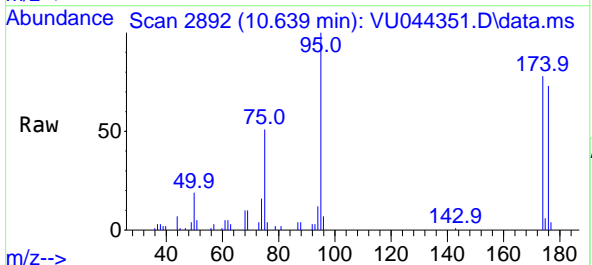

Tgt Ion: 95 Resp: 19969


Ion	Ratio	Lower	Upper
95	100		
174	78.6	62.2	93.2
176	74.8	60.3	90.5

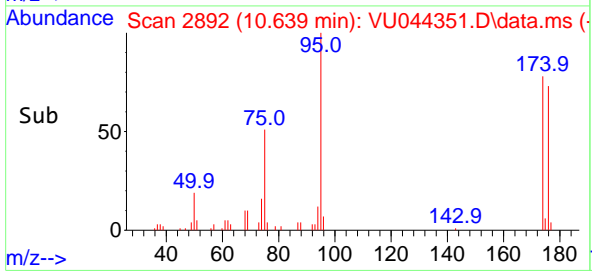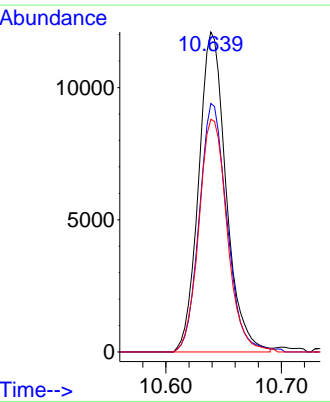

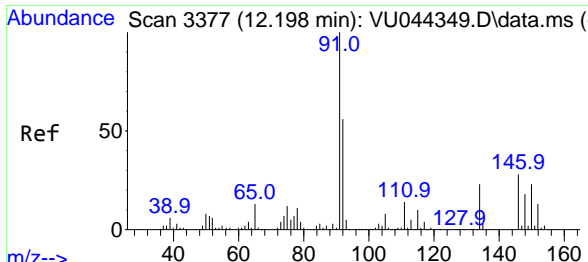

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.953 ug/l
 RT: 12.201 min Scan# 3378
 Delta R.T. 0.003 min
 Lab File: VU044351.D
 Acq: 16 Jul 2021 13:45

Instrument :
 MSVOA_U
 ClientSampled :
 IBLK

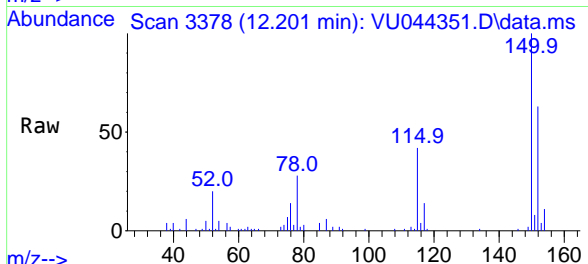

Tgt Ion:152 Resp: 20005
 Ion Ratio Lower Upper
 152 100
 115 64.7 0.0 257.0
 150 157.7 0.0 630.2

