

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071624\
 Data File : VU059966.D
 Acq On : 16 Jul 2024 11:51
 Operator : MD/SY
 Sample : P3217-23
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YDZN6

Quant Time: Jul 17 02:26:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 17 02:25:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	129274	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	139588	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	59168	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	41785	4.648	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.000%
7) Chloroethane-d5	1.907	69	36028	4.165	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.400%
11) 1,1-Dichloroethene-d2	2.560	65	15923	4.270	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	85.400%
20) 2-Butanone-d5	4.621	46	91890	49.627	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.260%
24) Chloroform-d	5.058	84	82089	4.449	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%
26) 1,2-Dichloroethane-d4	5.698	65	41748	4.697	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.000%
32) Benzene-d6	5.724	84	154534	4.023	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.400%
36) 1,2-Dichloropropane-d6	6.685	67	51516	4.376	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.600%
41) Toluene-d8	7.894	98	122082	3.418	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.400%#
43) trans-1,3-Dichloroprop...	8.181	79	16121	4.373	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.400%
46) 2-Hexanone-d5	8.631	63	67834	44.289	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.580%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	44928	4.619	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.400%
66) 1,2-Dichlorobenzene-d4	12.190	152	50470	4.793	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.800%
Target Compounds						
					Qvalue	
13) Acetone	2.628	43	17987	14.975	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU071624\
Data File : VU059966.D
Acq On : 16 Jul 2024 11:51
Operator : MD/SY
Sample : P3217-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YDZN6

Quant Time: Jul 17 02:26:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 17 02:25:31 2024
Response via : Initial Calibration

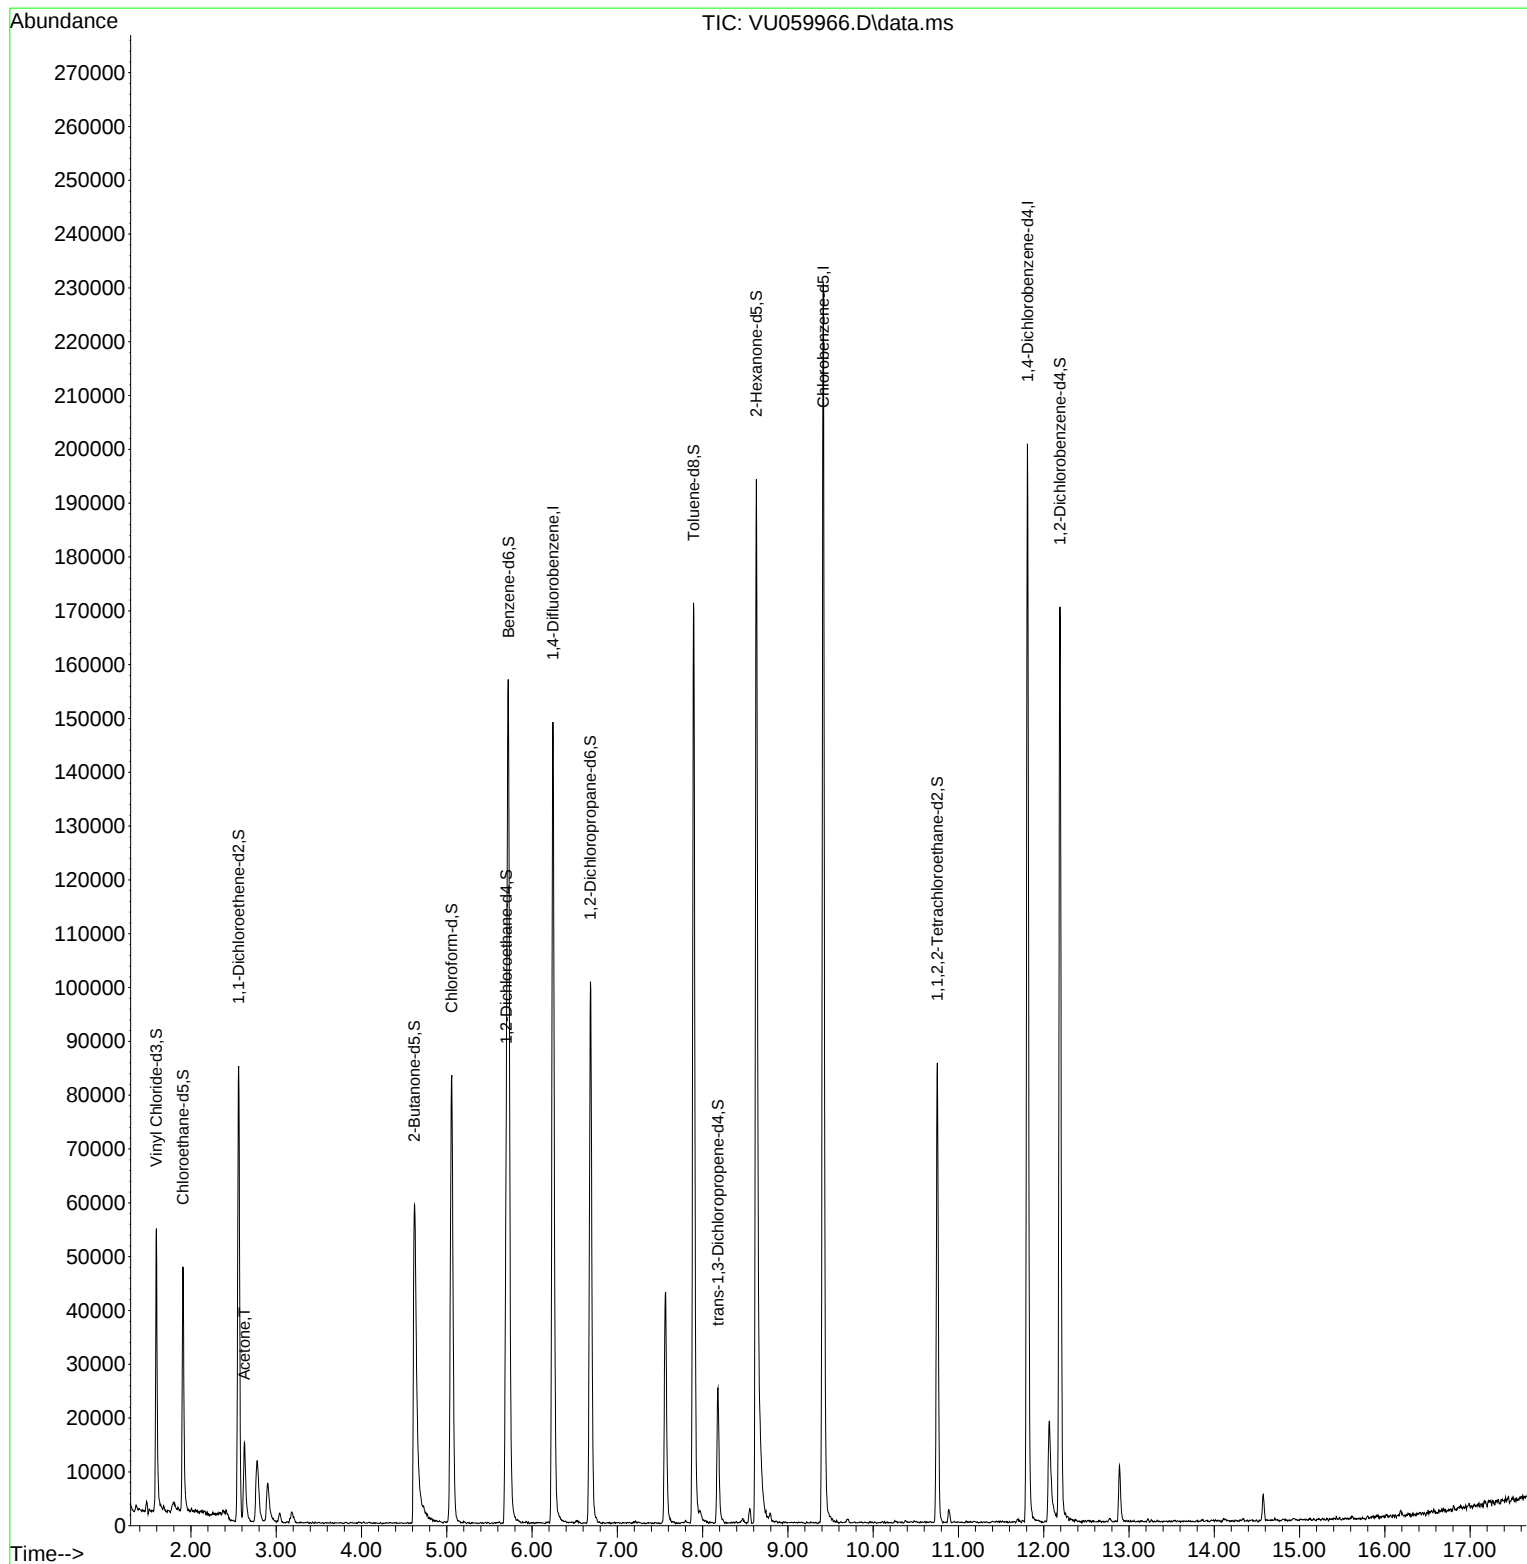

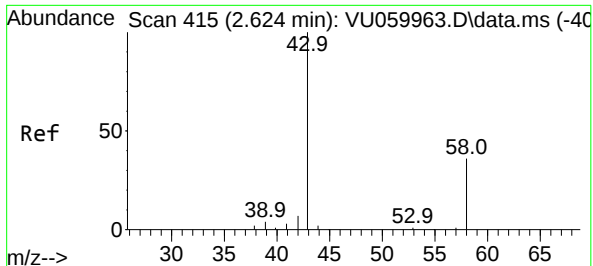

#13
 Acetone
 Concen: 14.975 ug/L
 RT: 2.628 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: VU059966.D
 Acq: 16 Jul 2024 11:51

Instrument :
 MSVOA_U
 ClientSampleId :
 YDZN6

Tgt Ion: 43 Resp: 17987
 Ion Ratio Lower Upper
 43 100
 58 38.0 0.0 68.0

